

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102720\
Data File : FG007248.D
Signal(s) : FID1A.ch
Acq On : 27 Oct 2020 09:34
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 15:43:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100220.M
Quant Title :
QLast Update : Mon Oct 05 13:04:52 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.792	91510	0.752 ug/ml
Target Compounds				
16)	N-HEXATRIACONTANE	20.217	81796	0.878 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102720\
Data File : FG007248.D
Signal(s) : FID1A.ch
Acq On : 27 Oct 2020 09:34
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 15:43:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100220.M
Quant Title :
QLast Update : Mon Oct 05 13:04:52 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

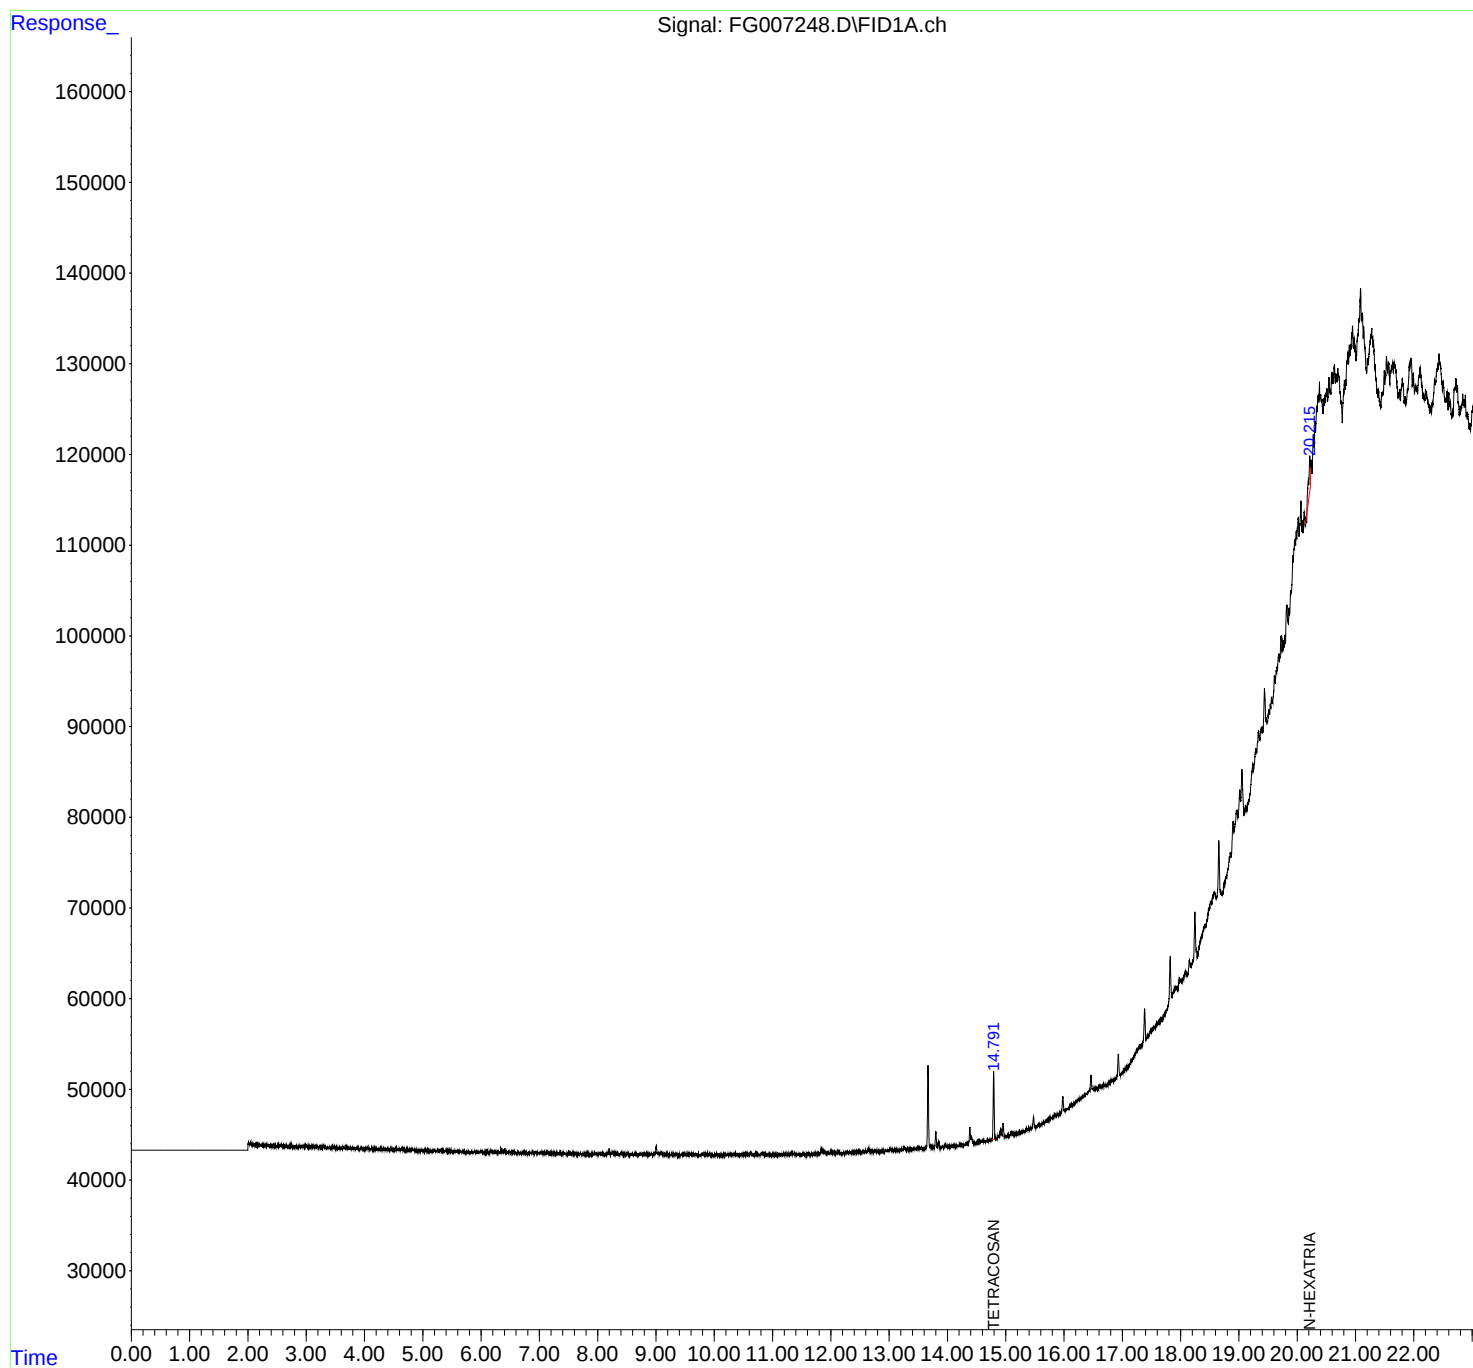


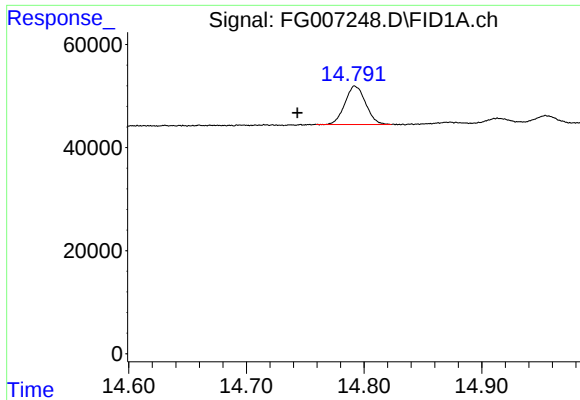

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.792 min
Delta R.T.: 0.049 min
Response: 91510
Conc: 0.75 ug/ml

Instrument :
FID_G
ClientSampleId :

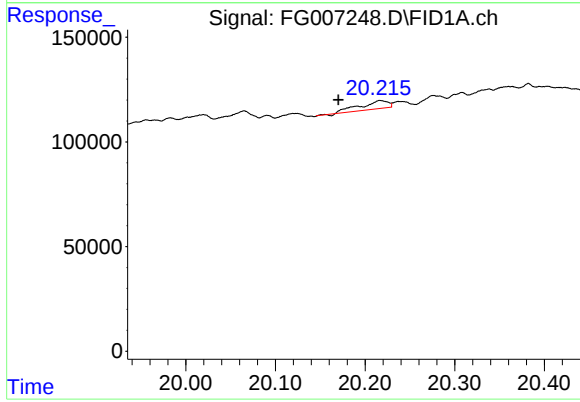

#16 N-HEXATRIACONTANE

R.T.: 20.217 min
Delta R.T.: 0.047 min
Response: 81796
Conc: 0.88 ug/ml