

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102720\
 Data File : FG007250.D
 Signal(s) : FID1A.ch
 Acq On : 27 Oct 2020 11:20
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Oct 27 15:43:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100220.M
 Quant Title :
 QLast Update : Mon Oct 05 13:04:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.754	6224529	51.120 ug/ml
Target Compounds			
2) N-DECANE	4.449	8070440	59.483 ug/ml
3) N-DODECANE	6.480	8058259	58.799 ug/ml
4) N-TETRADECANE	8.282	7926481	58.078 ug/ml
5) N-HEXADECANE	9.888	7959360	56.516 ug/ml
6) N-OCTADECANE	11.336	7835057	55.019 ug/ml
7) N-EICOSANE	12.650	7574685	53.547 ug/ml
8) N-DOCOSANE	13.853	7287059	52.204 ug/ml
10) N-TETRACOSANE	14.960	7102011	50.905 ug/ml
11) N-HEXACOSANE	15.984	6826801	49.832 ug/ml
12) N-OCTACOSANE	16.936	6645908	49.276 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102720\
Data File : FG007250.D
Signal(s) : FID1A.ch
Acq On : 27 Oct 2020 11:20
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Oct 27 15:43:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100220.M
Quant Title :
QLast Update : Mon Oct 05 13:04:52 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

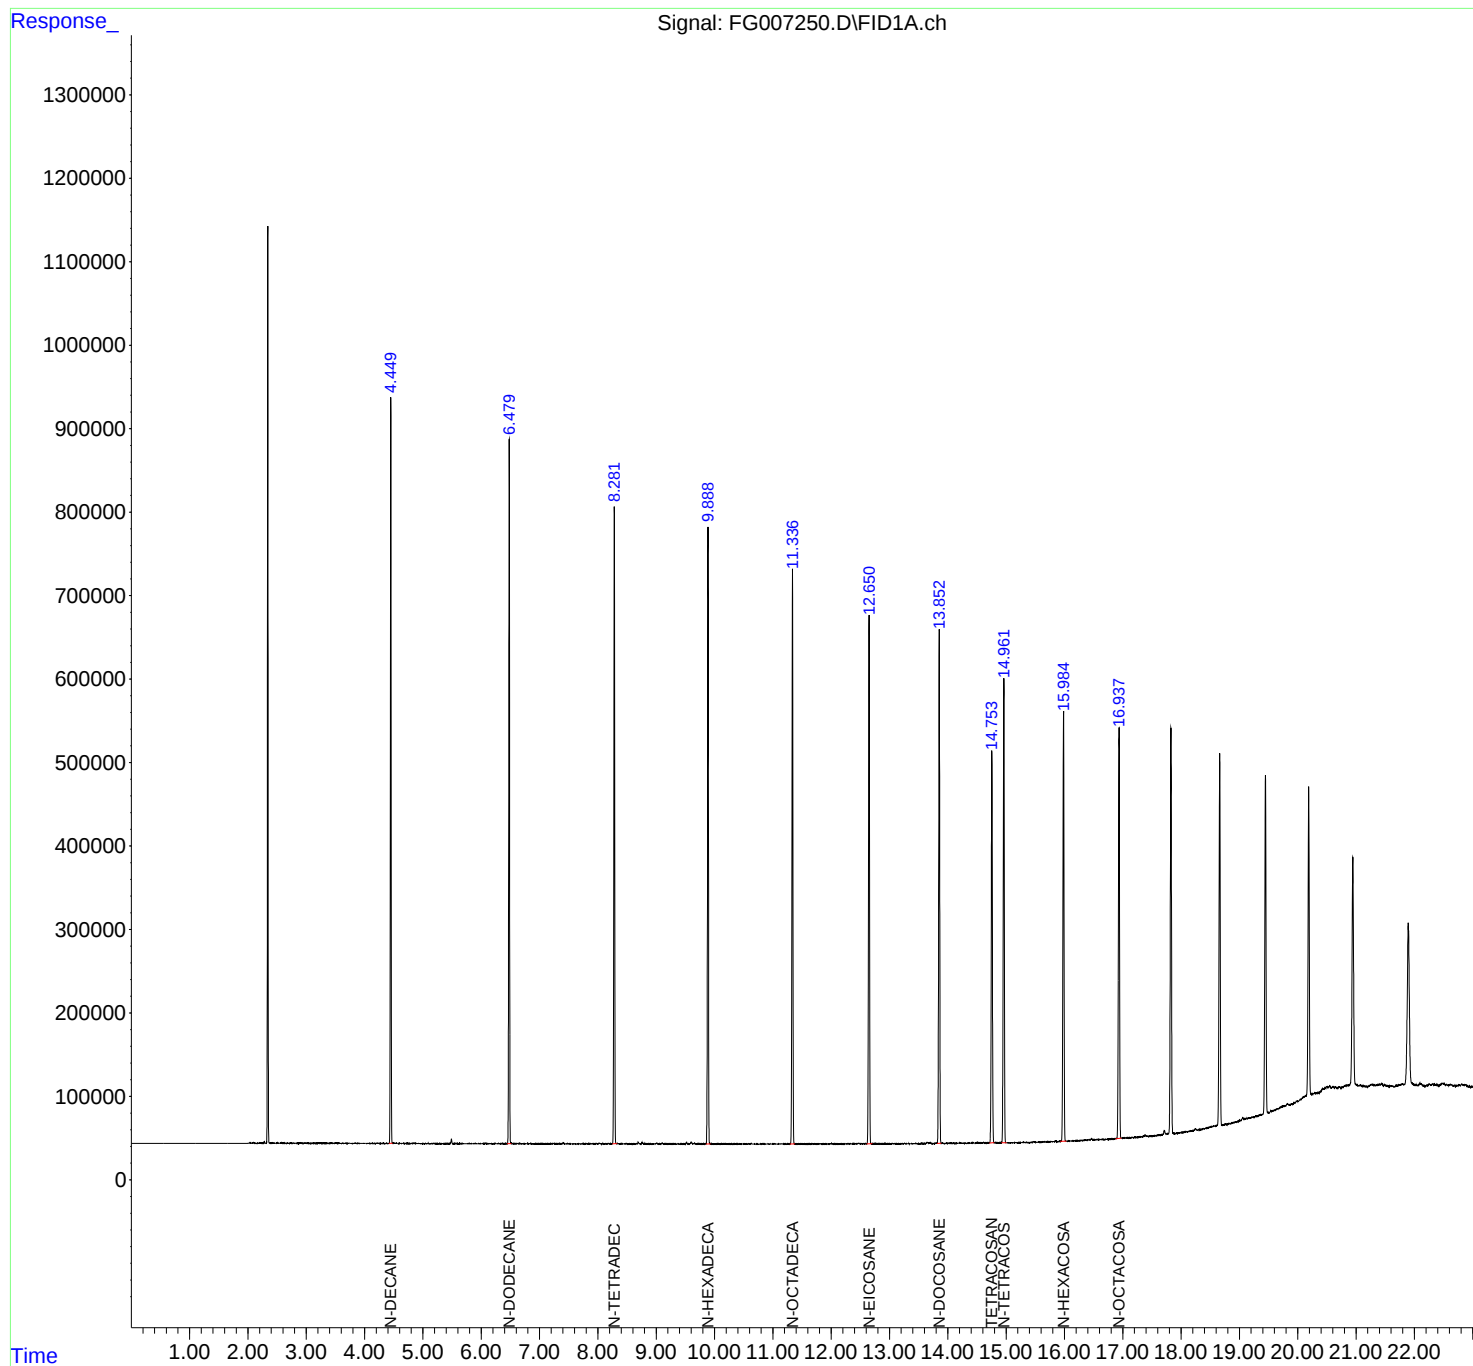


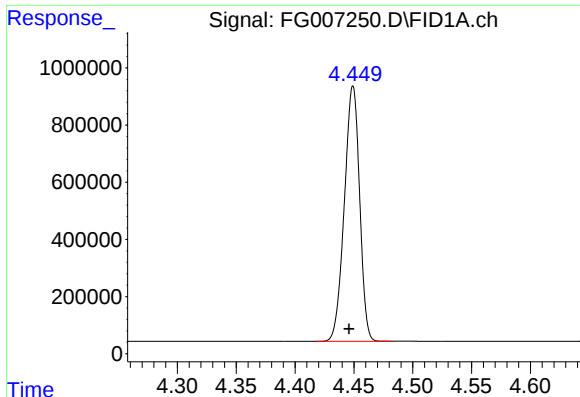

#2 N-DECANE


R.T.: 4.449 min
Delta R.T.: 0.003 min
Response: 8070440
Conc: 59.48 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

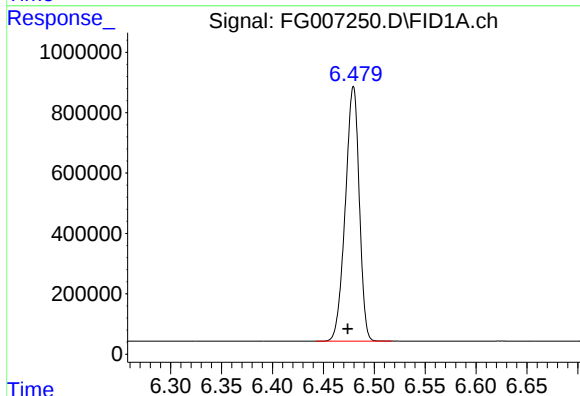


#3 N-DODECANE

R.T.: 6.480 min
Delta R.T.: 0.006 min
Response: 8058259
Conc: 58.80 ug/ml

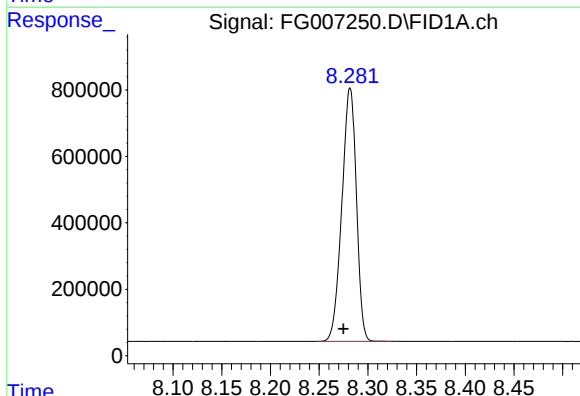


#4 N-TETRADECANE

R.T.: 8.282 min
Delta R.T.: 0.007 min
Response: 7926481
Conc: 58.08 ug/ml

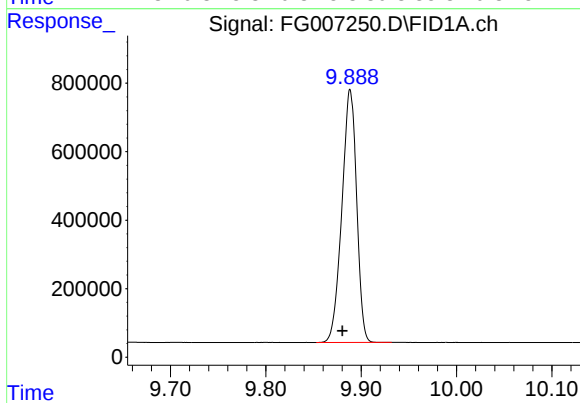

#5 N-HEXADECANE


R.T.: 9.888 min
Delta R.T.: 0.008 min
Response: 7959360
Conc: 56.52 ug/ml

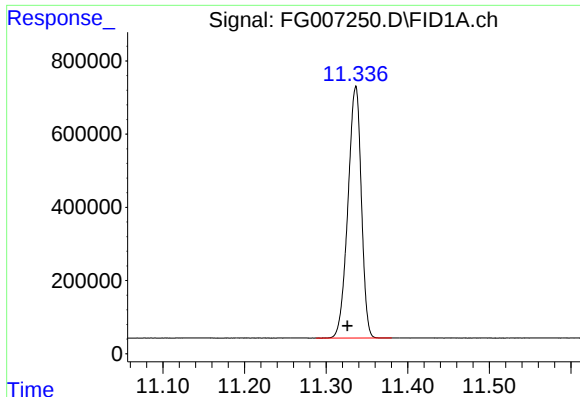

#6 N-OCTADECANE


R.T.: 11.336 min
Delta R.T.: 0.010 min
Response: 7835057
Conc: 55.02 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

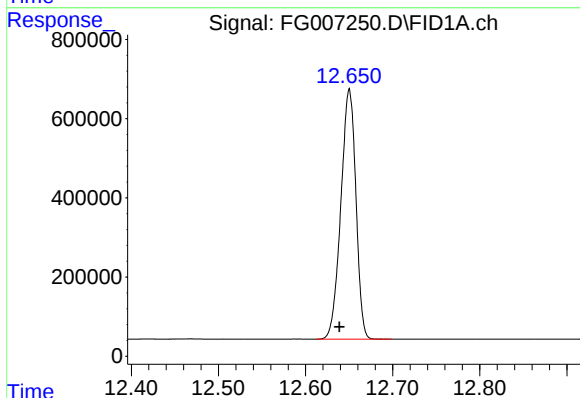


#7 N-EICOSANE

R.T.: 12.650 min
Delta R.T.: 0.011 min
Response: 7574685
Conc: 53.55 ug/ml

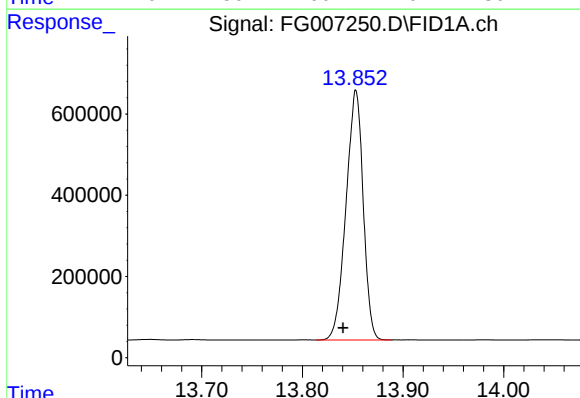


#8 N-DOCOSANE

R.T.: 13.853 min
Delta R.T.: 0.013 min
Response: 7287059
Conc: 52.20 ug/ml

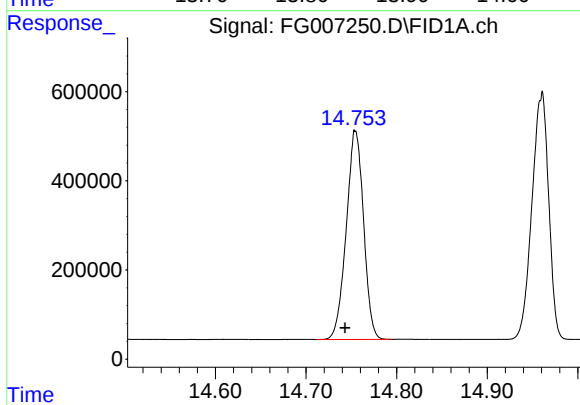

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.754 min
Delta R.T.: 0.011 min
Response: 6224529
Conc: 51.12 ug/ml

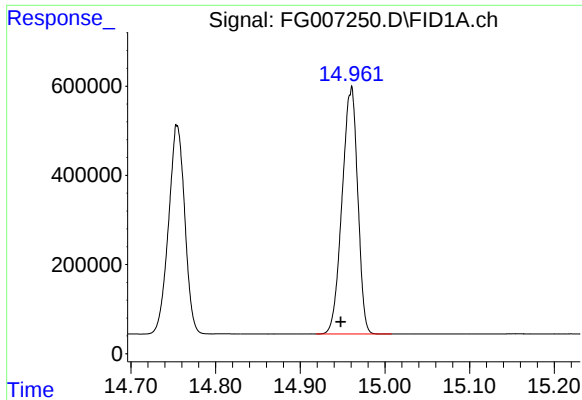

#10 N-TETRACOSANE


R.T.: 14.960 min
Delta R.T.: 0.013 min
Response: 7102011
Conc: 50.91 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

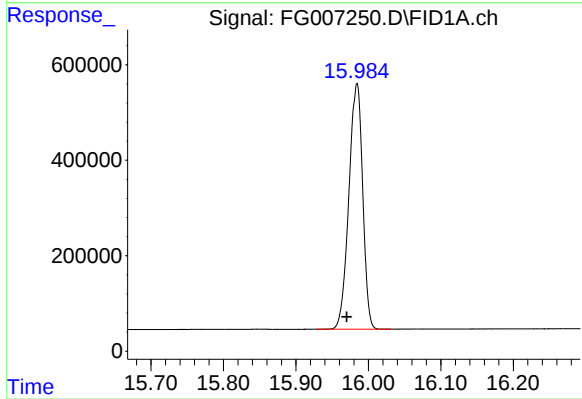

#11 N-HEXACOSANE

R.T.: 15.984 min
Delta R.T.: 0.014 min
Response: 6826801
Conc: 49.83 ug/ml

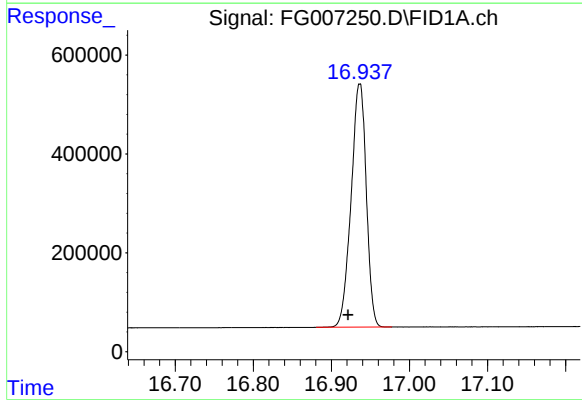

#12 N-OCTACOSANE

R.T.: 16.936 min
Delta R.T.: 0.015 min
Response: 6645908
Conc: 49.28 ug/ml