

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102920\
 Data File : FG007265.D
 Signal(s) : FID1A.ch
 Acq On : 29 Oct 2020 15:56
 Operator : DD\AJ
 Sample : L4531-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 30 03:09:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100220.M
 Quant Title :
 QLast Update : Mon Oct 05 13:04:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.743	1459333	11.985 ug/ml
Target Compounds			
4) N-TETRADECANE	8.334f	548368	4.018 ug/ml
7) N-EICOSANE	12.701f	86238	0.610 ug/ml
14) N-DOTRIACONTANE	18.644	126800	1.003 ug/ml
16) N-HEXATRIACONTANE	20.174	83715	0.898 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102920\
Data File : FG007265.D
Signal(s) : FID1A.ch
Acq On : 29 Oct 2020 15:56
Operator : DD\AJ
Sample : L4531-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 30 03:09:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100220.M
Quant Title :
QLast Update : Mon Oct 05 13:04:52 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

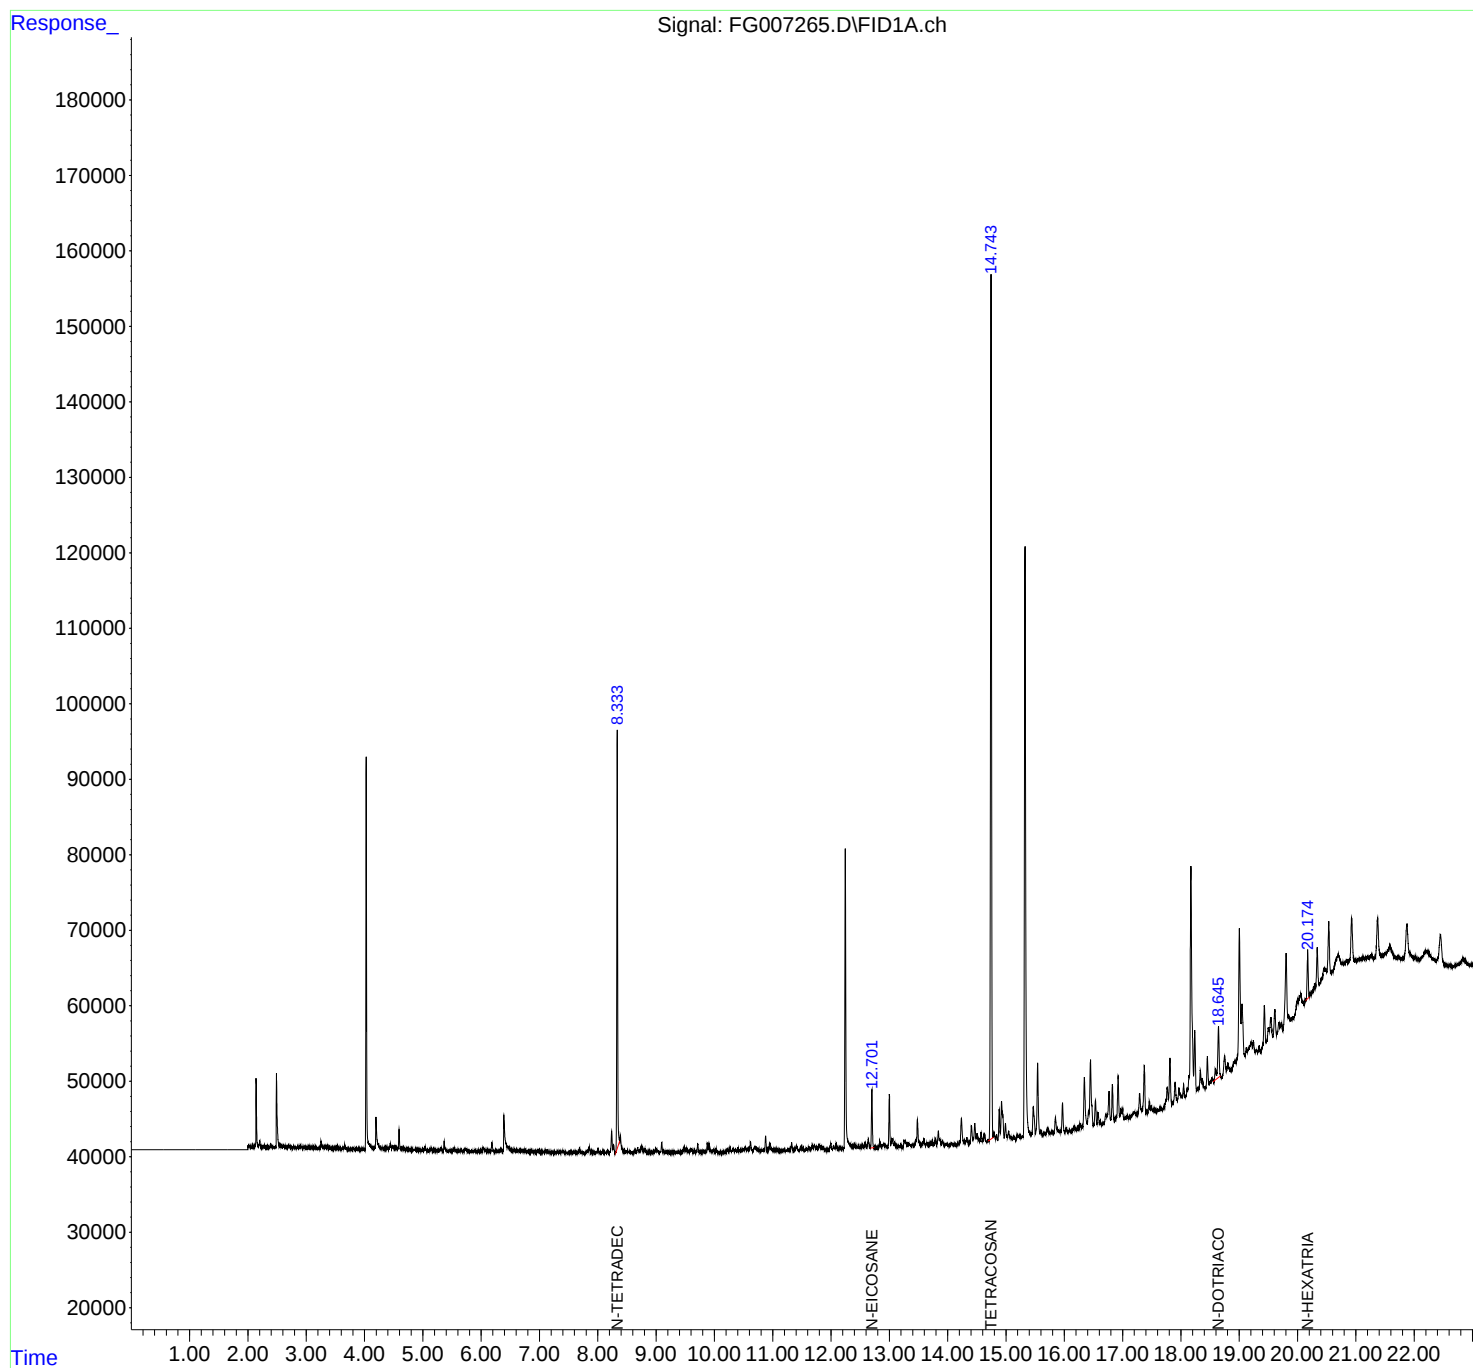


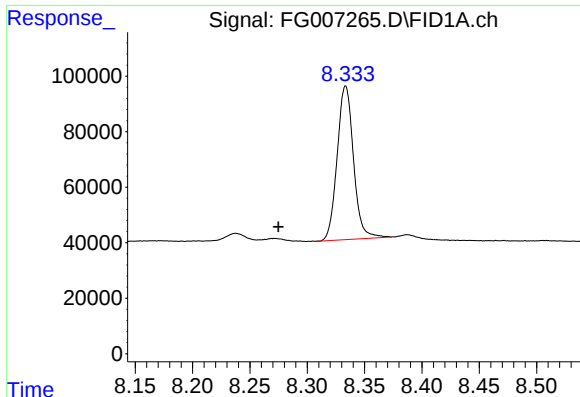

#4 N-TETRADECANE


R.T.: 8.334 min
Delta R.T.: 0.059 min
Response: 548368
Conc: 4.02 ug/ml

Instrument :
FID_G
ClientSampleId :

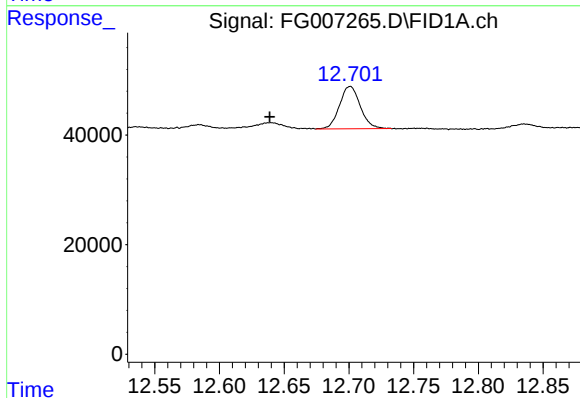


#7 N-EICOSANE

R.T.: 12.701 min
Delta R.T.: 0.062 min
Response: 86238
Conc: 0.61 ug/ml

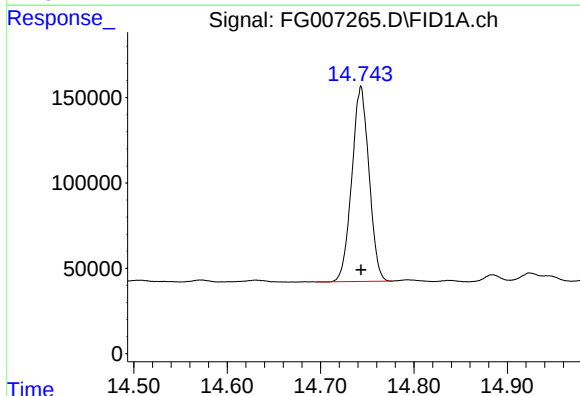


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.743 min
Delta R.T.: 0.000 min
Response: 1459333
Conc: 11.98 ug/ml

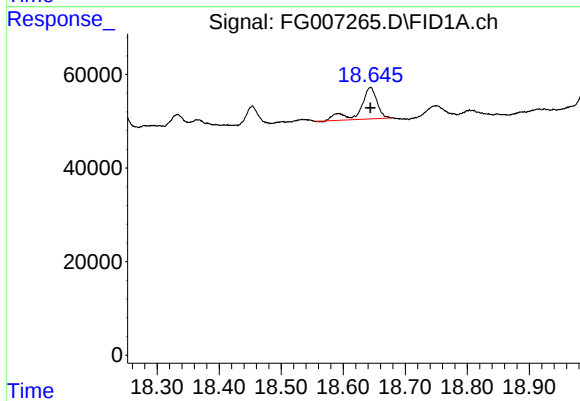

#14 N-DOTRIACONTANE

R.T.: 18.644 min
Delta R.T.: 0.000 min
Response: 126800
Conc: 1.00 ug/ml

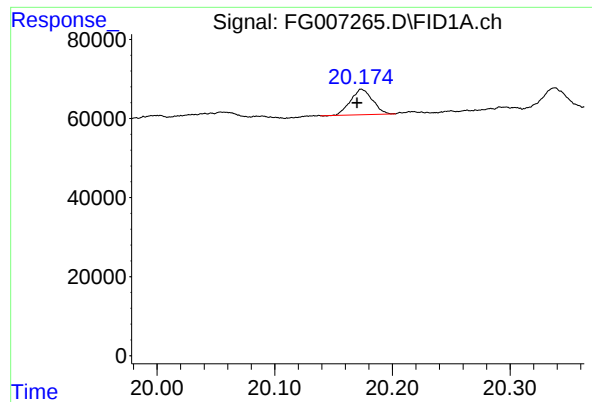

#16 N-HEXATRIACONTANE

R.T.: 20.174 min
Delta R.T.: 0.004 min
Response: 83715
Conc: 0.90 ug/ml

Instrument :
FID_G
ClientSampleId :