

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102920\
Data File : FG007264.D
Signal(s) : FID1A.ch
Acq On : 29 Oct 2020 15:25
Operator : DD\AJ
Sample : L4531-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-1916-GC-GRAB-A

Integration File: autoint1.e
Quant Time: Oct 30 03:09:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100220.M
Quant Title :
QLast Update : Mon Oct 05 13:04:52 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.744	2292453	18.827 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102920\
Data File : FG007264.D
Signal(s) : FID1A.ch
Acq On : 29 Oct 2020 15:25
Operator : DD\AJ
Sample : L4531-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
TP-1916-GC-GRAB-A

Integration File: autoint1.e
Quant Time: Oct 30 03:09:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG100220.M
Quant Title :
QLast Update : Mon Oct 05 13:04:52 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

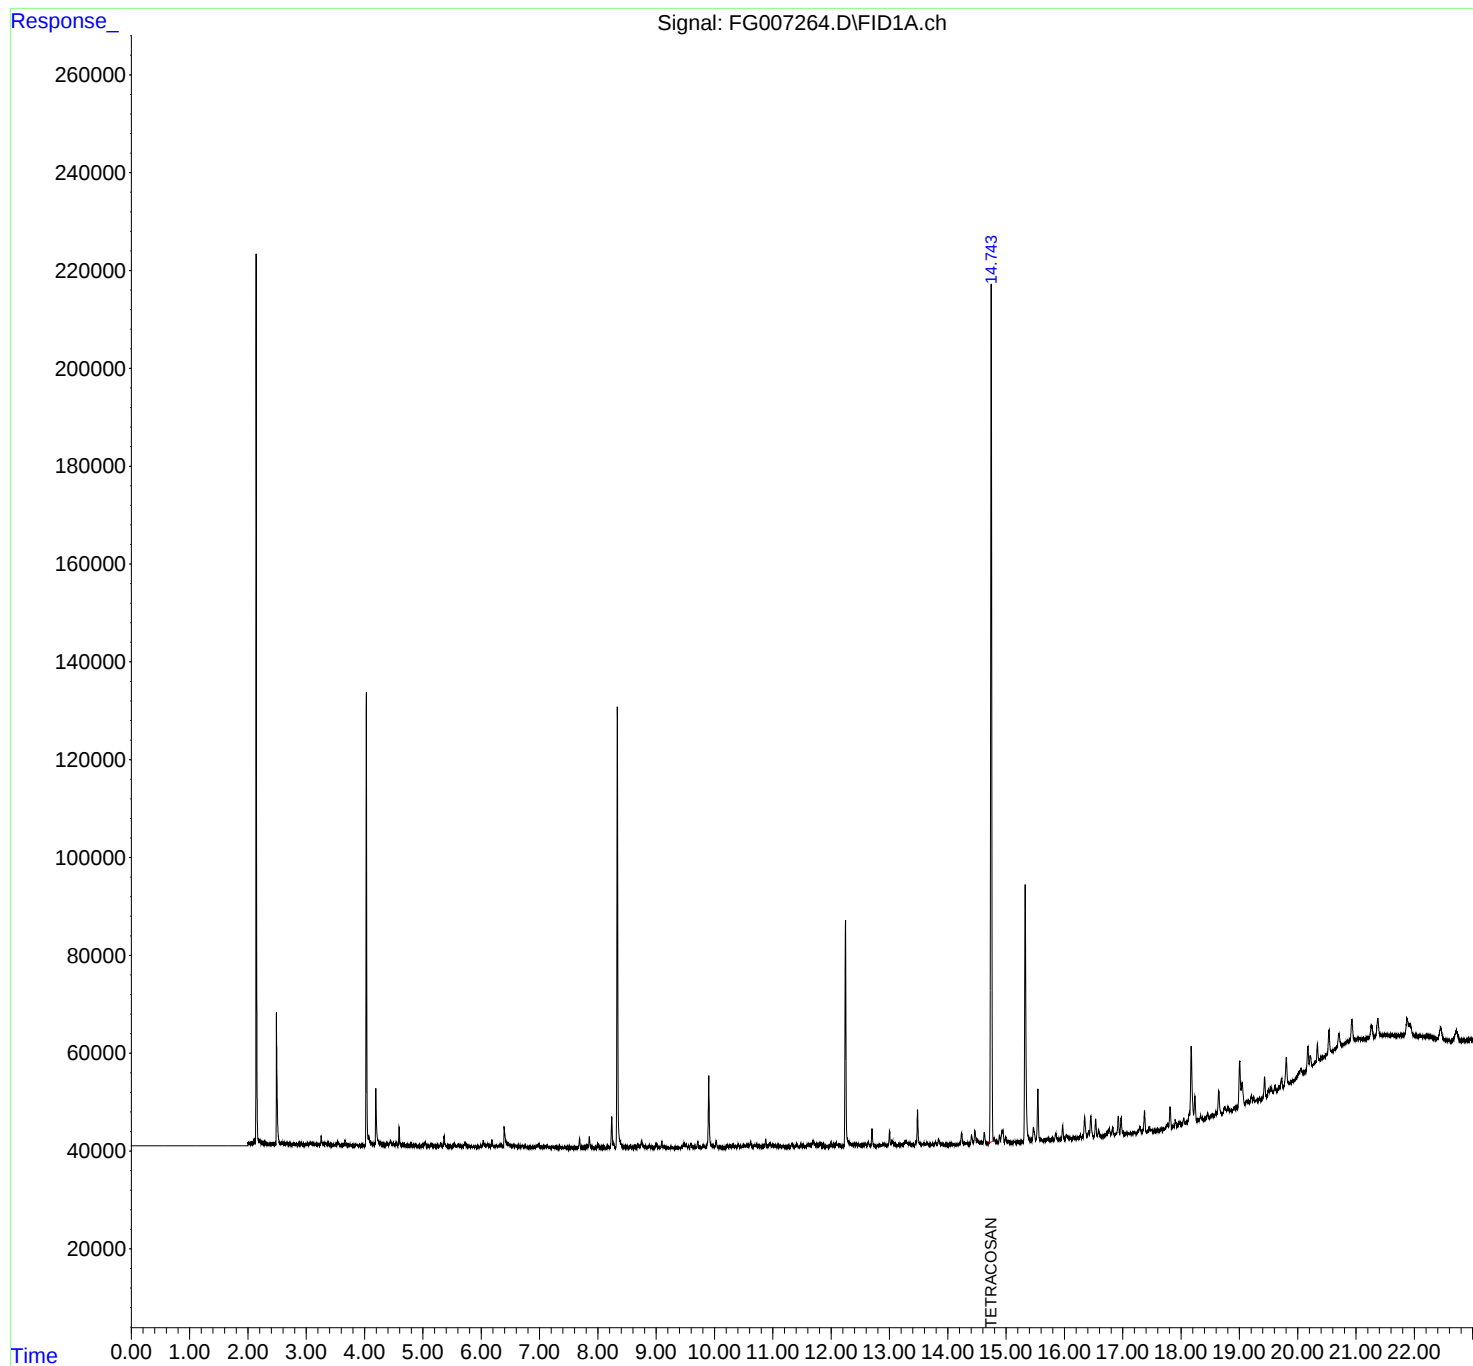

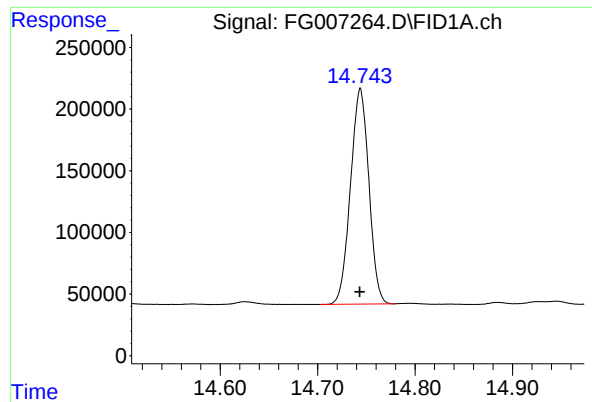

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.744 min
Delta R.T.: 0.000 min
Response: 2292453
Conc: 18.83 ug/ml

Instrument :
FID_G
ClientSampleId :
TP-1916-GC-GRAB-A