

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102922\
Data File : FG011057.D
Signal(s) : FID1A.ch
Acq On : 28 Oct 2022 08:05
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 29 07:14:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102722.M
Quant Title :
QLast Update : Thu Oct 27 00:27:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
7)	N-EICOSANE	12.609	410678	2.807 ug/ml
8)	N-DOCOSANE	13.820	375609	2.669 ug/ml
10)	N-TETRACOSANE	14.881	1181050	8.545 ug/ml
15)	N-TETRATRIACONTANE	19.408	347671	2.244 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102922\
Data File : FG011057.D
Signal(s) : FID1A.ch
Acq On : 28 Oct 2022 08:05
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 29 07:14:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102722.M
Quant Title :
QLast Update : Thu Oct 27 00:27:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

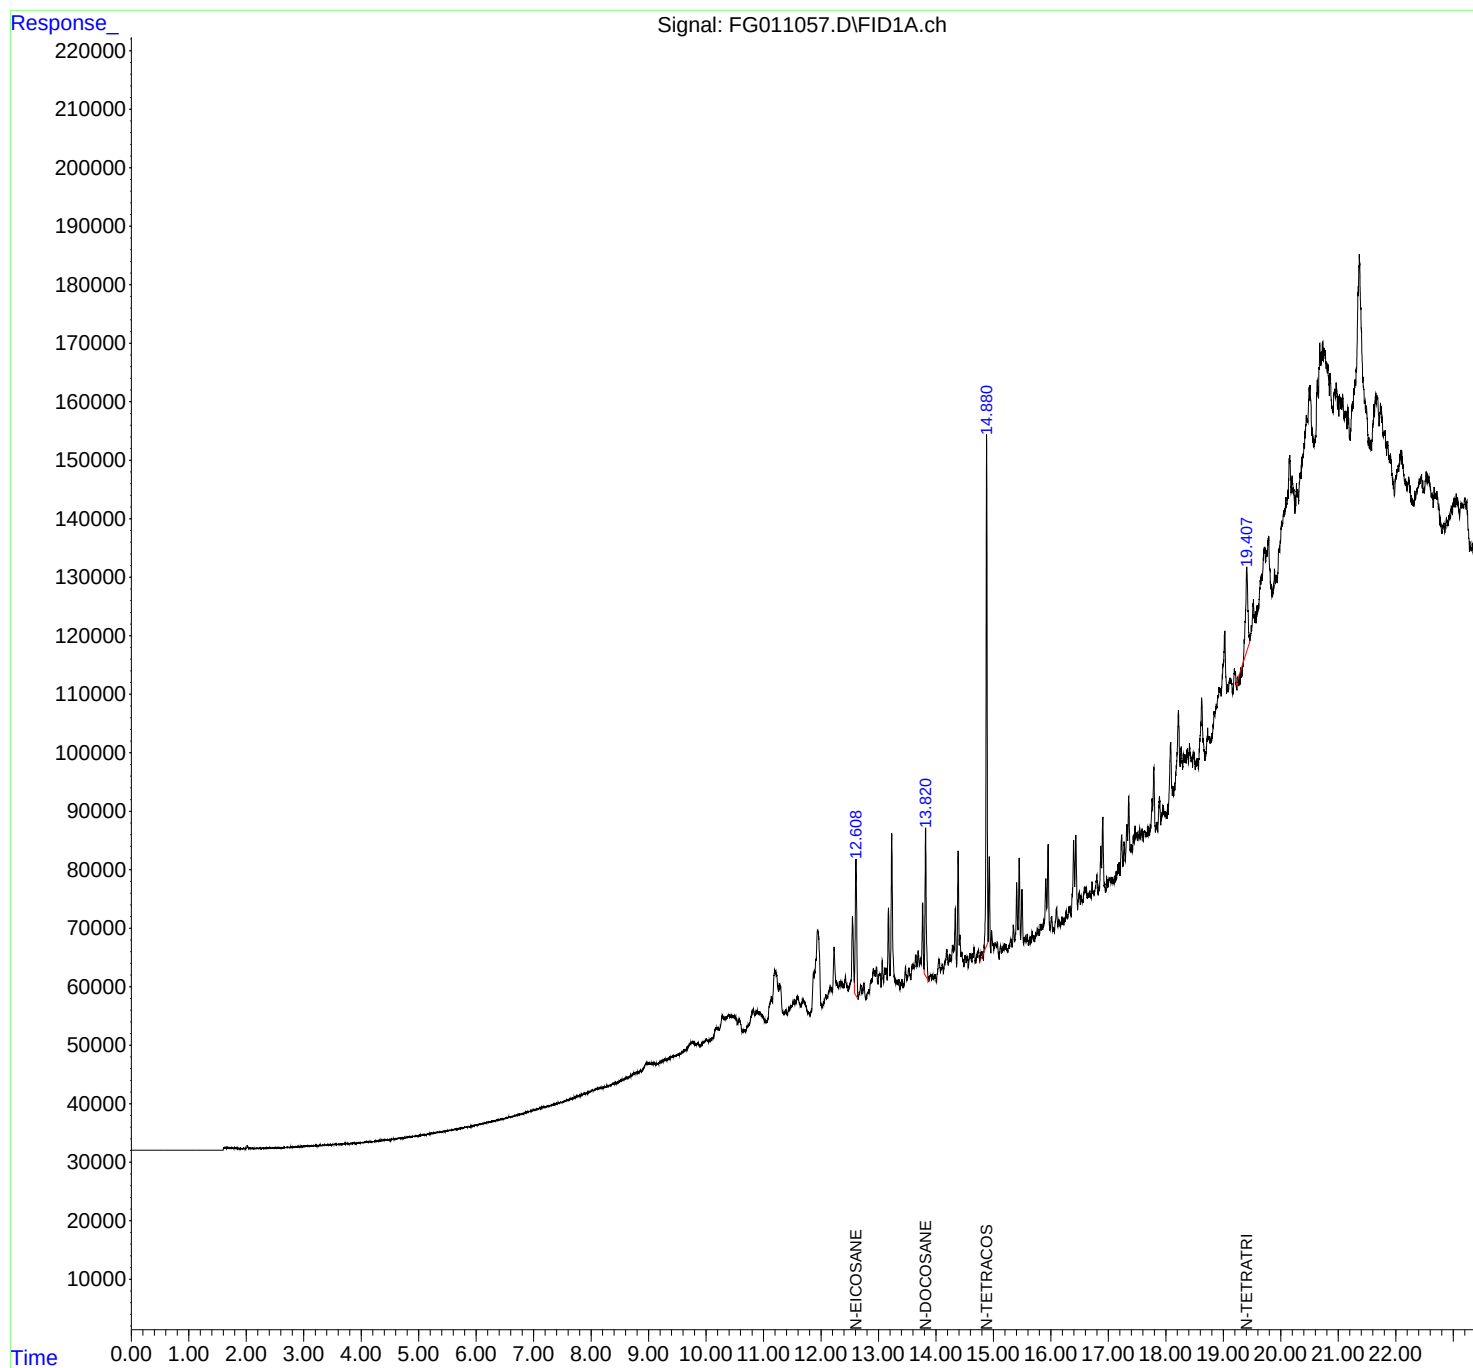


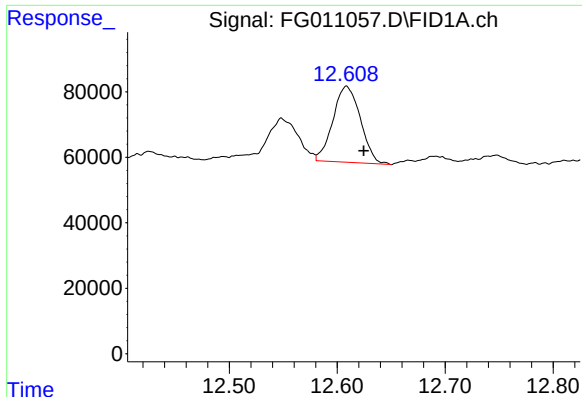

#7 N-EICOSANE


R.T.: 12.609 min
Delta R.T.: -0.016 min
Response: 410678
Conc: 2.81 ug/ml

Instrument :
FID_G
ClientSampleId :

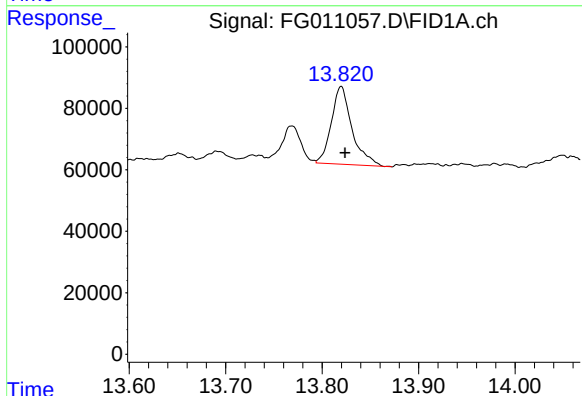


#8 N-DOCOSANE

R.T.: 13.820 min
Delta R.T.: -0.004 min
Response: 375609
Conc: 2.67 ug/ml

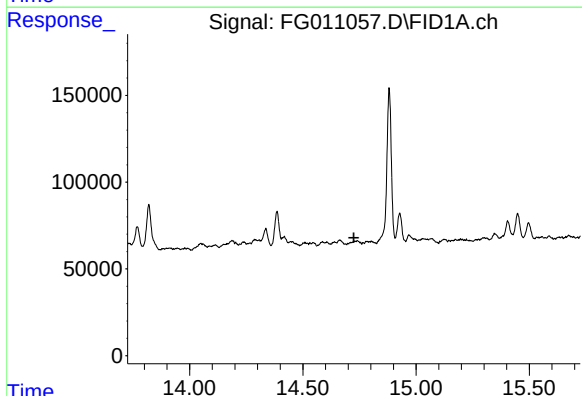


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.725 min
Response: 0
Conc: N.D.

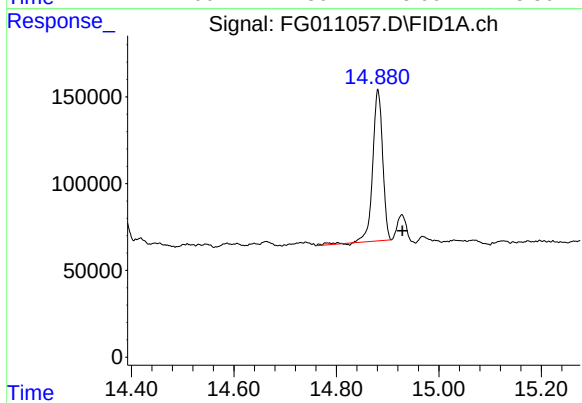

#10 N-TETRACOSANE

R.T.: 14.881 min
Delta R.T.: -0.048 min
Response: 1181050
Conc: 8.54 ug/ml

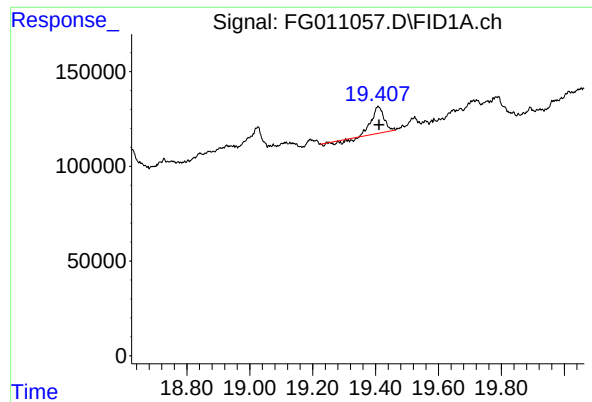

#15 N-TETRATRIACONTANE

R.T.: 19.408 min
Delta R.T.: -0.003 min
Response: 347671
Conc: 2.24 ug/ml

Instrument :

FID_G

ClientSampleId :