

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102922\
Data File : FG011061.D
Signal(s) : FID1A.ch
Acq On : 28 Oct 2022 10:10
Operator : YP\AJ
Sample : N5235-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
LSP-GW-03-DUP

Integration File: autoint1.e
Quant Time: Oct 29 07:14:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102722.M
Quant Title :
QLast Update : Thu Oct 27 00:27:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.727	2112664	17.173 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102922\
Data File : FG011061.D
Signal(s) : FID1A.ch
Acq On : 28 Oct 2022 10:10
Operator : YP\AJ
Sample : N5235-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
LSP-GW-03-DUP

Integration File: autoint1.e
Quant Time: Oct 29 07:14:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102722.M
Quant Title :
QLast Update : Thu Oct 27 00:27:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

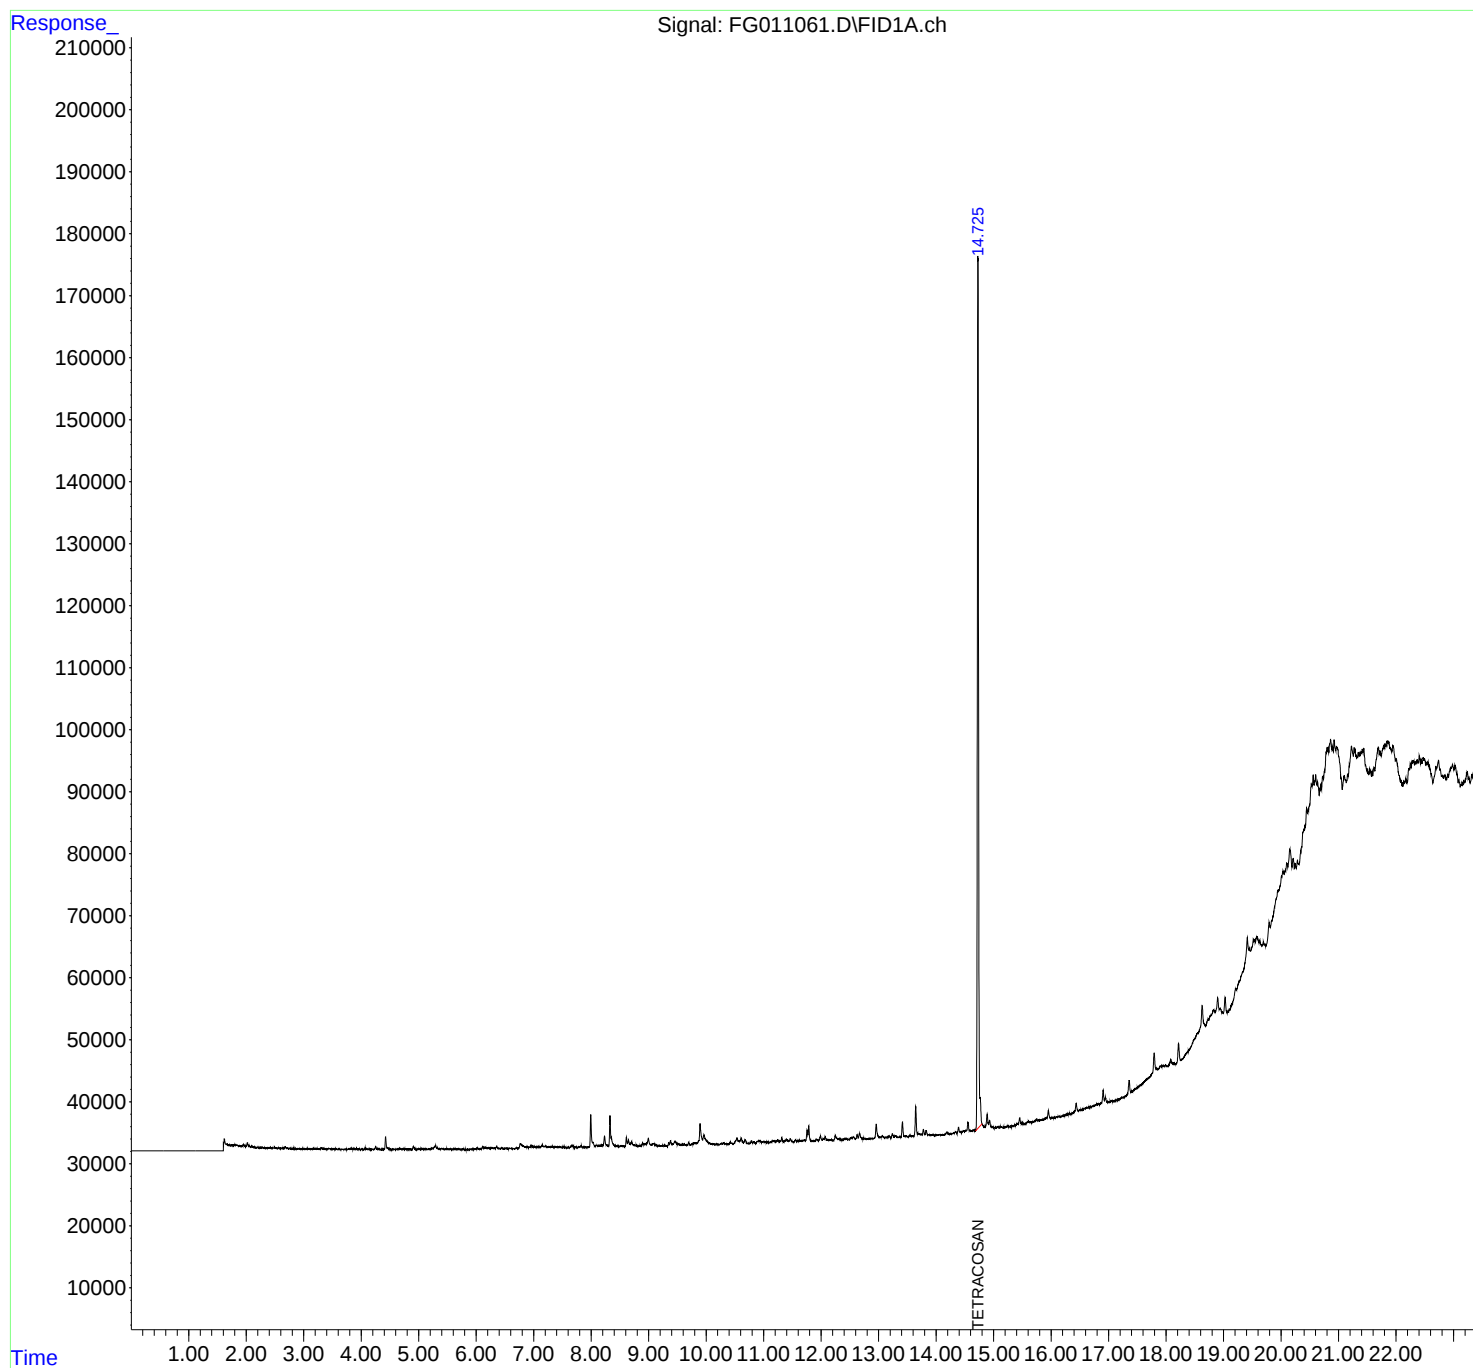

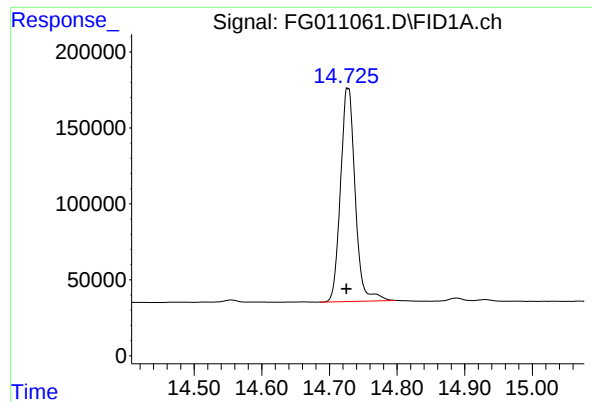

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.727 min
Delta R.T.: 0.002 min
Response: 2112664
Conc: 17.17 ug/ml

Instrument :
FID_G
ClientSampleId :
LSP-GW-03-DUP