

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102924AL\
Data File : FG014572.D
Signal(s) : FID1A.ch
Acq On : 29 Oct 2024 22:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 30 06:19:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 102124.M
Quant Title : GC Extractables
QLast Update : Tue Oct 22 06:49:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.117	54080	0.390 ug/ml
18) T	n-Dotriacontane (C32)	18.950	66568	0.508 ug/ml
19) T	n-Tetratriacontane (C34)	19.732	51539	0.460 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG102924AL\
Data File : FG014572.D
Signal(s) : FID1A.ch
Acq On : 29 Oct 2024 22:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 30 06:19:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 102124.M
Quant Title : GC Extractables
QLast Update : Tue Oct 22 06:49:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

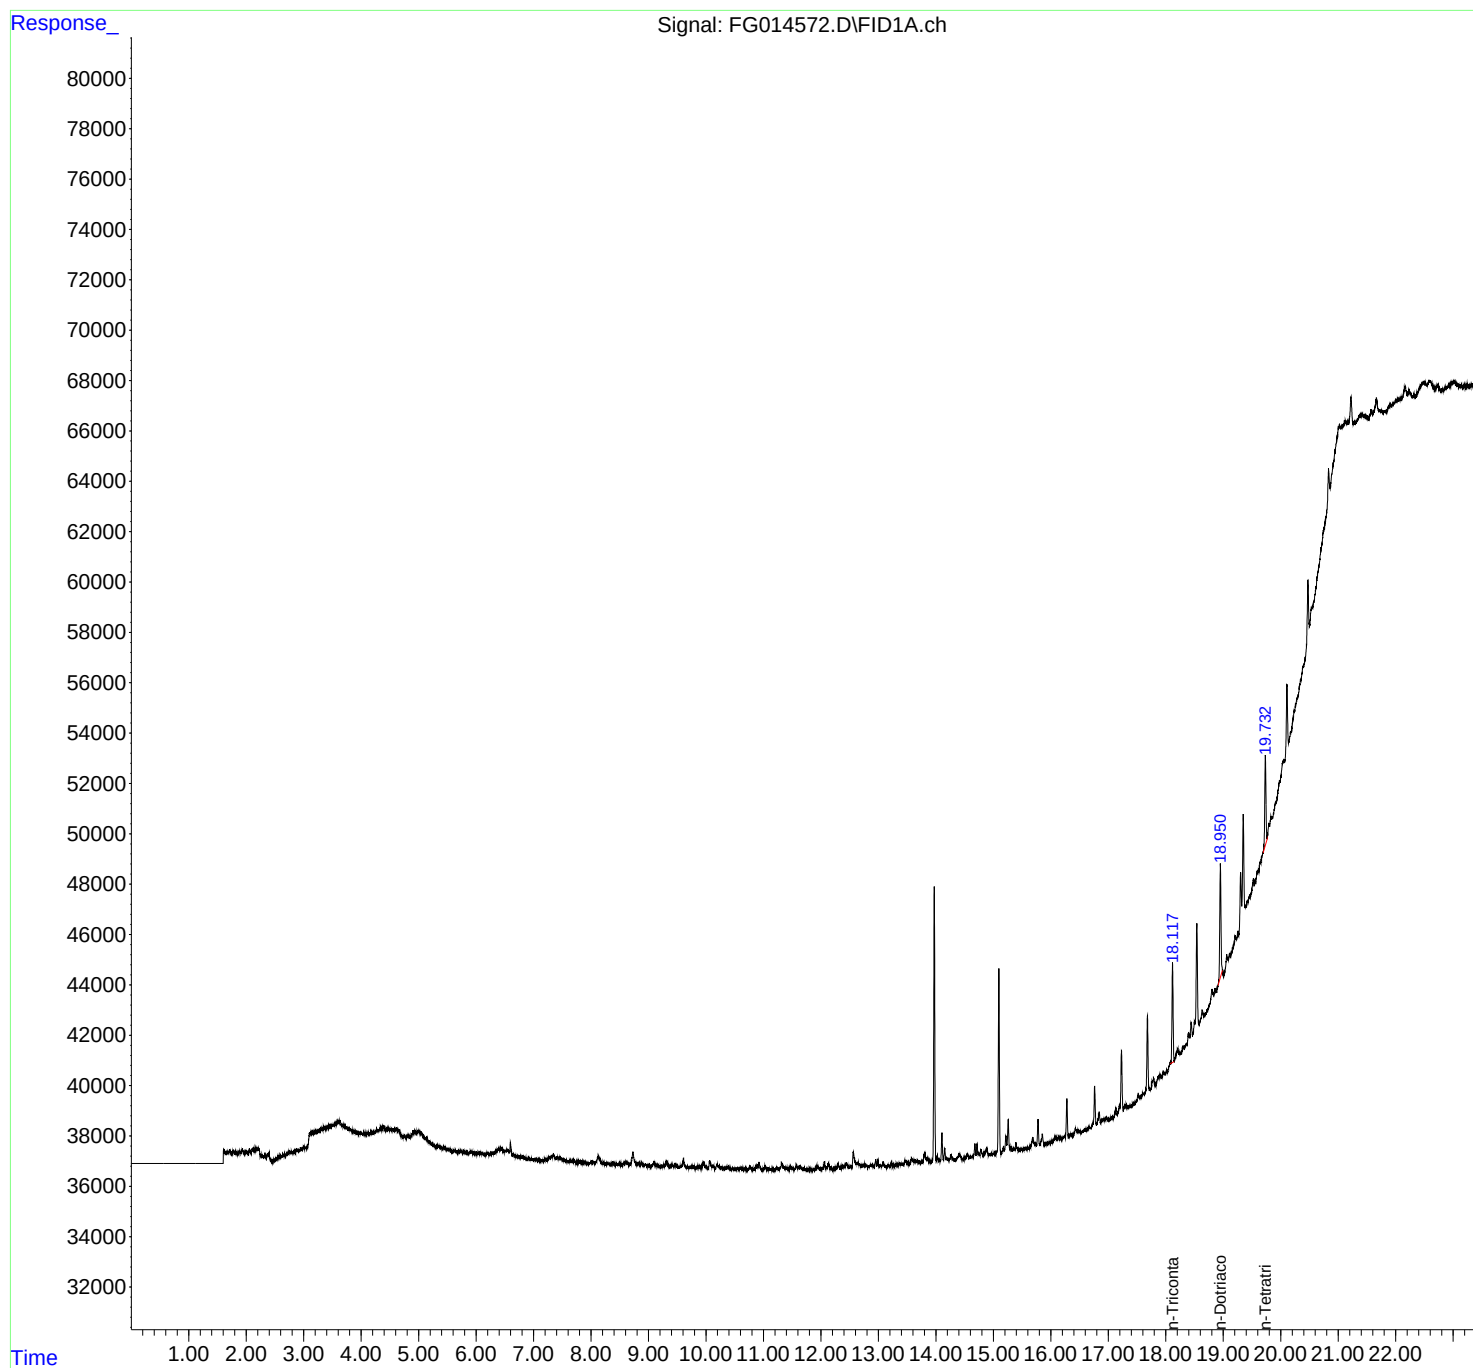


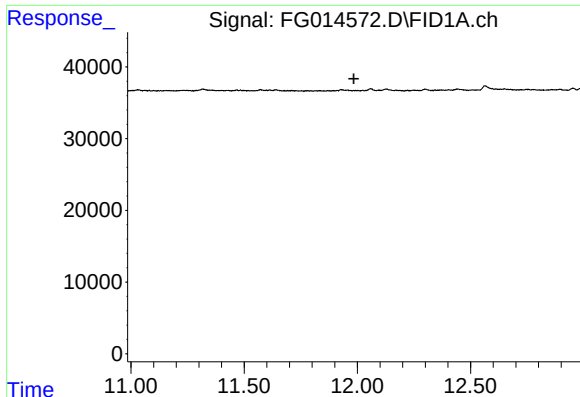

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.984 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

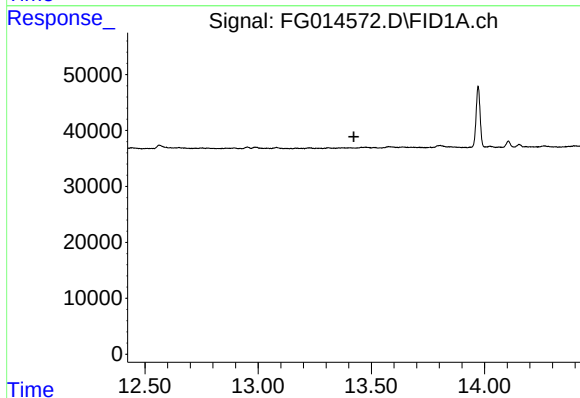


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.423 min
Response: 0
Conc: N.D.

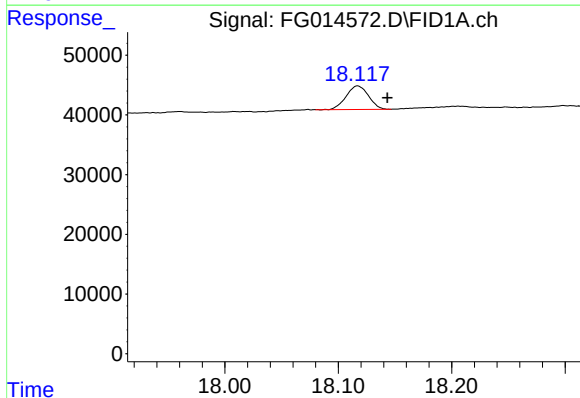


#17 n-Tricontane (C30)

R.T.: 18.117 min
Delta R.T.: -0.026 min
Response: 54080
Conc: 0.39 ug/ml

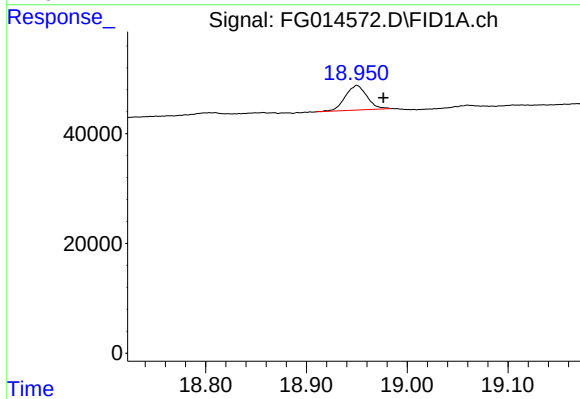

#18 n-Dotriacontane (C32)

R.T.: 18.950 min
Delta R.T.: -0.026 min
Response: 66568
Conc: 0.51 ug/ml

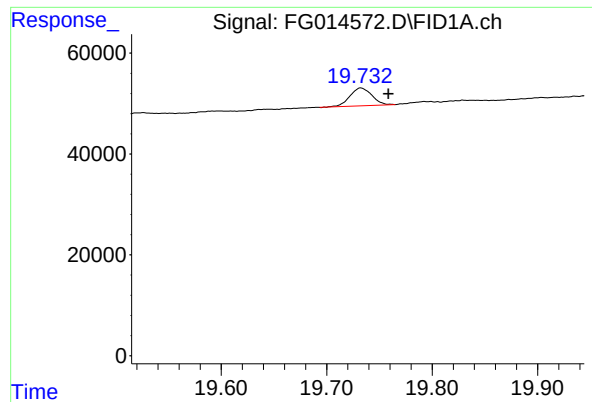

#19 n-Tetratriacontane (C34)

R.T.: 19.732 min
Delta R.T.: -0.026 min
Response: 51539
Conc: 0.46 ug/ml

Instrument :

FID_G

ClientSampleId :