

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG103118\  
 Data File : FG002715.D  
 Signal(s) : FID1A.ch  
 Acq On : 31 Oct 2018 16:20  
 Operator : AJ\SJ  
 Sample : J5737-01  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Sample.e  
 Quant Time: Nov 01 00:33:10 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG102618.M  
 Quant Title :  
 QLast Update : Sat Oct 27 02:13:37 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.773	1292218	11.758 ug/ml
Target Compounds			
2) N-DECANE	4.460	3139	0.025 ug/ml
3) N-DODECANE	6.491	10451	0.080 ug/ml
4) N-TETRADECANE	8.294	19130	0.145 ug/ml
5) N-HEXADECANE	9.902	18043	0.135 ug/ml
6) N-OCTADECANE	11.351	13938	0.105 ug/ml
7) N-EICOSANE	12.665	15997	0.123 ug/ml
8) N-DOCOSANE	13.869	21781	0.171 ug/ml
10) N-TETRACOSANE	14.977	71610	0.573 ug/ml
11) N-HEXACOSANE	16.004	231149	1.876 ug/ml
12) N-OCTACOSANE	16.957	601455	4.945 ug/ml
-----			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG103118\  
 Data File : FG002715.D  
 Signal(s) : FID1A.ch  
 Acq On : 31 Oct 2018 16:20  
 Operator : AJ\SJ  
 Sample : J5737-01  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1


Integration File: Sample.e  
 Quant Time: Nov 01 00:33:10 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG102618.M  
 Quant Title :  
 QLast Update : Sat Oct 27 02:13:37 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

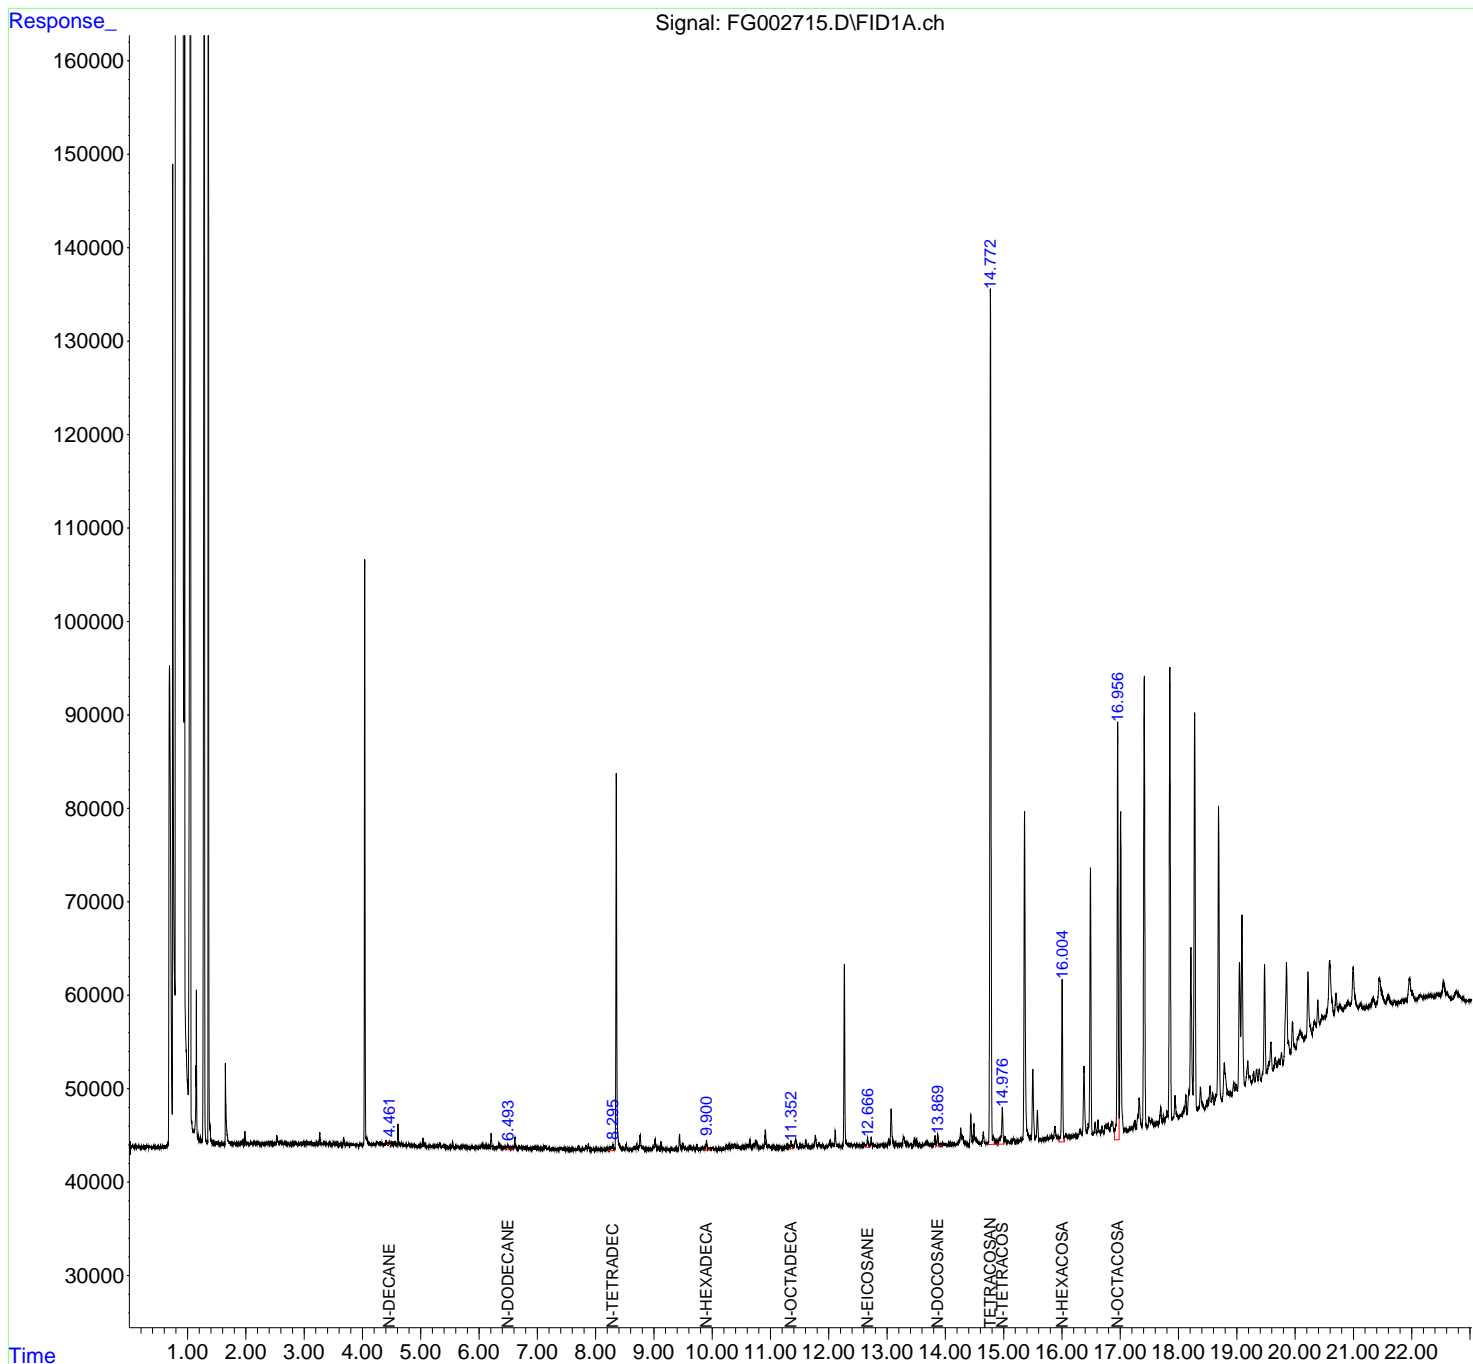


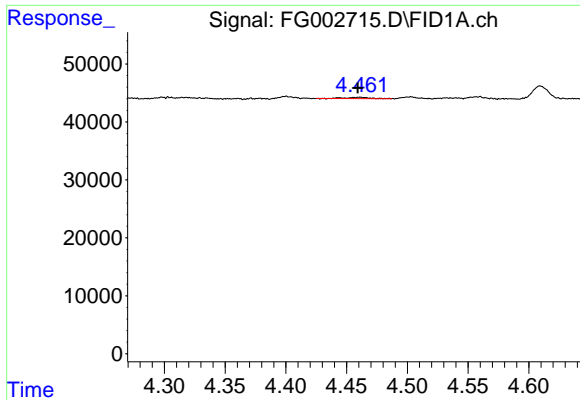


#2 N-DECANE  
R.T.: 4.460 min  
Delta R.T.: 0.001 min  
Response: 3139  
Conc: 0.02 ug/ml

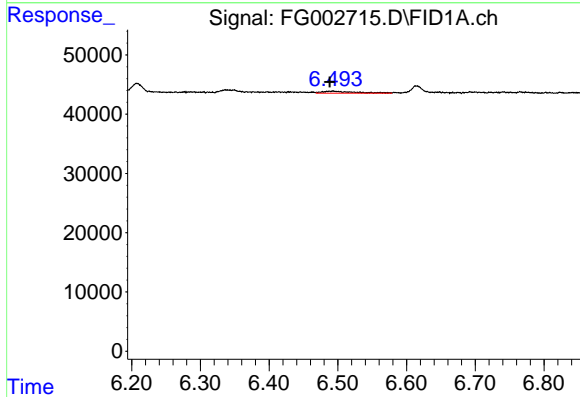


#3 N-DODECANE  
R.T.: 6.491 min  
Delta R.T.: 0.003 min  
Response: 10451  
Conc: 0.08 ug/ml

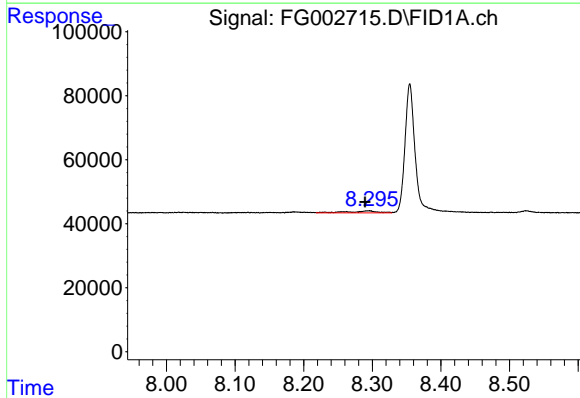


#4 N-TETRADECANE  
R.T.: 8.294 min  
Delta R.T.: 0.004 min  
Response: 19130  
Conc: 0.14 ug/ml

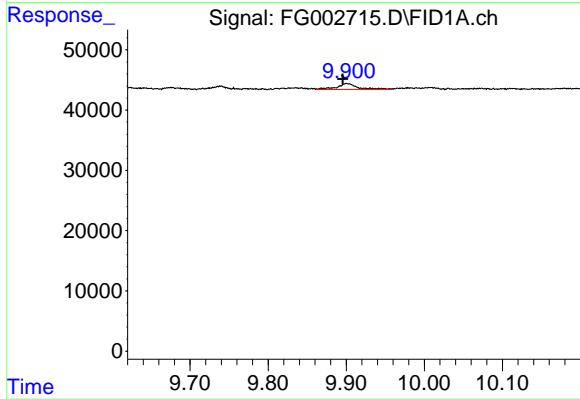


#5 N-HEXADECANE  
R.T.: 9.902 min  
Delta R.T.: 0.006 min  
Response: 18043  
Conc: 0.14 ug/ml

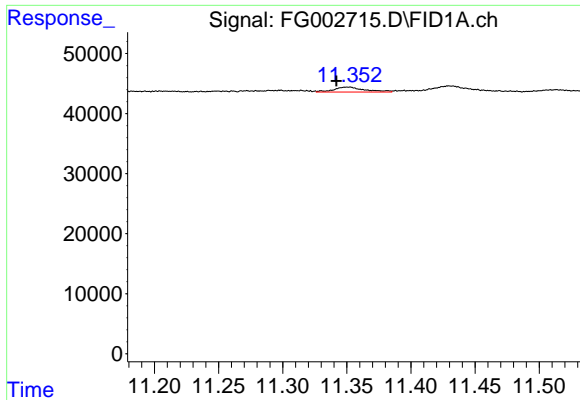


#6 N-OCTADECANE  
R.T.: 11.351 min  
Delta R.T.: 0.009 min  
Response: 13938  
Conc: 0.11 ug/ml

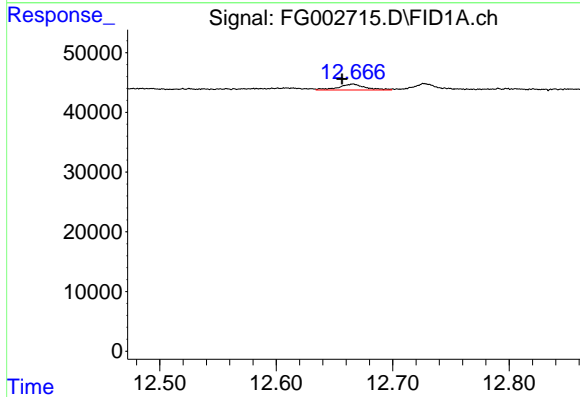


#7 N-EICOSANE  
R.T.: 12.665 min  
Delta R.T.: 0.009 min  
Response: 15997  
Conc: 0.12 ug/ml

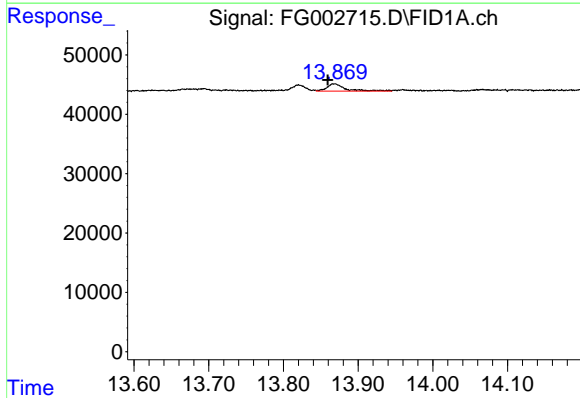

#8 N-DOCOSANE  
R.T.: 13.869 min  
Delta R.T.: 0.009 min  
Response: 21781  
Conc: 0.17 ug/ml

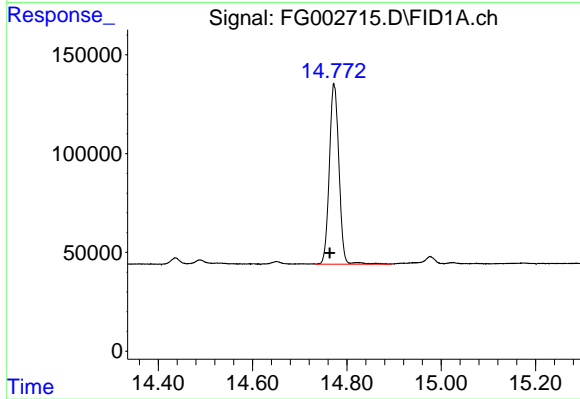


#9 TETRACOSANE-d50 (SURROGATE)  
R.T.: 14.773 min  
Delta R.T.: 0.010 min  
Response: 1292218  
Conc: 11.76 ug/ml

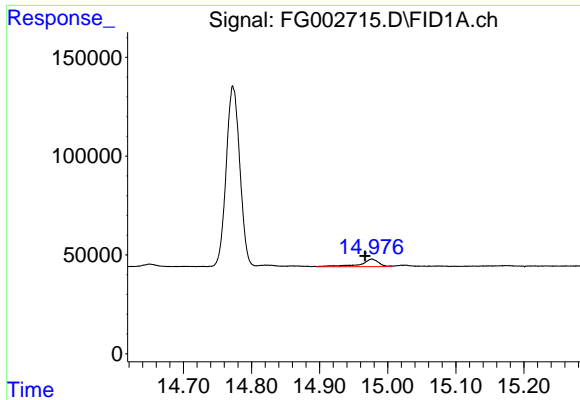


#10 N-TETRACOSANE

R.T.: 14.977 min  
Delta R.T.: 0.010 min  
Response: 71610  
Conc: 0.57 ug/ml

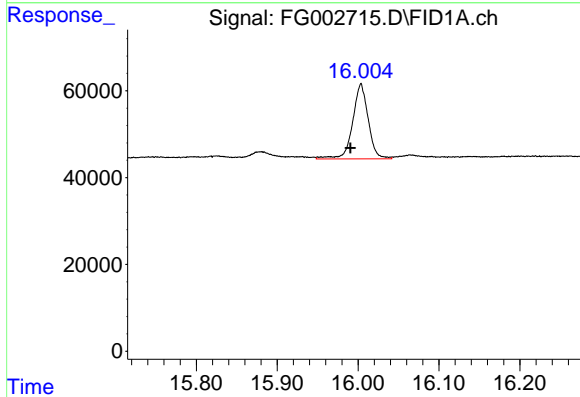

#11 N-HEXACOSANE

R.T.: 16.004 min  
Delta R.T.: 0.013 min  
Response: 231149  
Conc: 1.88 ug/ml

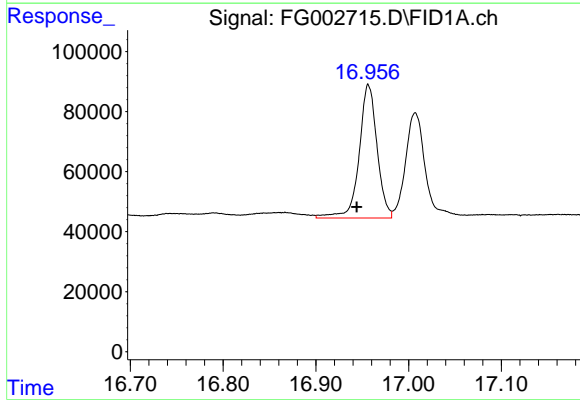

#12 N-OCTACOSANE

R.T.: 16.957 min  
Delta R.T.: 0.013 min  
Response: 601455  
Conc: 4.95 ug/ml