

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG103118\
 Data File : FG002720.D
 Signal(s) : FID1A.ch
 Acq On : 31 Oct 2018 18:54
 Operator : AJ\SJ
 Sample : J5737-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Nov 01 00:34:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.774	1226508	11.160 ug/ml
Target Compounds			
2) N-DECANE	4.460	1102	0.009 ug/ml
3) N-DODECANE	6.492	8341	0.064 ug/ml
4) N-TETRADECANE	8.292	15794	0.119 ug/ml
5) N-HEXADECANE	9.921	45485	0.342 ug/ml
6) N-OCTADECANE	11.355	18357	0.139 ug/ml
7) N-EICOSANE	12.666	21047	0.162 ug/ml
8) N-DOCOSANE	13.869	31066	0.244 ug/ml
10) N-TETRACOSANE	14.976	88544	0.709 ug/ml
11) N-HEXACOSANE	16.004	210409	1.707 ug/ml
12) N-OCTACOSANE	16.959	522748	4.298 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG103118\
Data File : FG002720.D
Signal(s) : FID1A.ch
Acq On : 31 Oct 2018 18:54
Operator : AJ\SJ
Sample : J5737-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 01 00:34:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

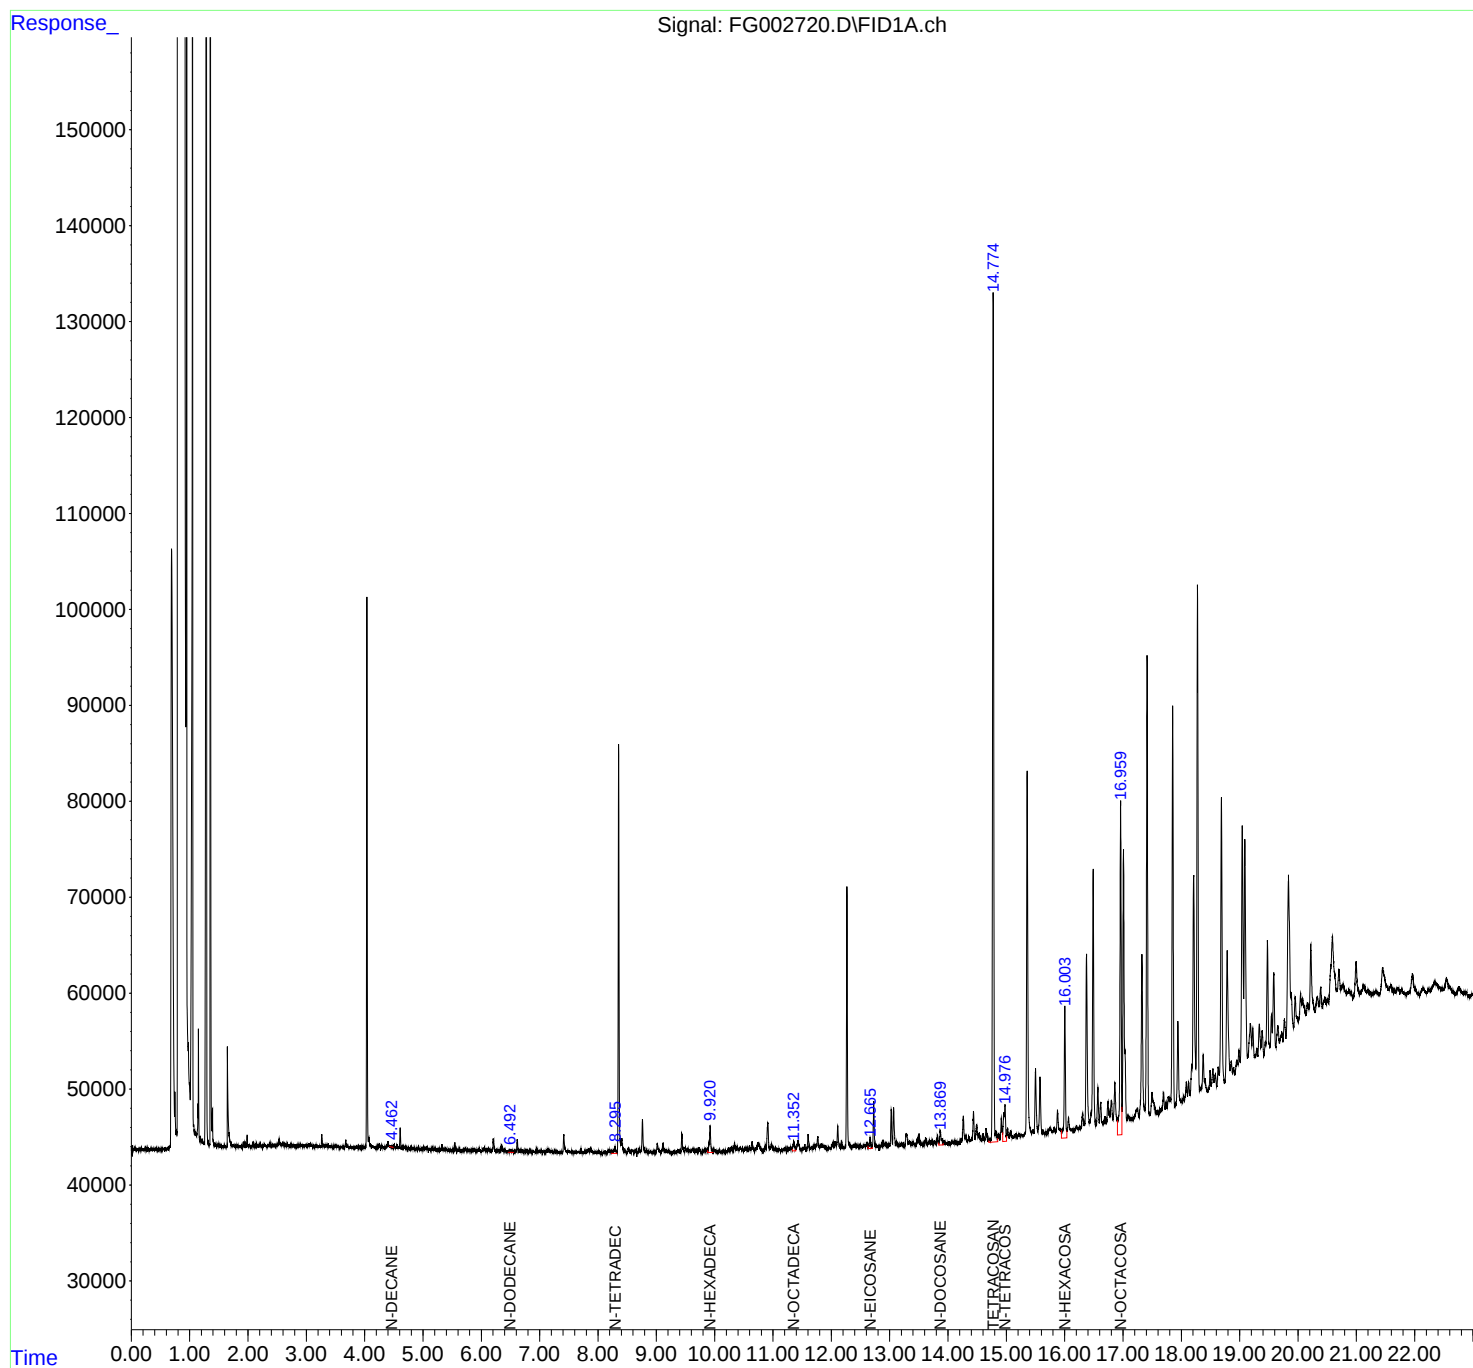

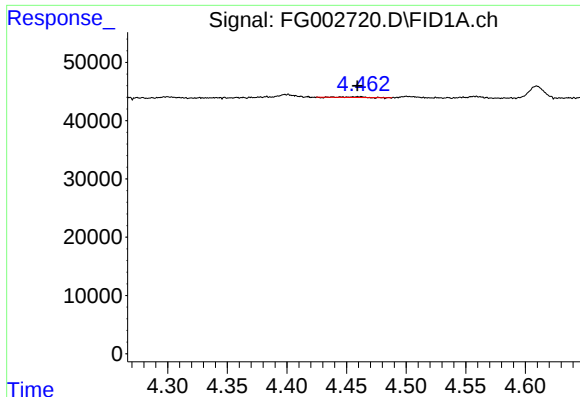


#2 N-DECANE

R.T.: 4.460 min
Delta R.T.: 0.000 min
Response: 1102
Conc: 0.01 ug/ml

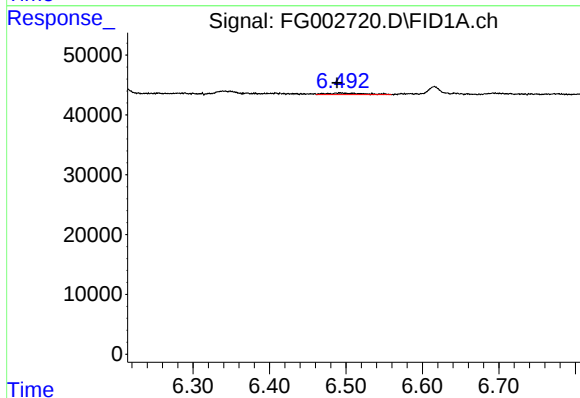


#3 N-DODECANE

R.T.: 6.492 min
Delta R.T.: 0.004 min
Response: 8341
Conc: 0.06 ug/ml

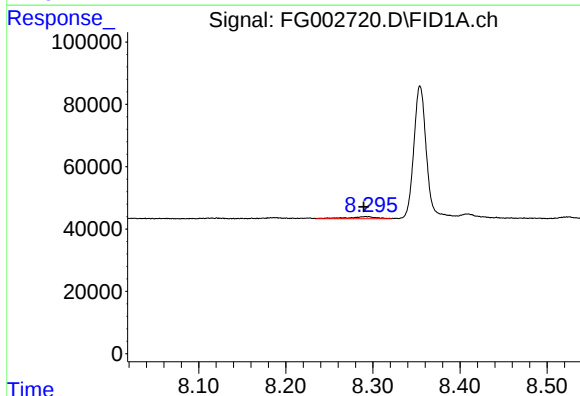


#4 N-TETRADECANE

R.T.: 8.292 min
Delta R.T.: 0.003 min
Response: 15794
Conc: 0.12 ug/ml

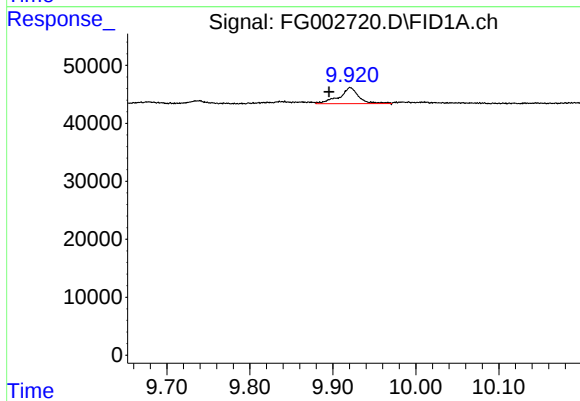


#5 N-HEXADECANE

R.T.: 9.921 min
Delta R.T.: 0.026 min
Response: 45485
Conc: 0.34 ug/ml

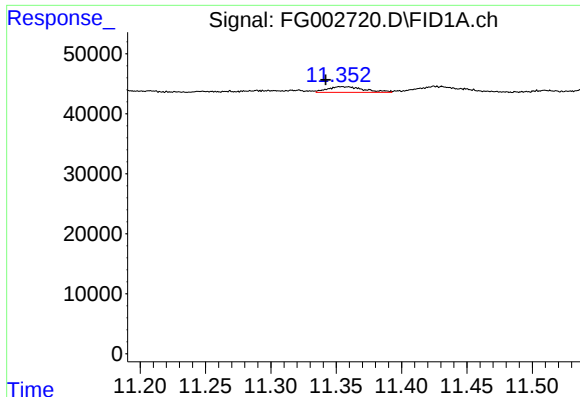


#6 N-OCTADECANE

R.T.: 11.355 min
Delta R.T.: 0.013 min
Response: 18357
Conc: 0.14 ug/ml

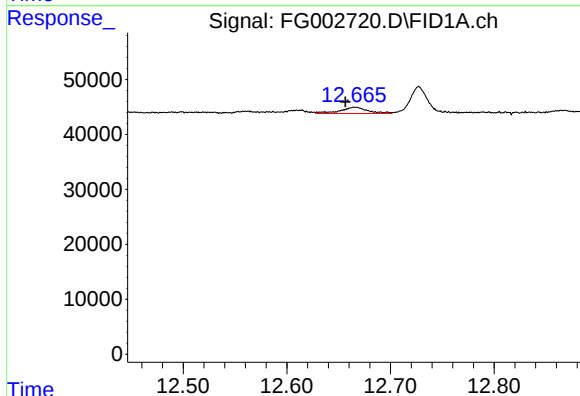


#7 N-EICOSANE

R.T.: 12.666 min
Delta R.T.: 0.009 min
Response: 21047
Conc: 0.16 ug/ml

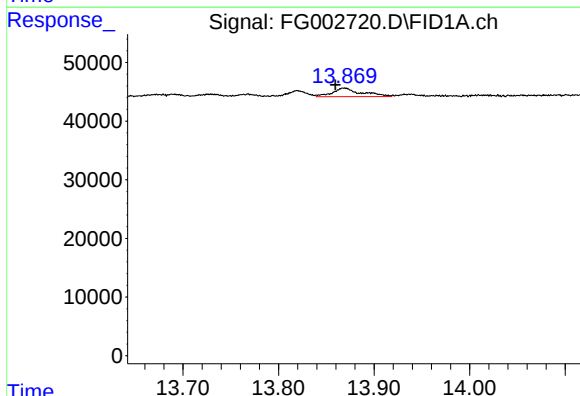


#8 N-DOCOSANE

R.T.: 13.869 min
Delta R.T.: 0.009 min
Response: 31066
Conc: 0.24 ug/ml

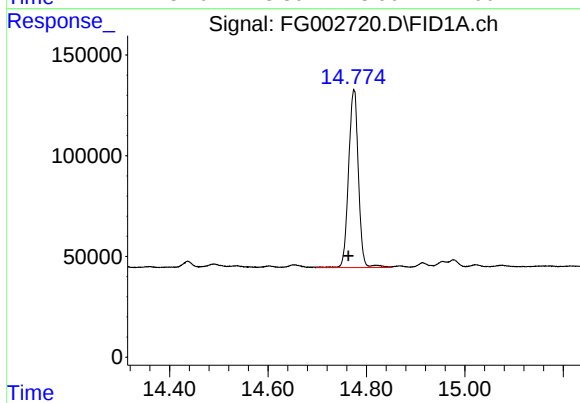


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.774 min
Delta R.T.: 0.011 min
Response: 1226508
Conc: 11.16 ug/ml

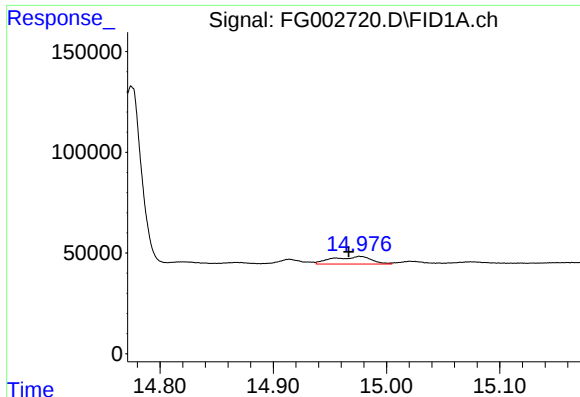


#10 N-TETRACOSANE

R.T.: 14.976 min
Delta R.T.: 0.009 min
Response: 88544
Conc: 0.71 ug/ml

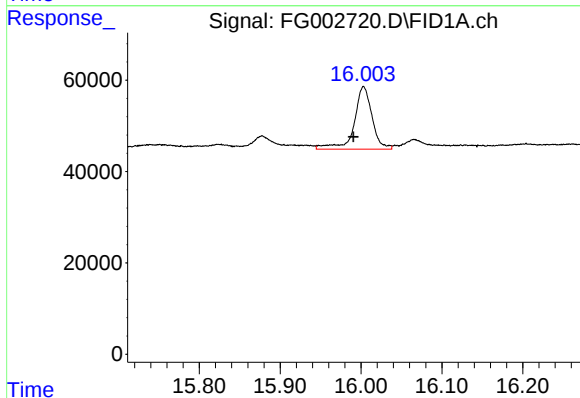

#11 N-HEXACOSANE

R.T.: 16.004 min
Delta R.T.: 0.013 min
Response: 210409
Conc: 1.71 ug/ml

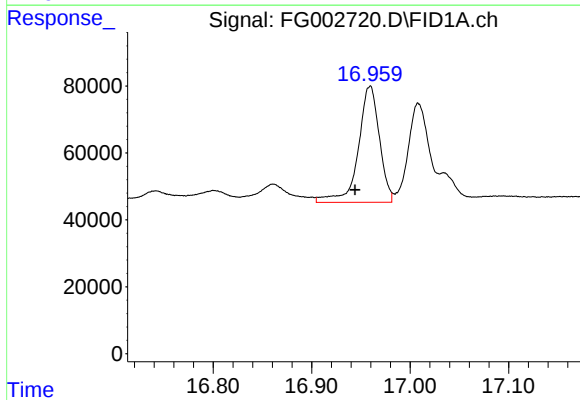

#12 N-OCTACOSANE

R.T.: 16.959 min
Delta R.T.: 0.015 min
Response: 522748
Conc: 4.30 ug/ml