

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG103119\
Data File : FG006221.D
Signal(s) : FID1A.ch
Acq On : 31 Oct 2019 14:45
Operator : DD\AJ
Sample : K5609-14 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 01 00:54:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG103019.M
Quant Title :
QLast Update : Thu Oct 31 03:29:10 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.364	336247	3.342 ug/ml
3) N-DODECANE	6.351	321228	3.187 ug/ml
4) N-TETRADECANE	8.116	540019	5.409 ug/ml
5) N-HEXADECANE	9.691	750802	7.561 ug/ml
6) N-OCTADECANE	11.110	462037	4.755 ug/ml
7) N-EICOSANE	12.400	323504	3.368 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG103119\
Data File : FG006221.D
Signal(s) : FID1A.ch
Acq On : 31 Oct 2019 14:45
Operator : DD\AJ
Sample : K5609-14 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 01 00:54:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG103019.M
Quant Title :
QLast Update : Thu Oct 31 03:29:10 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

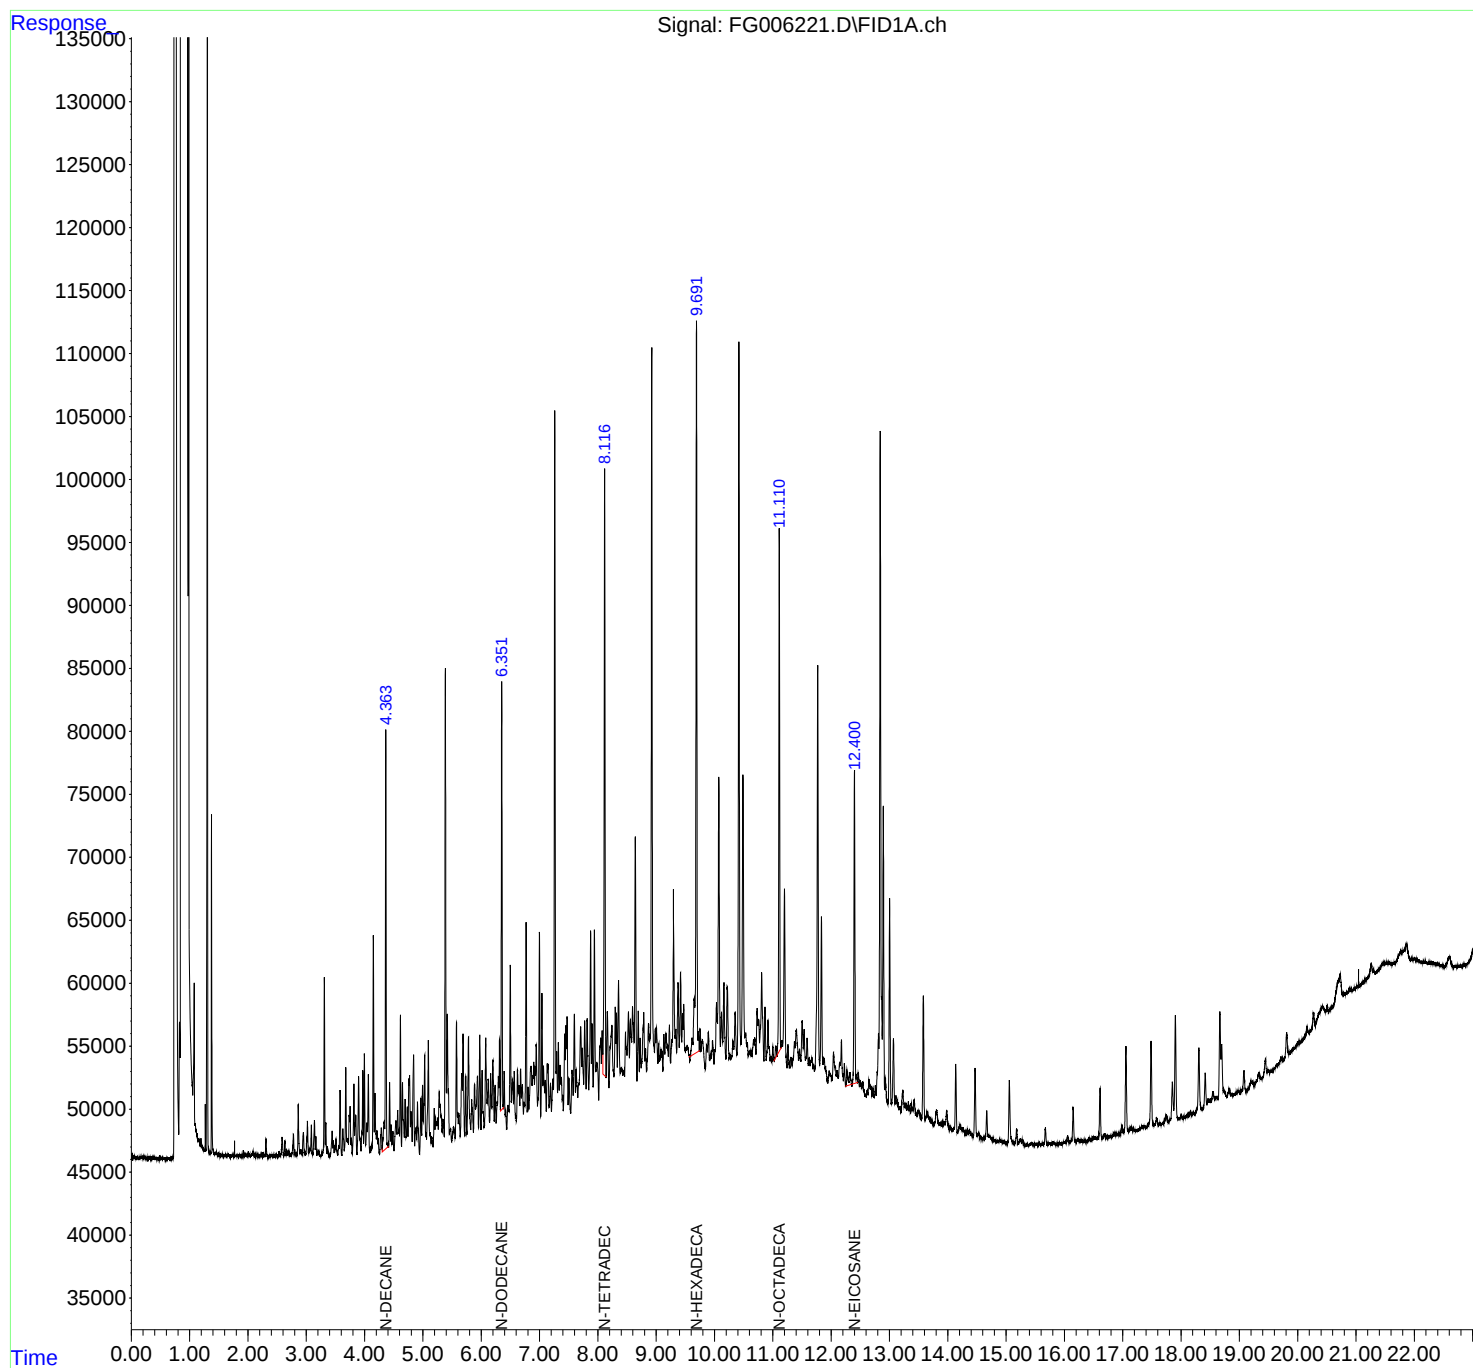


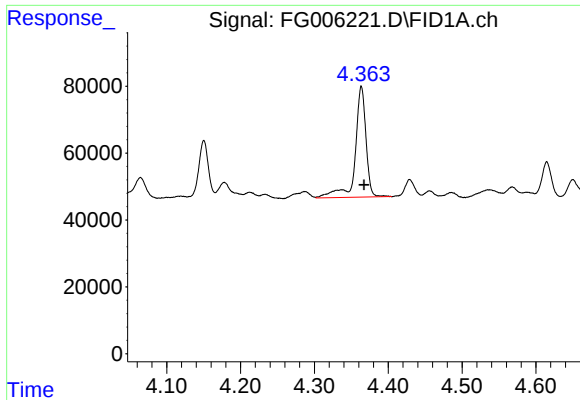

#2 N-DECANE


R.T.: 4.364 min
Delta R.T.: -0.003 min
Response: 336247
Conc: 3.34 ug/ml

Instrument :
FID_G
ClientSampleId :

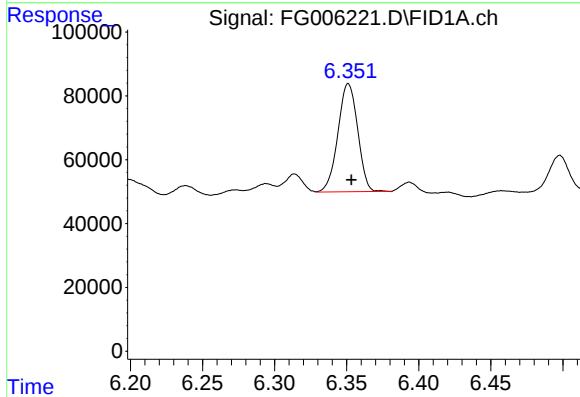


#3 N-DODECANE

R.T.: 6.351 min
Delta R.T.: -0.002 min
Response: 321228
Conc: 3.19 ug/ml

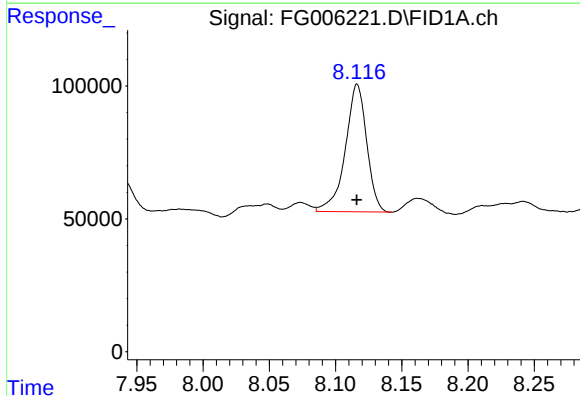


#4 N-TETRADECANE

R.T.: 8.116 min
Delta R.T.: 0.000 min
Response: 540019
Conc: 5.41 ug/ml

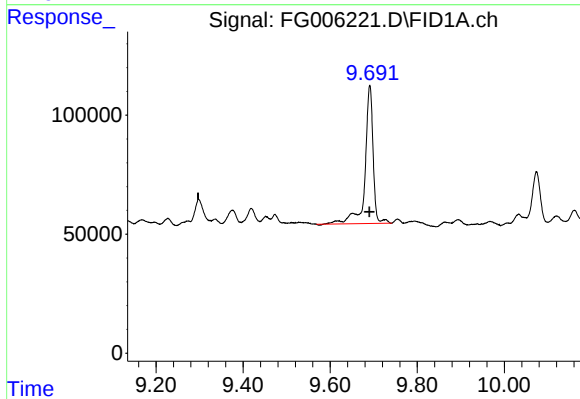

#5 N-HEXADECANE


R.T.: 9.691 min
Delta R.T.: 0.000 min
Response: 750802
Conc: 7.56 ug/ml

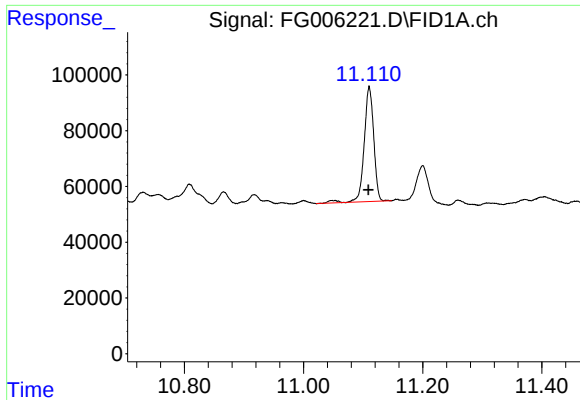

#6 N-OCTADECANE


R.T.: 11.110 min
Delta R.T.: 0.002 min
Response: 462037
Conc: 4.76 ug/ml

Instrument :
FID_G
ClientSampleId :

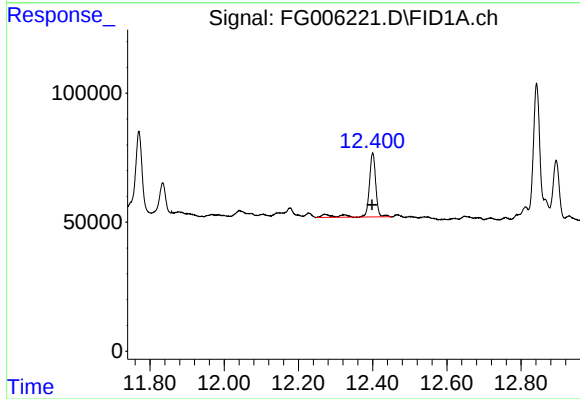

#7 N-EICOSANE

R.T.: 12.400 min
Delta R.T.: 0.002 min
Response: 323504
Conc: 3.37 ug/ml

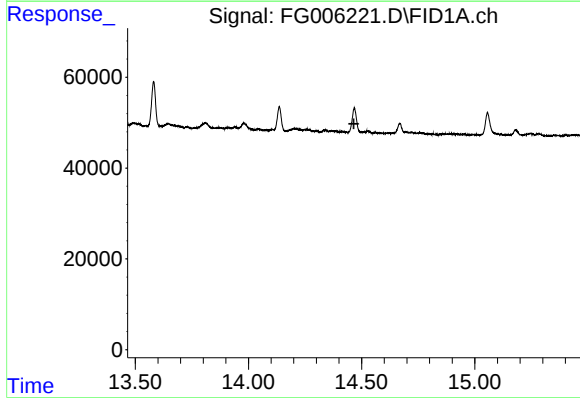

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.466 min
Response: 0
Conc: N.D.