

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110221\
Data File : FG008970.D
Signal(s) : FID1A.ch
Acq On : 02 Nov 2021 09:11
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:05:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.646	223406	2.052 ug/ml
16)	N-HEXATRIACONTANE	20.203	500694	5.308 ug/ml
18)	N-TETRACONTANE	21.893	451911	5.115 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110221\
Data File : FG008970.D
Signal(s) : FID1A.ch
Acq On : 02 Nov 2021 09:11
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:05:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

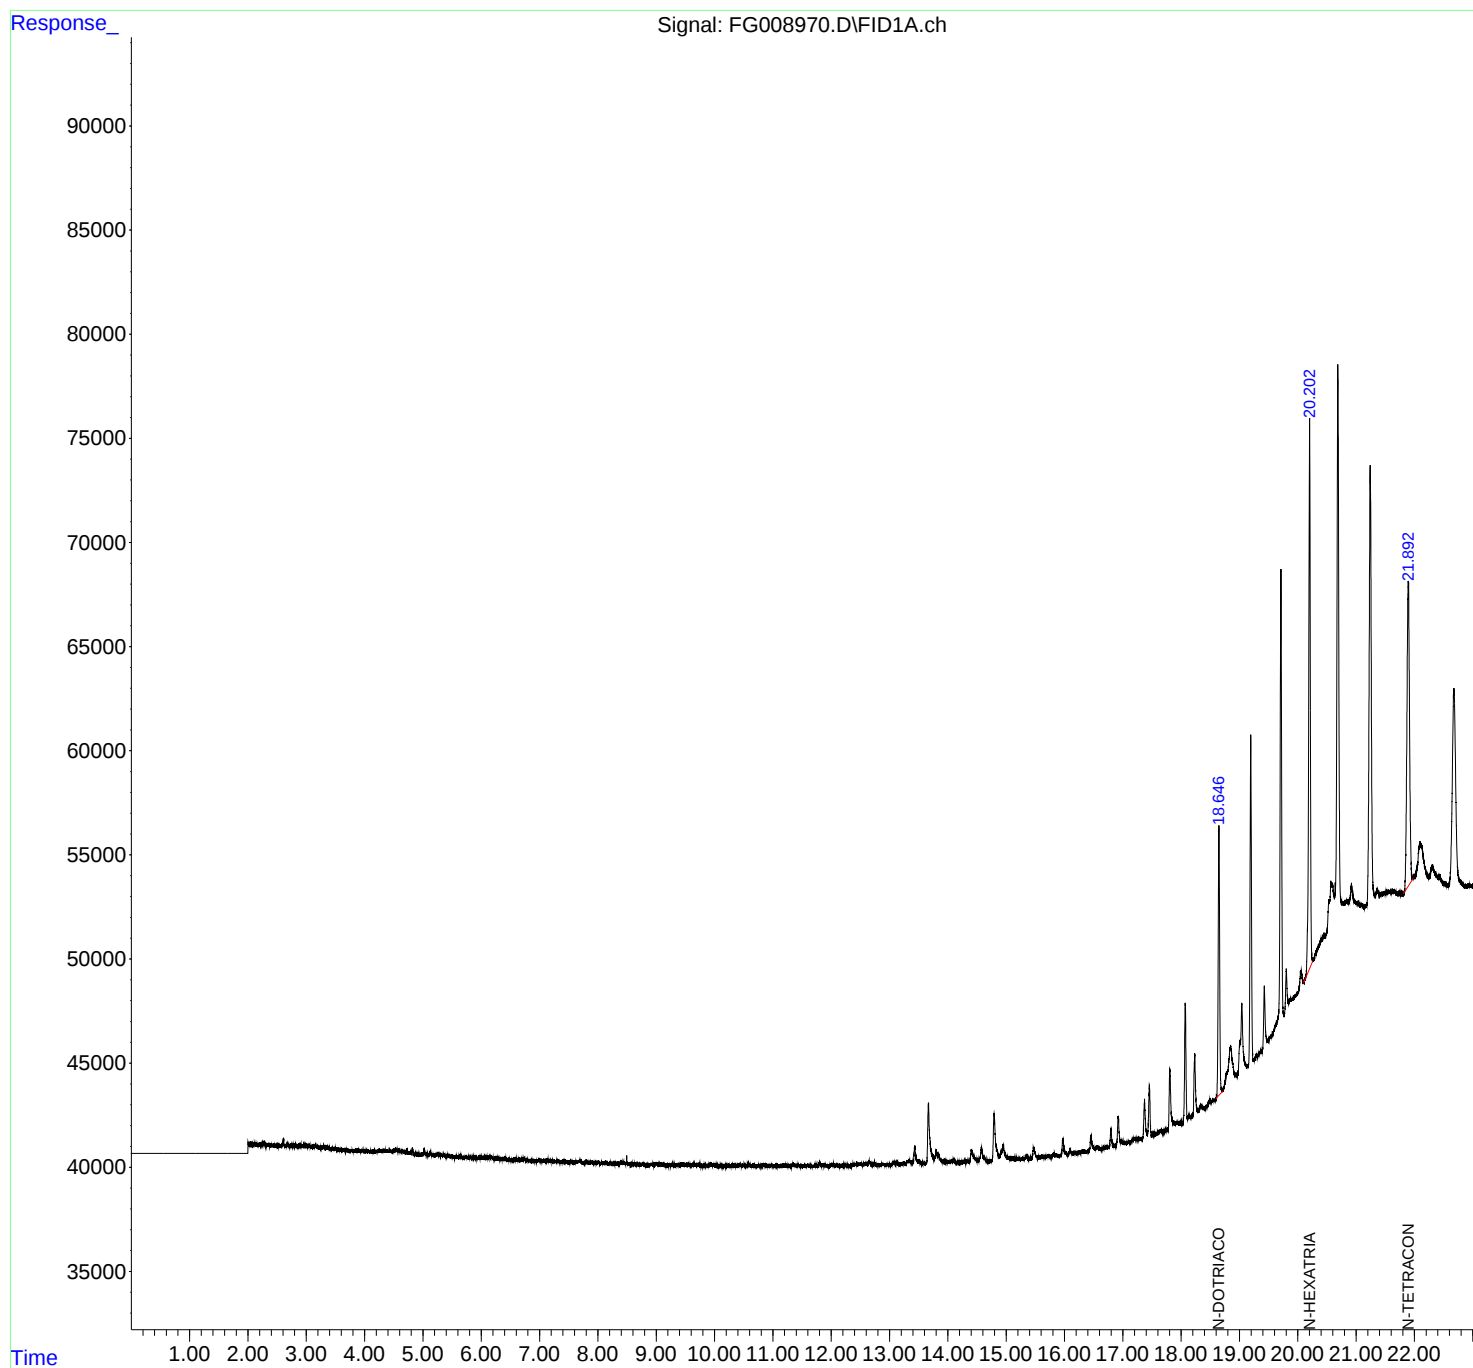


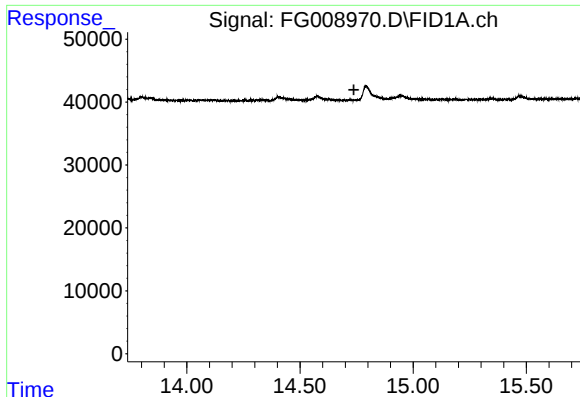

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.738 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

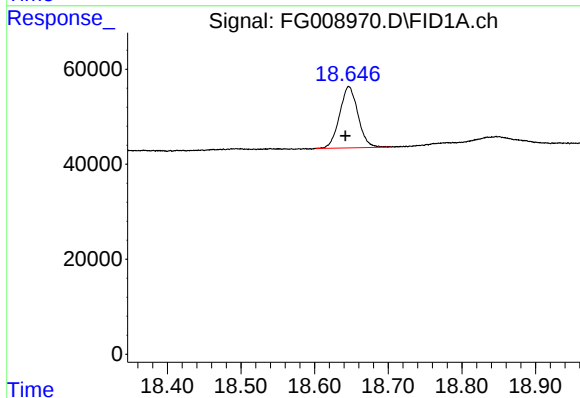


#14 N-DOTRIACONTANE

R.T.: 18.646 min
Delta R.T.: 0.004 min
Response: 223406
Conc: 2.05 ug/ml

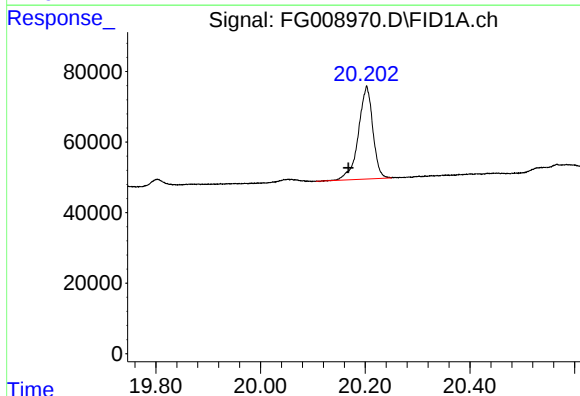

#16 N-HEXATRIACONTANE

R.T.: 20.203 min
Delta R.T.: 0.035 min
Response: 500694
Conc: 5.31 ug/ml

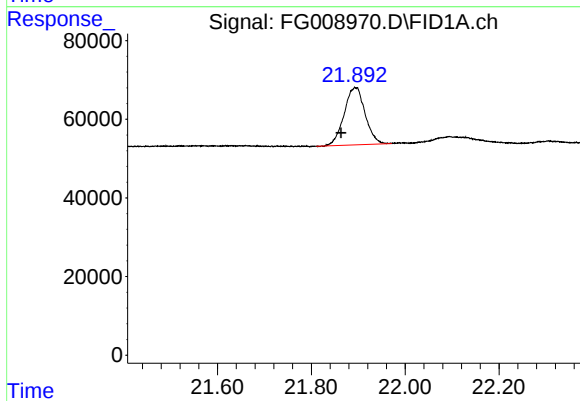

#18 N-TETRACONTANE

R.T.: 21.893 min
Delta R.T.: 0.029 min
Response: 451911
Conc: 5.12 ug/ml