

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110221\
Data File : FG008973.D
Signal(s) : FID1A.ch
Acq On : 02 Nov 2021 10:48
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:06:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.460	2414110	17.779 ug/ml
12)	N-OCTACOSANE	16.912	2474323	20.127 ug/ml
13)	N-TRIACONTANE	17.805	74465	0.636 ug/ml
14)	N-DOTRIACONTANE	18.637	91939	0.844 ug/ml
15)	N-TETRATRIACONTANE	19.420	77265	0.761 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110221\
Data File : FG008973.D
Signal(s) : FID1A.ch
Acq On : 02 Nov 2021 10:48
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 03 01:06:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

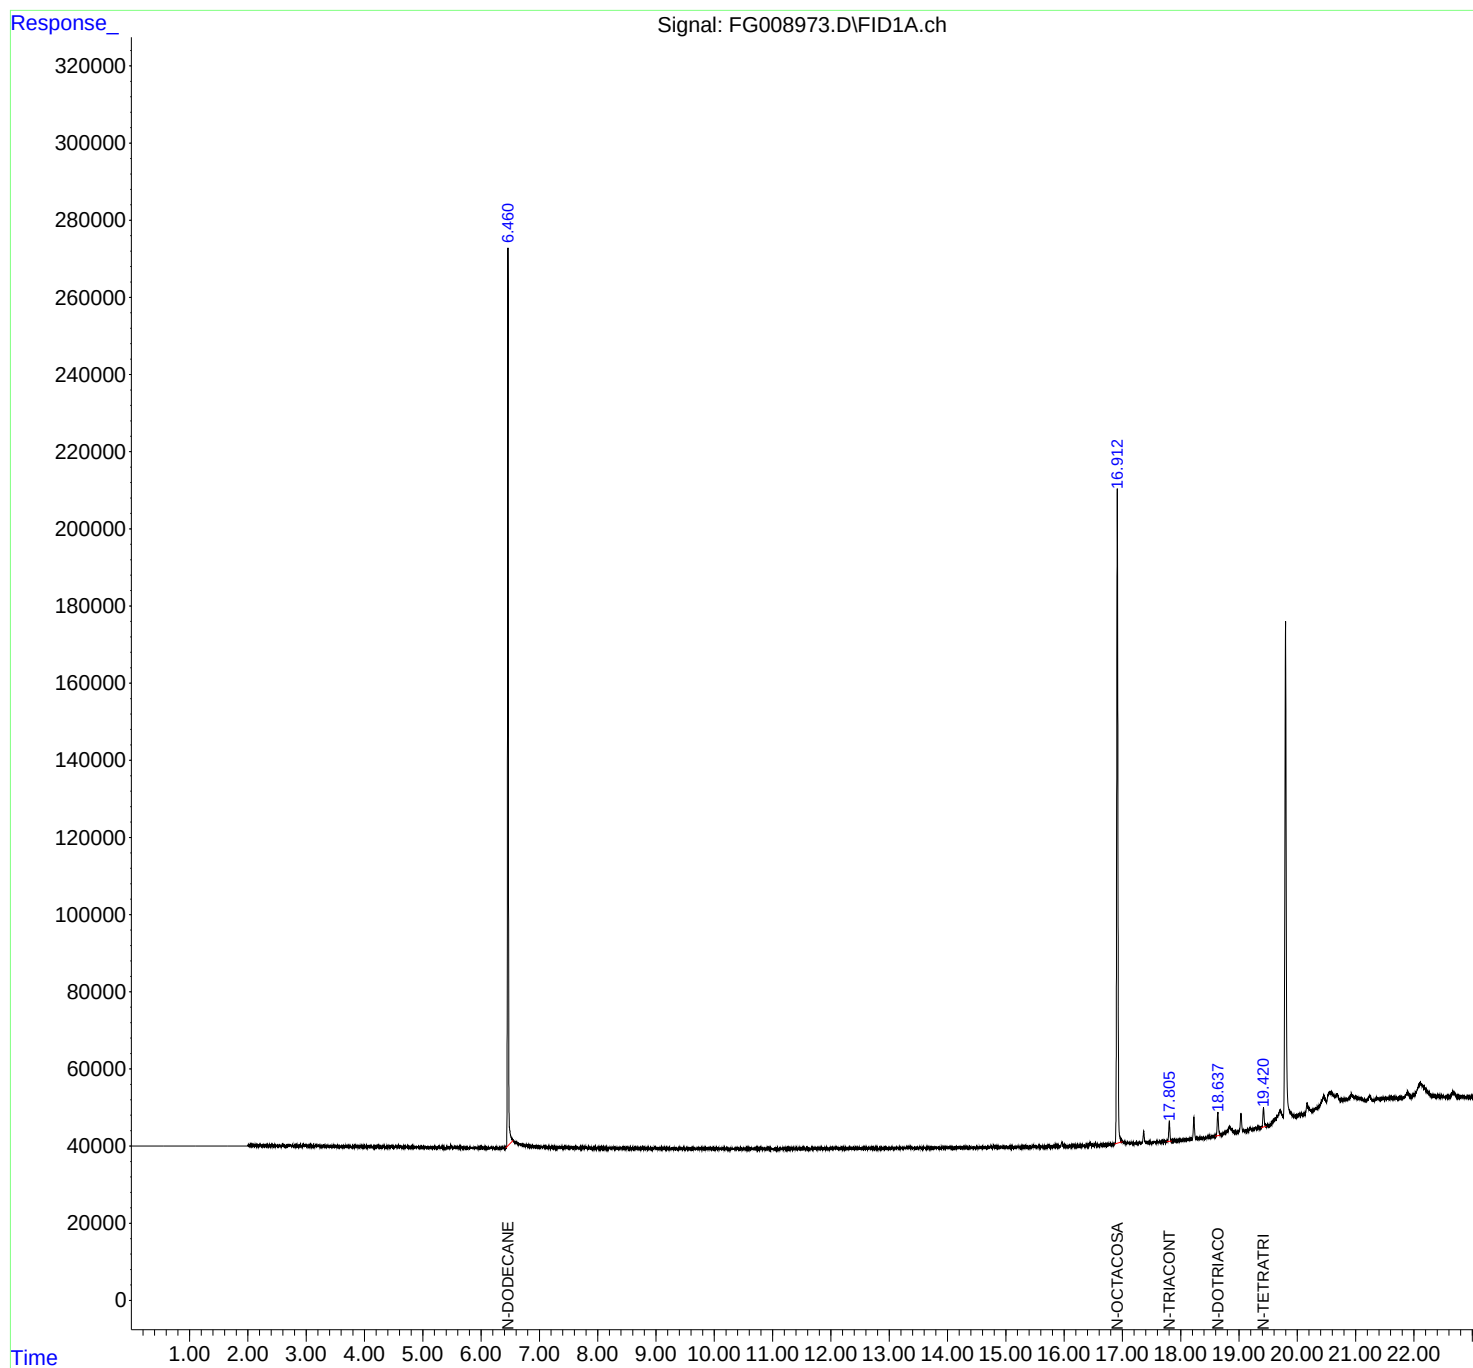


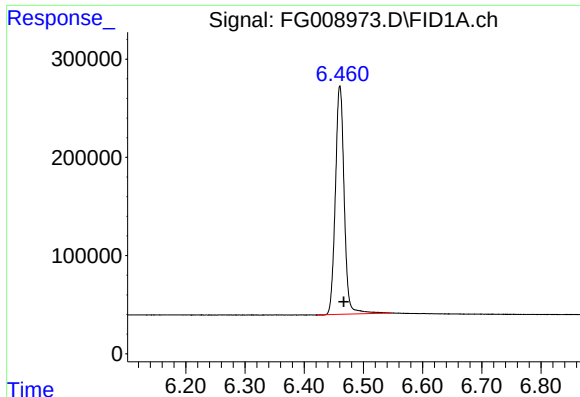

#3 N-DODECANE


R.T.: 6.460 min
Delta R.T.: -0.007 min
Response: 2414110
Conc: 17.78 ug/ml

Instrument :
FID_G
ClientSampleId :

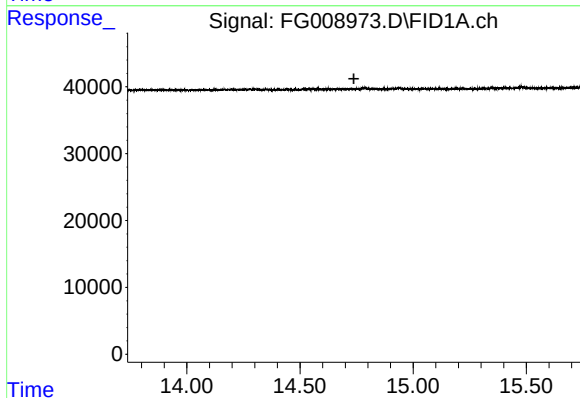


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.738 min
Response: 0
Conc: N.D.

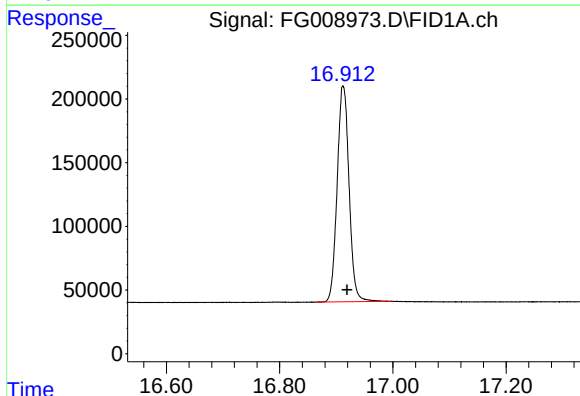


#12 N-OCTACOSANE

R.T.: 16.912 min
Delta R.T.: -0.007 min
Response: 2474323
Conc: 20.13 ug/ml

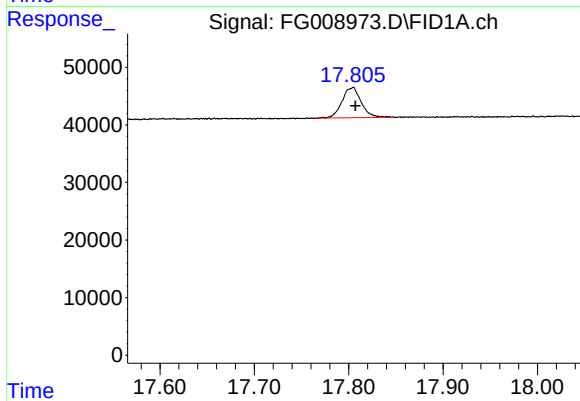

#13 N-TRIACONTANE


R.T.: 17.805 min
Delta R.T.: -0.002 min
Response: 74465
Conc: 0.64 ug/ml

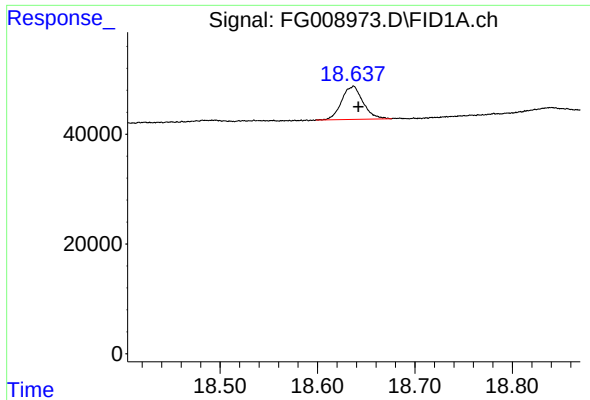

#14 N-DOTRIACONTANE

R.T.: 18.637 min
Delta R.T.: -0.005 min
Response: 91939
Conc: 0.84 ug/ml

Instrument :
FID_G
ClientSampleId :

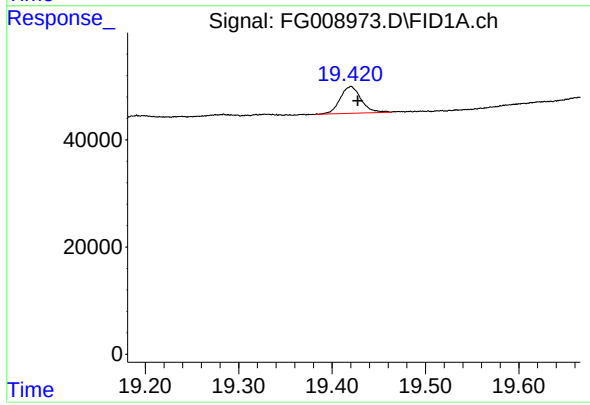

#15 N-TETRATRIACONTANE

R.T.: 19.420 min
Delta R.T.: -0.007 min
Response: 77265
Conc: 0.76 ug/ml