

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110221\
Data File : FG008981.D
Signal(s) : FID1A.ch
Acq On : 02 Nov 2021 10:48
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 03 01:06:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.460	2414110	17.779 ug/ml
12) N-OCTACOSANE	16.912	2474323	20.127 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110221\
Data File : FG008981.D
Signal(s) : FID1A.ch
Acq On : 02 Nov 2021 10:48
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 03 01:06:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

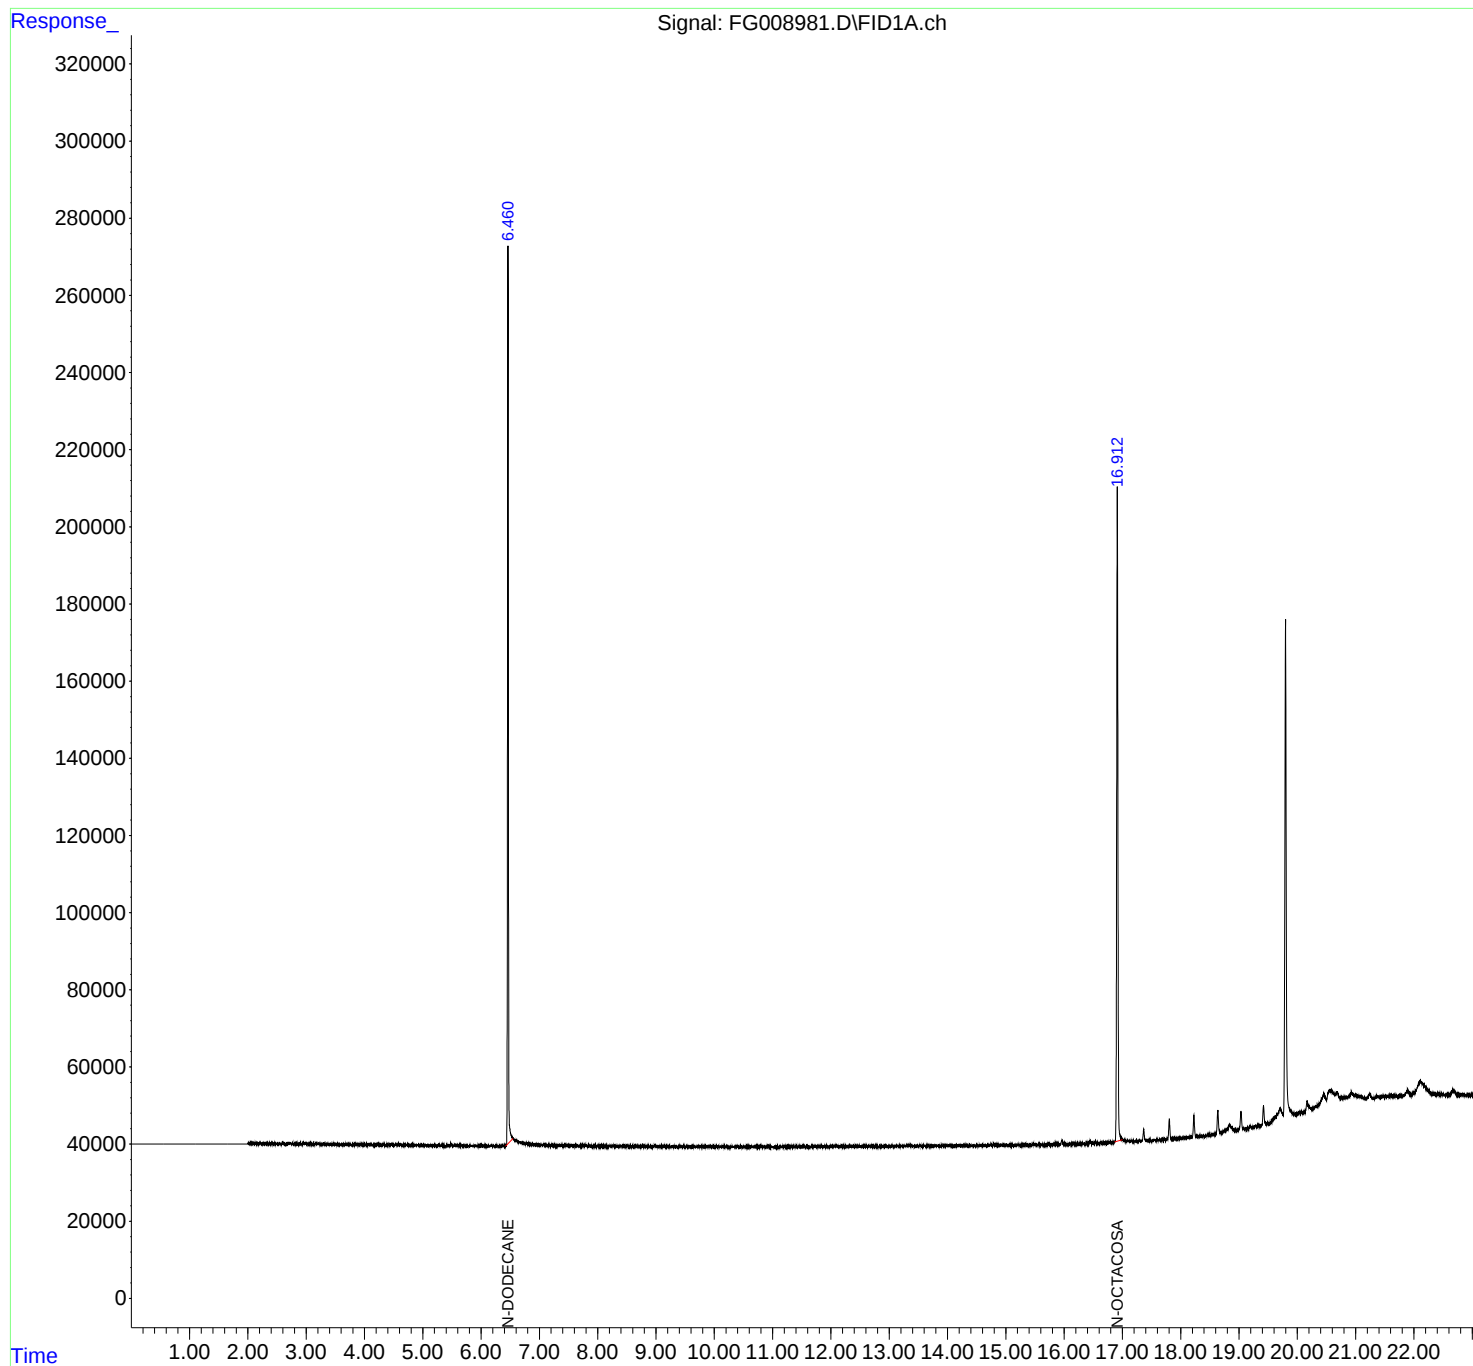


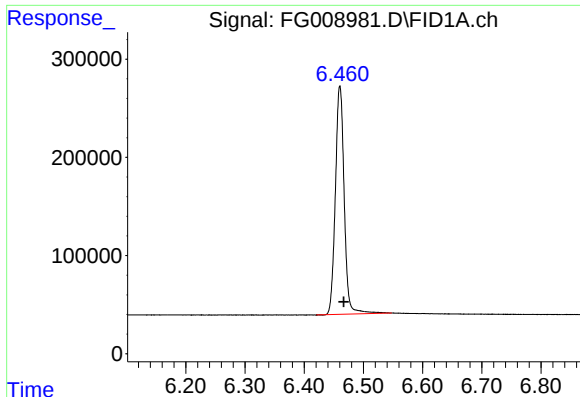

#3 N-DODECANE


R.T.: 6.460 min
Delta R.T.: -0.007 min
Response: 2414110
Conc: 17.78 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

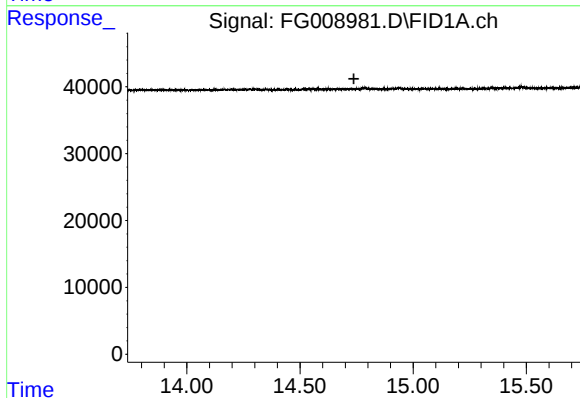

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.738 min
Response: 0
Conc: N.D.

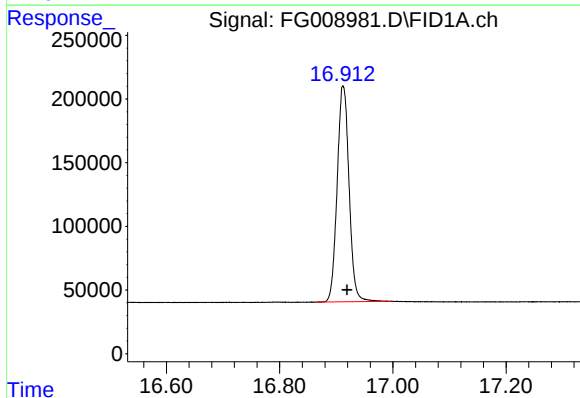

#12 N-OCTACOSANE

R.T.: 16.912 min
Delta R.T.: -0.007 min
Response: 2474323
Conc: 20.13 ug/ml