

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110221\
Data File : FG008985.D
Signal(s) : FID1A.ch
Acq On : 02 Nov 2021 13:05
Operator : AJ\MA
Sample : M4386-15 20X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PT-DIES-SOIL

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/03/2021
Supervised By :mohammad ahmed 11/05/2021

Integration File: autoint1.e
Quant Time: Nov 03 01:07:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.733	110053	0.954 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110221\
Data File : FG008985.D
Signal(s) : FID1A.ch
Acq On : 02 Nov 2021 13:05
Operator : AJ\MA
Sample : M4386-15 20X
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
PT-DIES-SOIL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/03/2021
Supervised By :mohammad ahmed 11/05/2021

Integration File: autoint1.e
Quant Time: Nov 03 01:07:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

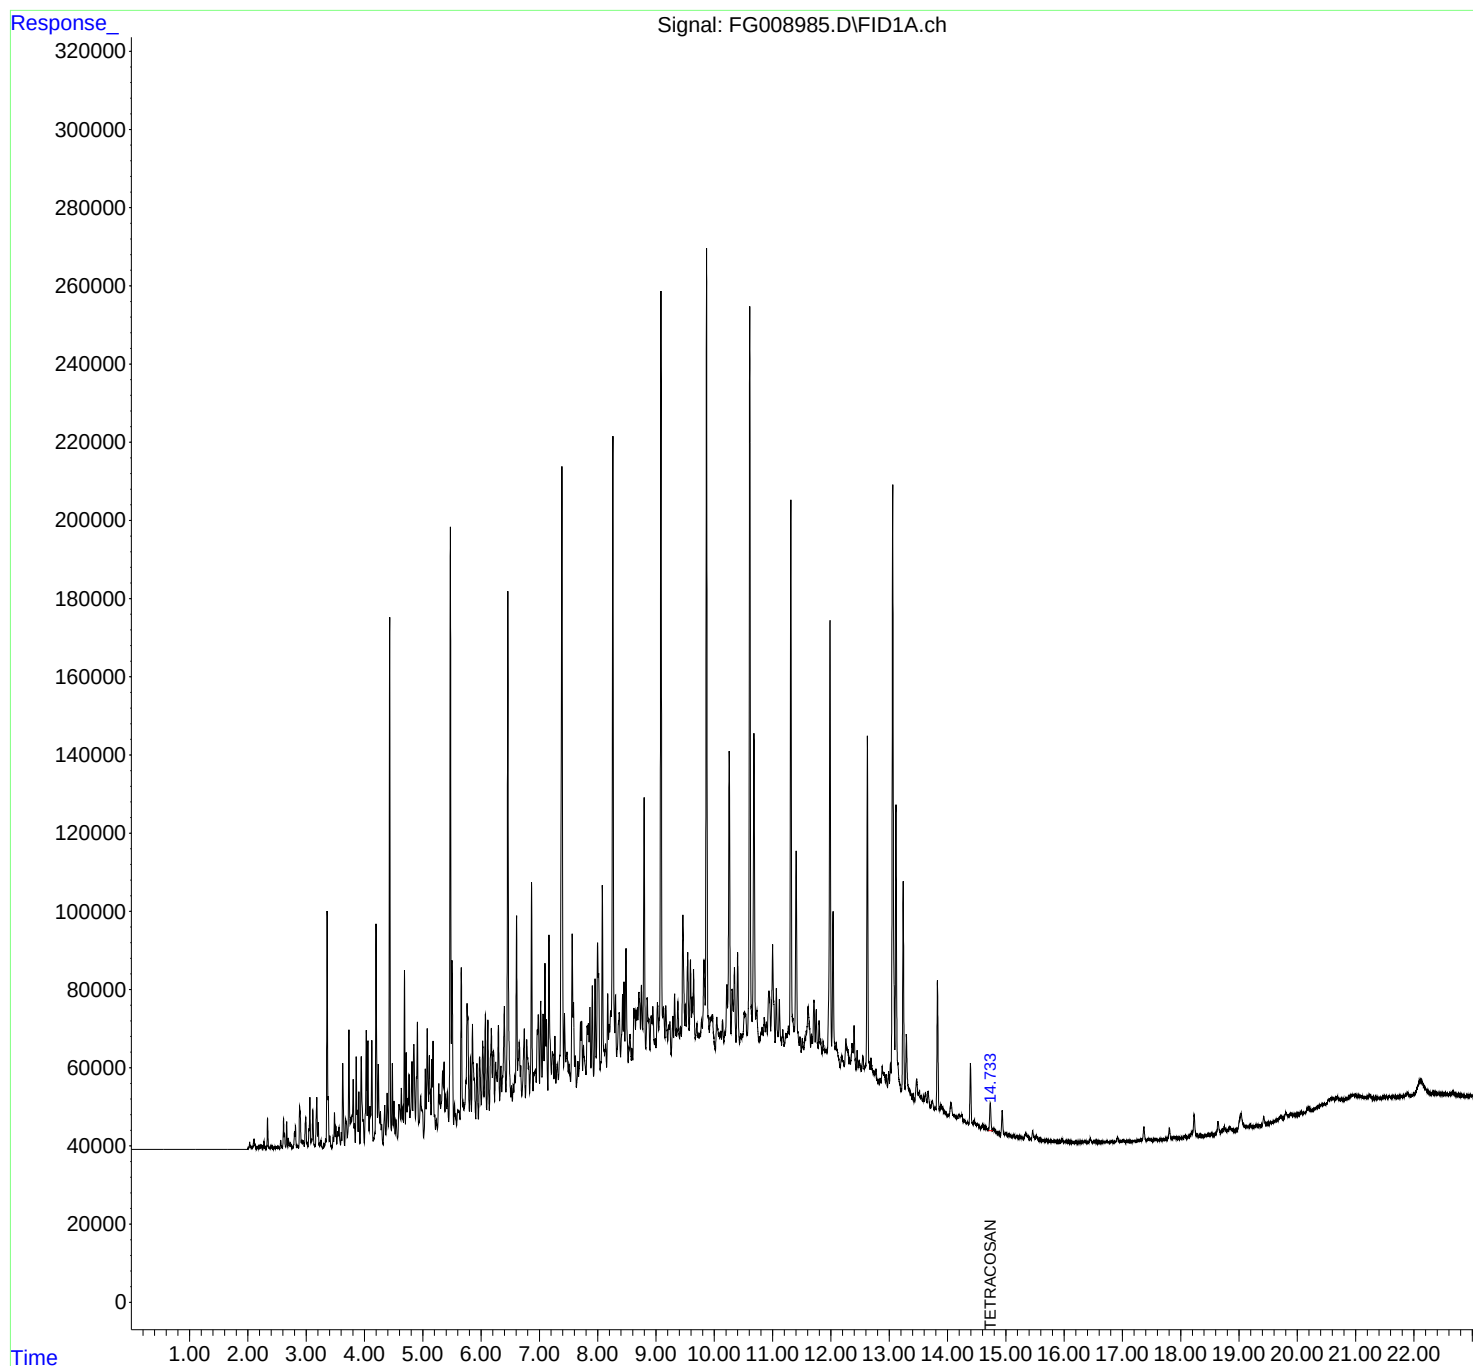

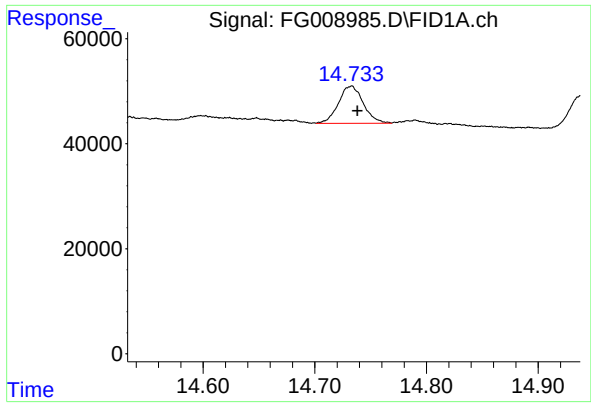

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.733 min
Delta R.T.: -0.006 min
Response: 110053
Conc: 0.95 ug/ml

Instrument :

FID_G

ClientSampleId :

PT-DIES-SOIL

Manual Integrations

APPROVED

Reviewed By :Ankita Jodhani 11/03/2021

Supervised By :mohammad ahmed 11/05/2021