

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110223\
 Data File : FG013130.D
 Signal(s) : FID1A.ch
 Acq On : 02 Nov 2023 15:04
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 02 23:08:38 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG101623.M
 Quant Title :
 QLast Update : Mon Oct 16 12:31:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.078	1764424	16.843 ug/ml
Target Compounds			
17) N-OCTATRIACONTANE	21.278	60785	0.859 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110223\
Data File : FG013130.D
Signal(s) : FID1A.ch
Acq On : 02 Nov 2023 15:04
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 02 23:08:38 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG101623.M
Quant Title :
QLast Update : Mon Oct 16 12:31:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

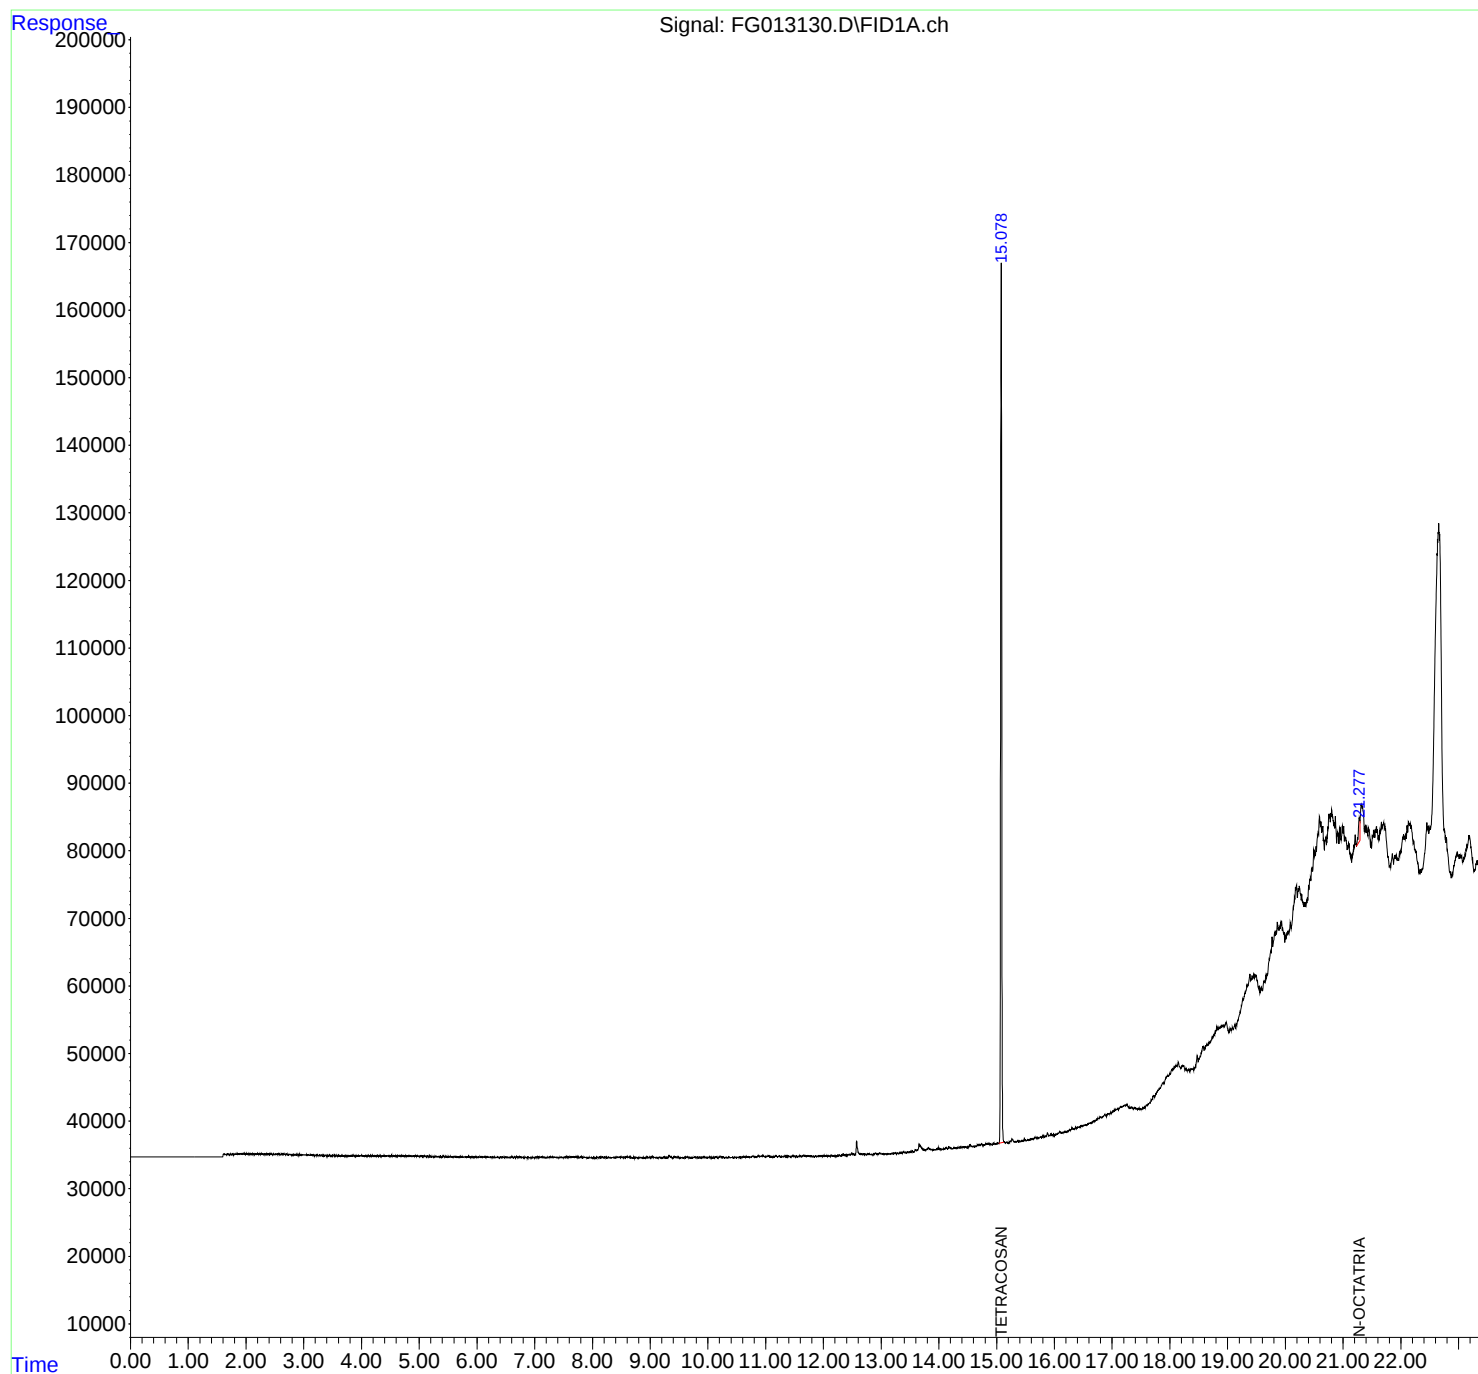


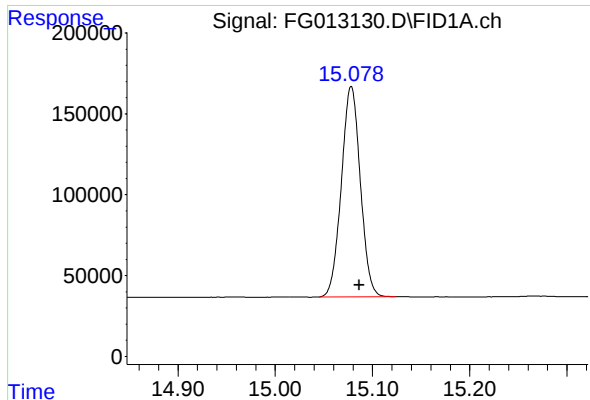

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.078 min
Delta R.T.: -0.009 min
Response: 1764424
Conc: 16.84 ug/ml

Instrument :
FID_G
ClientSampleId :

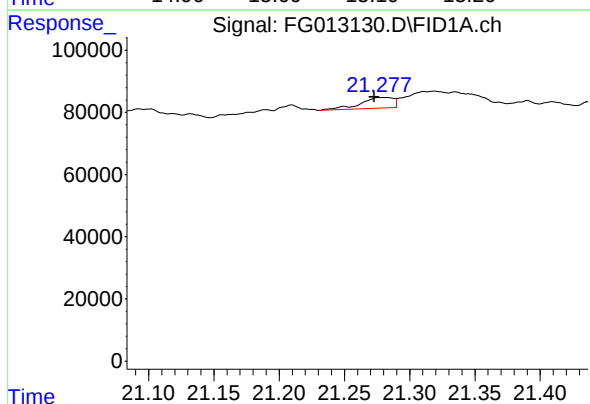

#17 N-OCTATRIACONTANE

R.T.: 21.278 min
Delta R.T.: 0.005 min
Response: 60785
Conc: 0.86 ug/ml