

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110223\
 Data File : FG013136.D
 Signal(s) : FID1A.ch
 Acq On : 02 Nov 2023 17:58
 Operator : YP\AJ
 Sample : 05172-01 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 AU-05-103123

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/03/2023
 Supervised By :mohammad ahmed 11/03/2023

Integration File: autoint1.e
 Quant Time: Nov 02 23:09:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG101623.M
 Quant Title :
 QLast Update : Mon Oct 16 12:31:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.082	355639	3.395 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110223\
Data File : FG013136.D
Signal(s) : FID1A.ch
Acq On : 02 Nov 2023 17:58
Operator : YP\AJ
Sample : 05172-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
AU-05-103123


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/03/2023
Supervised By :mohammad ahmed 11/03/2023

Integration File: autoint1.e
Quant Time: Nov 02 23:09:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG101623.M
Quant Title :
QLast Update : Mon Oct 16 12:31:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

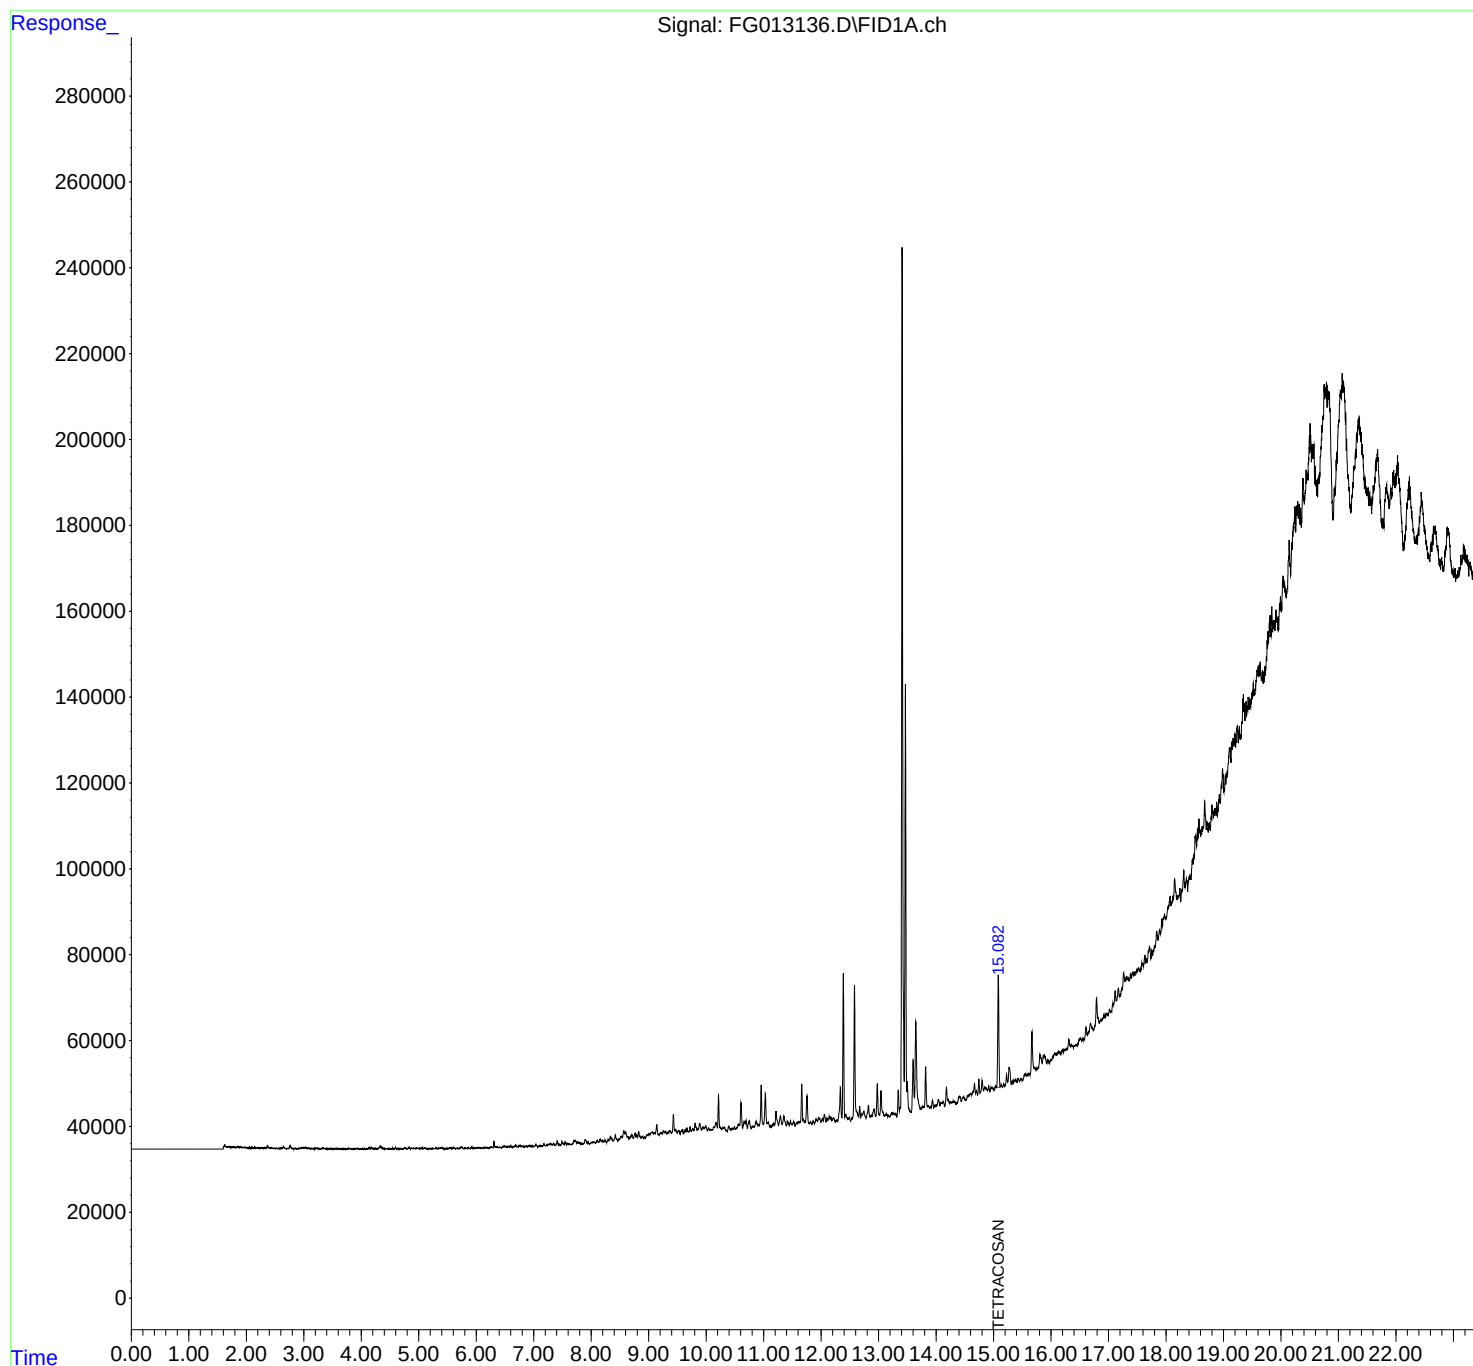

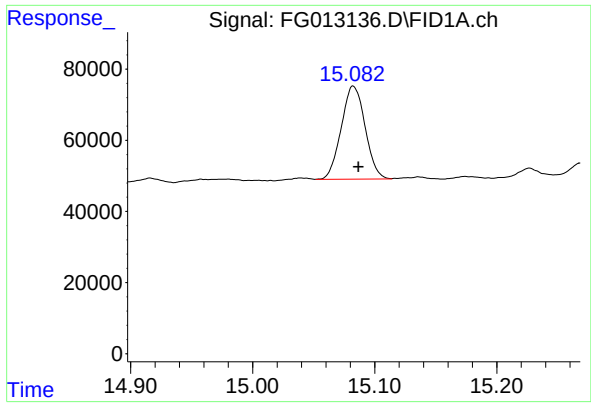

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.082 min
Delta R.T.: -0.005 min
Response: 355639
Conc: 3.39 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-05-103123

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/03/2023
Supervised By :mohammad ahmed 11/03/2023