

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110421\
 Data File : FG008991.D
 Signal(s) : FID1A.ch
 Acq On : 04 Nov 2021 10:59
 Operator : AJ\MA
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Nov 08 01:18:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
 Quant Title :
 QLast Update : Tue Nov 02 01:56:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.730	6324650	54.798 ug/ml
Target Compounds			
2) N-DECANE	4.434	7544708	55.798 ug/ml
3) N-DODECANE	6.461	7608304	56.033 ug/ml
4) N-TETRADECANE	8.263	7619237	57.367 ug/ml
5) N-HEXADECANE	9.867	7524925	56.763 ug/ml
6) N-OCTADECANE	11.313	7625069	55.612 ug/ml
7) N-EICOSANE	12.627	7546482	55.173 ug/ml
8) N-DOCOSANE	13.828	7348357	54.908 ug/ml
10) N-TETRACOSANE	14.935	7241639	54.823 ug/ml
11) N-HEXACOSANE	15.957	6967234	54.722 ug/ml
12) N-OCTACOSANE	16.910	6706706	54.554 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110421\
Data File : FG008991.D
Signal(s) : FID1A.ch
Acq On : 04 Nov 2021 10:59
Operator : AJ\MA
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Nov 08 01:18:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

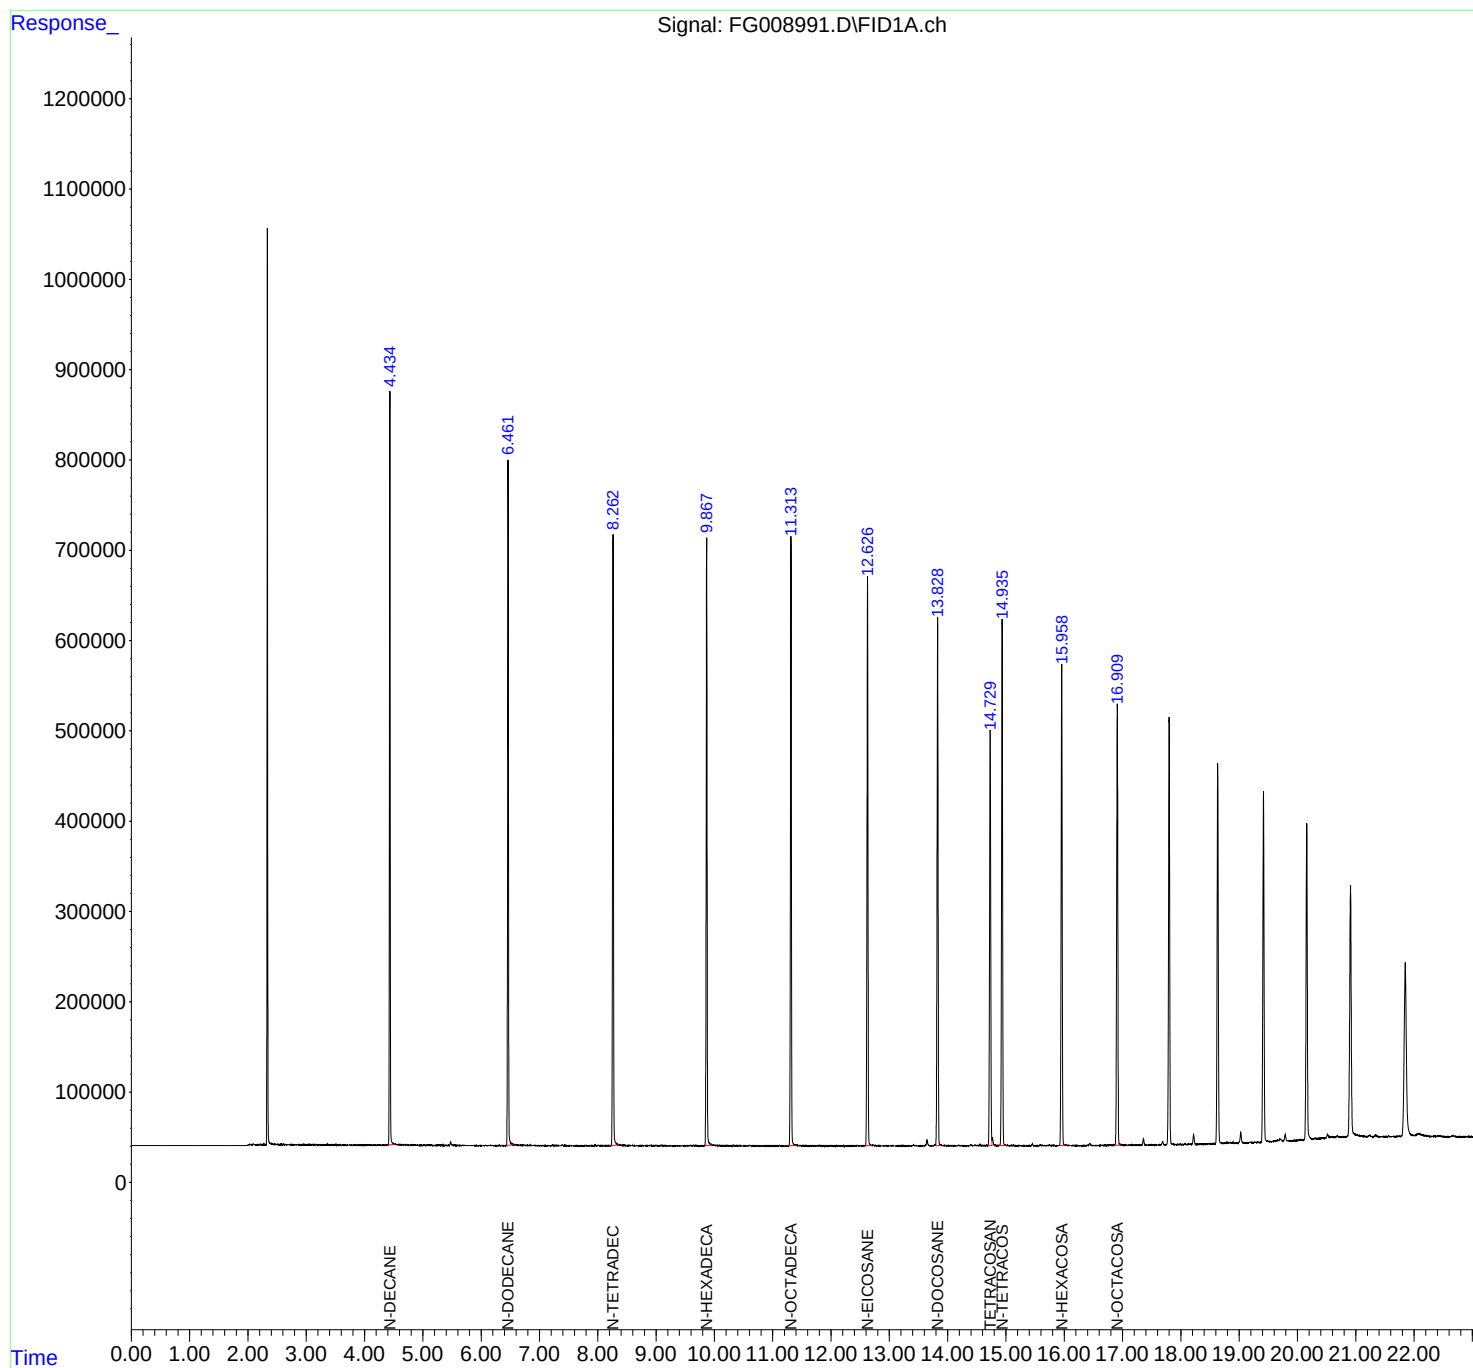

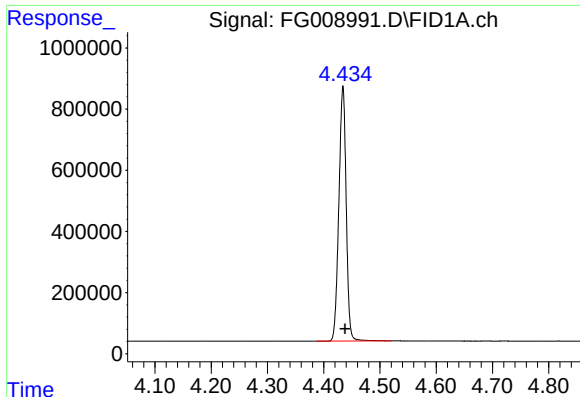


#2 N-DECANE

R.T.: 4.434 min
Delta R.T.: -0.003 min
Response: 7544708
Conc: 55.80 ug/ml

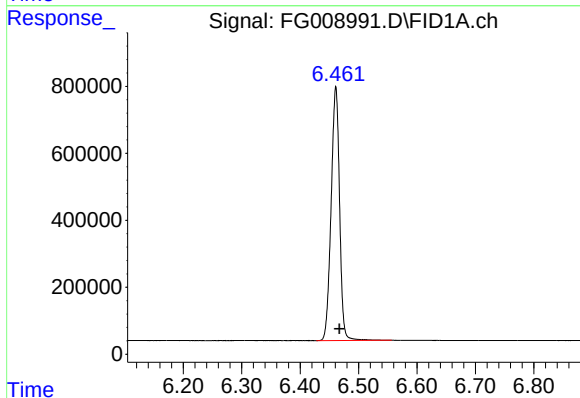


#3 N-DODECANE

R.T.: 6.461 min
Delta R.T.: -0.006 min
Response: 7608304
Conc: 56.03 ug/ml

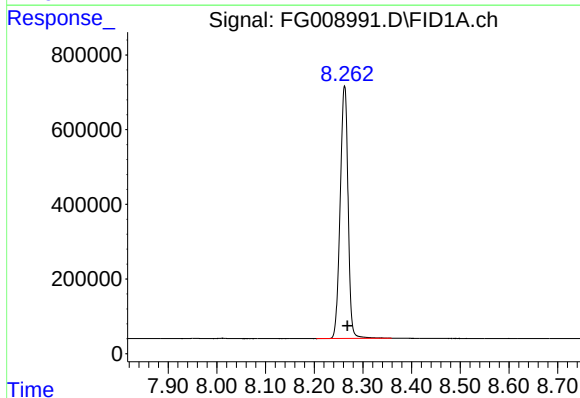


#4 N-TETRADECANE

R.T.: 8.263 min
Delta R.T.: -0.006 min
Response: 7619237
Conc: 57.37 ug/ml

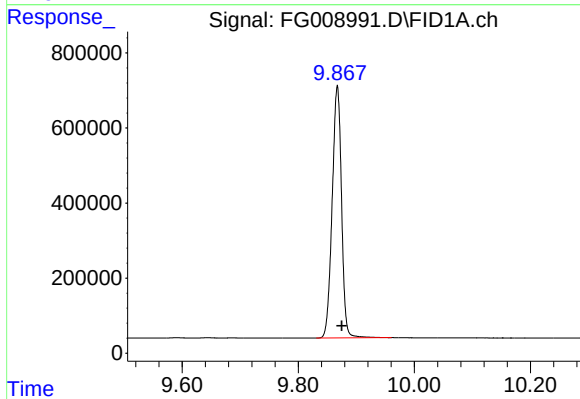


#5 N-HEXADECANE

R.T.: 9.867 min
Delta R.T.: -0.008 min
Response: 7524925
Conc: 56.76 ug/ml

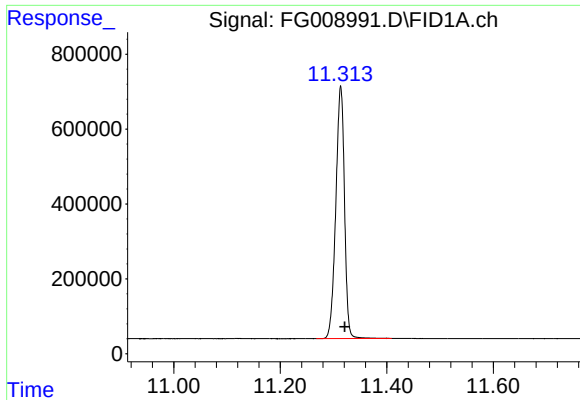


#6 N-OCTADECANE

R.T.: 11.313 min
Delta R.T.: -0.008 min
Response: 7625069
Conc: 55.61 ug/ml

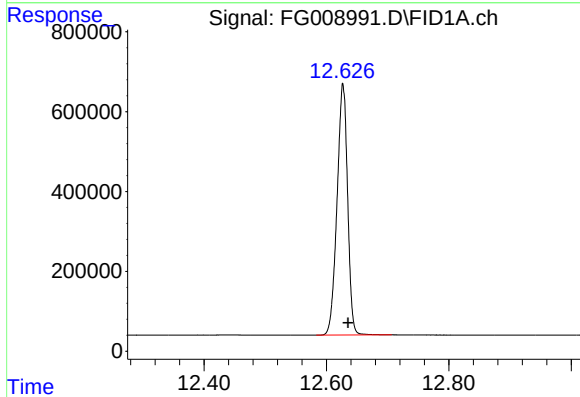


#7 N-EICOSANE

R.T.: 12.627 min
Delta R.T.: -0.009 min
Response: 7546482
Conc: 55.17 ug/ml

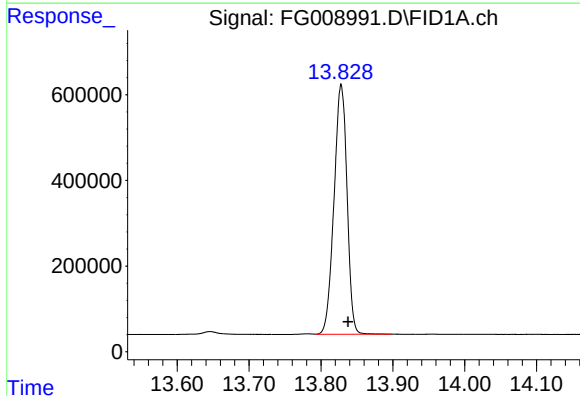


#8 N-DOCOSANE

R.T.: 13.828 min
Delta R.T.: -0.010 min
Response: 7348357
Conc: 54.91 ug/ml

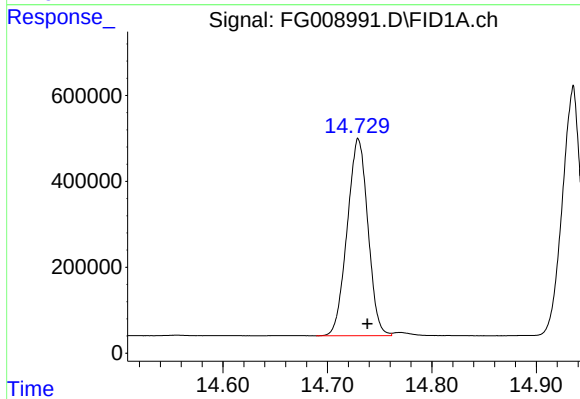


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.730 min
Delta R.T.: -0.009 min
Response: 6324650
Conc: 54.80 ug/ml

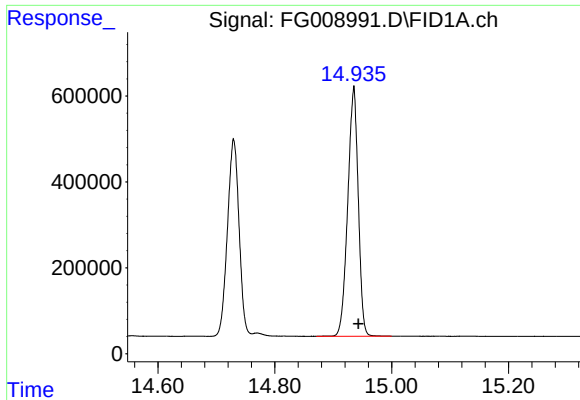


#10 N-TETRACOSANE

R.T.: 14.935 min
Delta R.T.: -0.008 min
Response: 7241639
Conc: 54.82 ug/ml

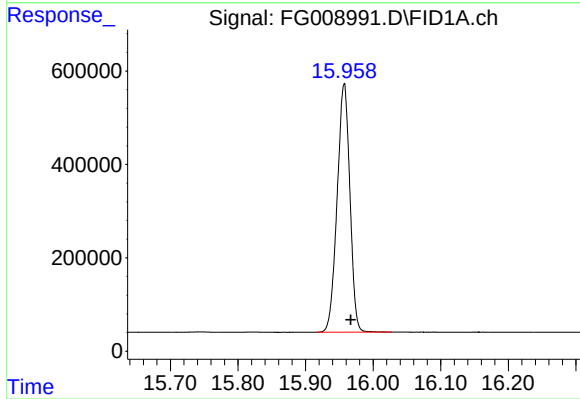

#11 N-HEXACOSANE

R.T.: 15.957 min
Delta R.T.: -0.010 min
Response: 6967234
Conc: 54.72 ug/ml

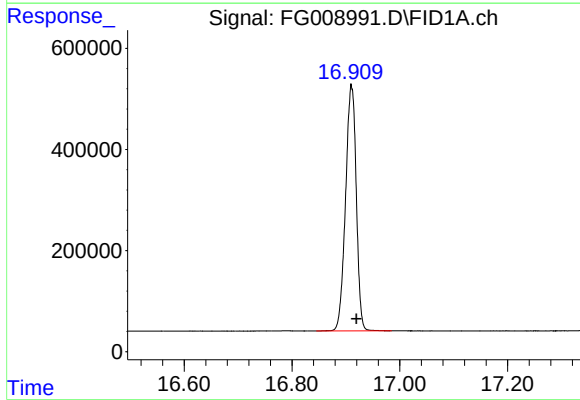

#12 N-OCTACOSANE

R.T.: 16.910 min
Delta R.T.: -0.009 min
Response: 6706706
Conc: 54.55 ug/ml