

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110618\
 Data File : FG002781.D
 Signal(s) : FID1A.ch
 Acq On : 06 Nov 2018 21:35
 Operator : AJ\SJ
 Sample : 4400 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 07 10:21:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
 Quant Title :
 QLast Update : Wed Nov 07 10:15:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.764	5795733	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.359	43681490	400.000 ug/ml
2) N-NONANE	3.400	44124273	400.000 ug/ml
3) N-DECANE	4.489	65947041	400.000 ug/ml
4) N-UNDECANE	5.535	68635669	600.000 ug/ml
5) N-DODECANE	6.521	67411508	600.000 ug/ml
6) N-TETRADECANE	8.322	65605245	600.000 ug/ml
7) N-HEXADECANE	9.925	54872306	500.000 ug/ml
8) N-OCTADECANE	11.360	27024999	250.000 ug/ml
9) N-EICOSANE	12.663	10681247	100.000 ug/ml
10) N-TETRACOSANE	14.971	9890832	100.000 ug/ml
11) N-OCTACOSANE	16.943	4580880	50.000 ug/ml
12) N-DOTRIACONTANE	18.667	3923185	50.000 ug/ml
14) N-HEXATRIACONTANE	20.194	3095777	50.000 ug/ml
15) N-TETRACONTANE	21.914	2112572	50.000 ug/ml
16) N-TETRTETRACOOCTANE	24.828	1388179	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110618\
Data File : FG002781.D
Signal(s) : FID1A.ch
Acq On : 06 Nov 2018 21:35
Operator : AJ\SJ
Sample : 4400 TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 10:21:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
Quant Title :
QLast Update : Wed Nov 07 10:15:21 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

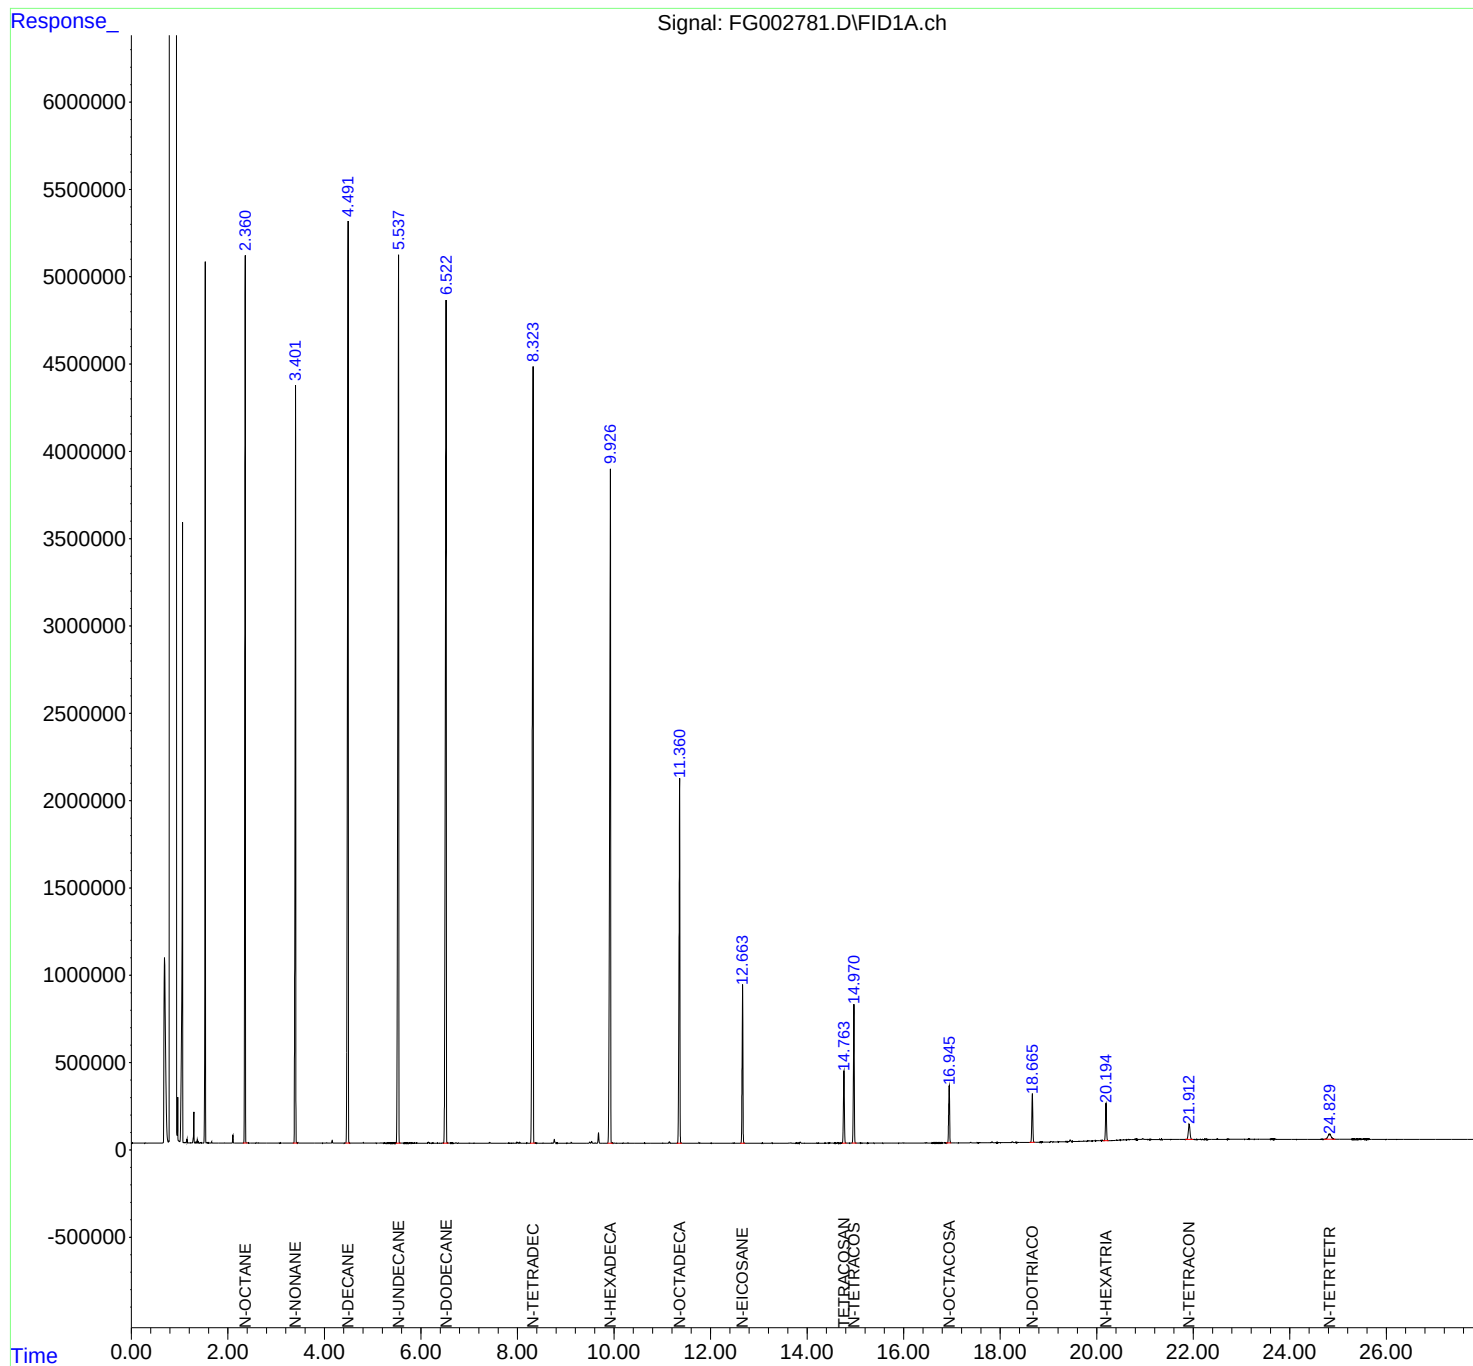

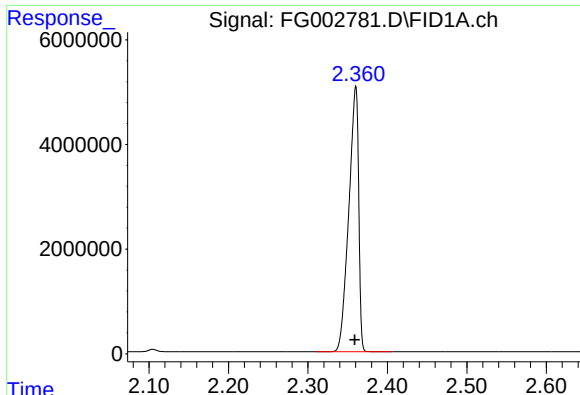


#1 N-OCTANE

R.T.: 2.359 min
Delta R.T.: 0.000 min
Response: 43681490
Conc: 400.00 ug/ml

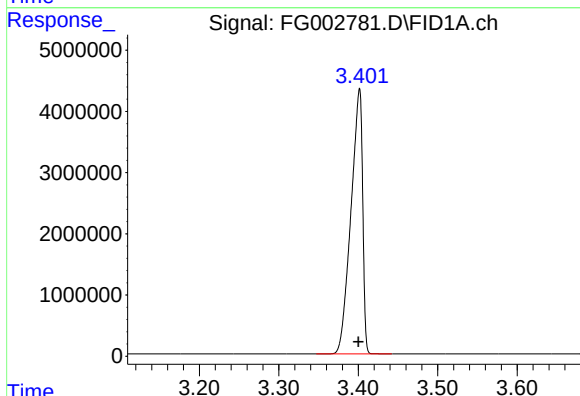


#2 N-NONANE

R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 44124273
Conc: 400.00 ug/ml

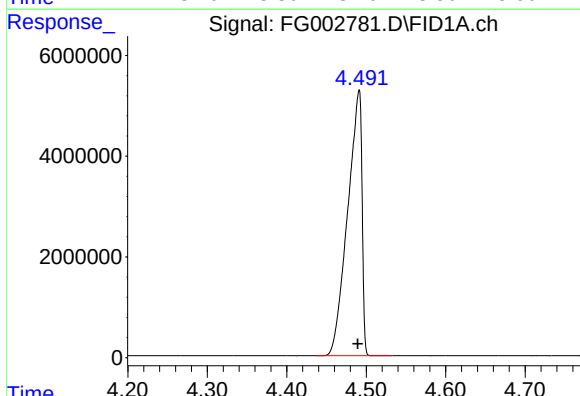


#3 N-DECANE

R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 65947041
Conc: 400.00 ug/ml

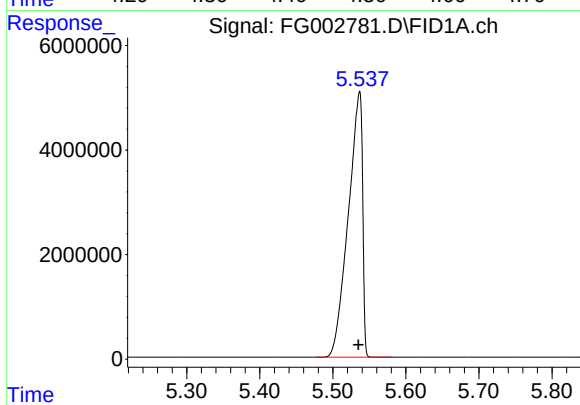


#4 N-UNDECANE

R.T.: 5.535 min
Delta R.T.: 0.000 min
Response: 68635669
Conc: 600.00 ug/ml

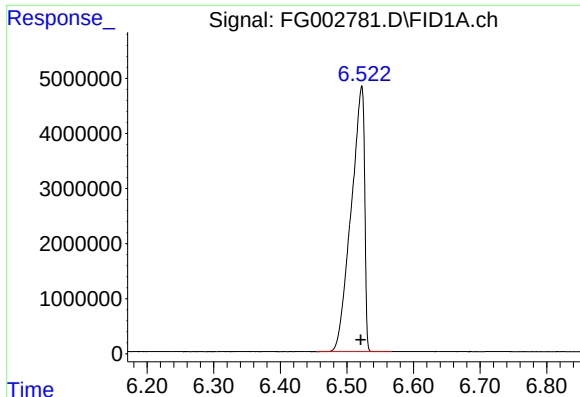


#5 N-DODECANE

R.T.: 6.521 min
Delta R.T.: 0.000 min
Response: 67411508
Conc: 600.00 ug/ml

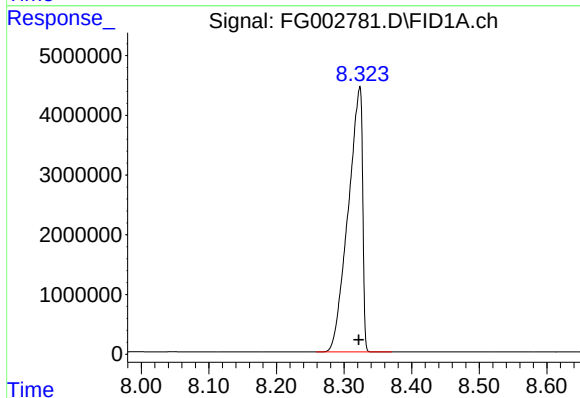


#6 N-TETRADECANE

R.T.: 8.322 min
Delta R.T.: 0.000 min
Response: 65605245
Conc: 600.00 ug/ml

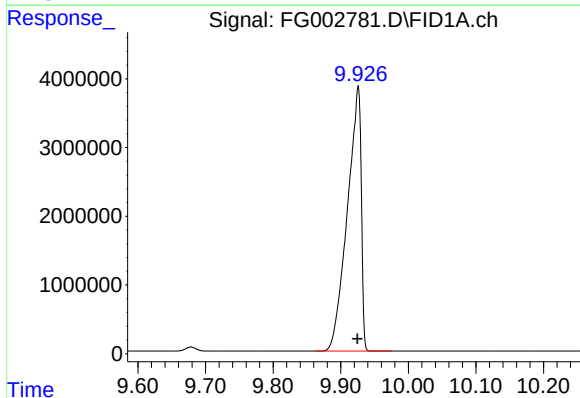


#7 N-HEXADECANE

R.T.: 9.925 min
Delta R.T.: 0.000 min
Response: 54872306
Conc: 500.00 ug/ml

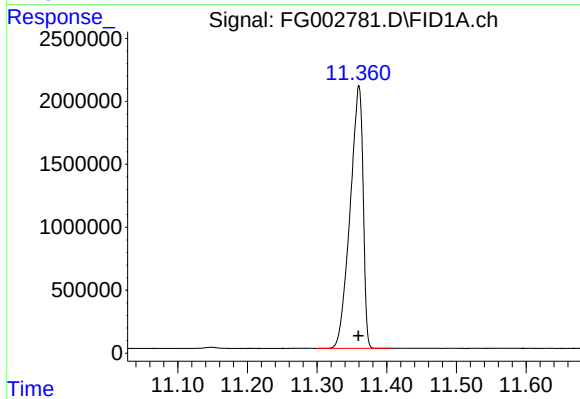


#8 N-OCTADECANE

R.T.: 11.360 min
Delta R.T.: 0.000 min
Response: 27024999
Conc: 250.00 ug/ml

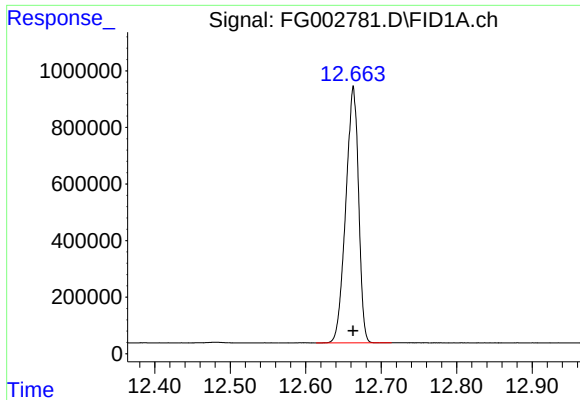


#9 N-EICOSANE

R.T.: 12.663 min
Delta R.T.: 0.000 min
Response: 10681247
Conc: 100.00 ug/ml

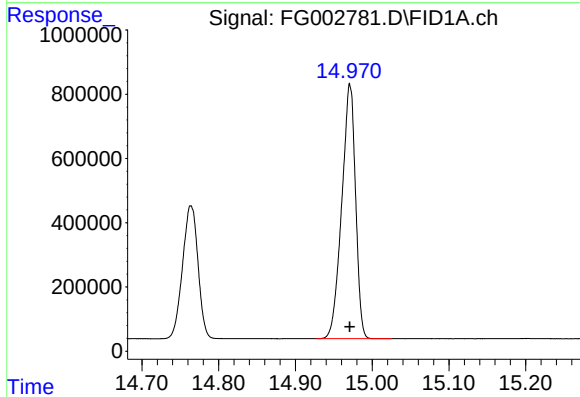


#10 N-TETRACOSANE

R.T.: 14.971 min
Delta R.T.: 0.000 min
Response: 9890832
Conc: 100.00 ug/ml

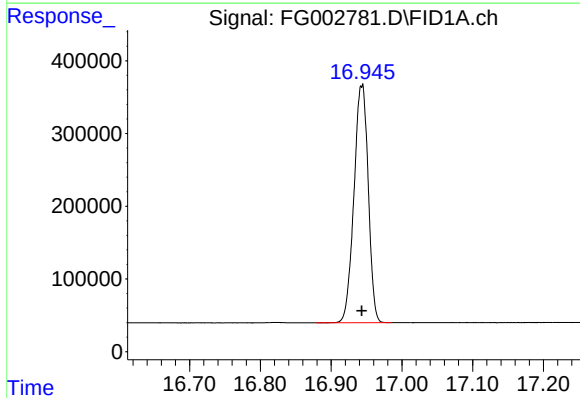


#11 N-OCTACOSANE

R.T.: 16.943 min
Delta R.T.: 0.000 min
Response: 4580880
Conc: 50.00 ug/ml

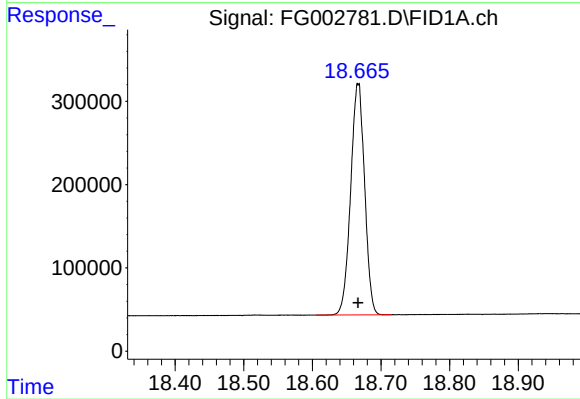


#12 N-DOTRIACONTANE

R.T.: 18.667 min
Delta R.T.: 0.000 min
Response: 3923185
Conc: 50.00 ug/ml

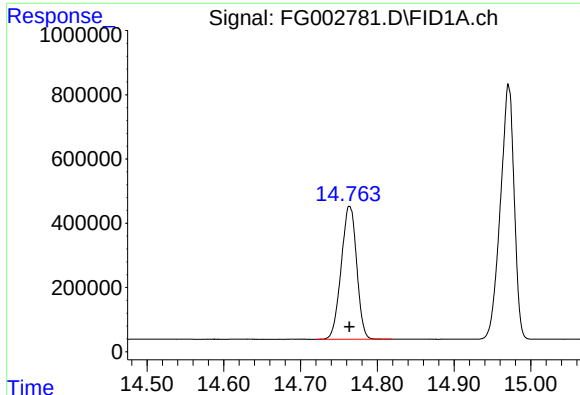


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.764 min
Delta R.T.: 0.000 min
Response: 5795733
Conc: 50.00 ug/ml

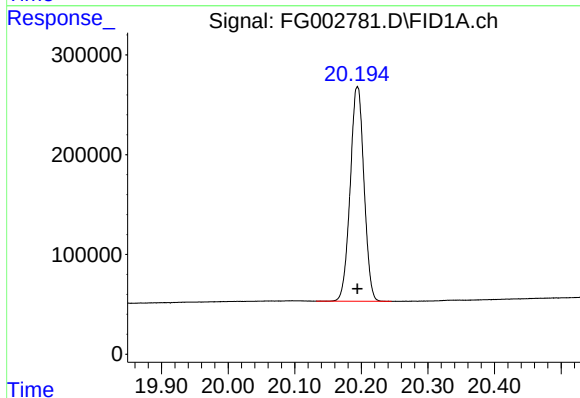


#14 N-HEXATRIACONTANE

R.T.: 20.194 min
Delta R.T.: 0.000 min
Response: 3095777
Conc: 50.00 ug/ml

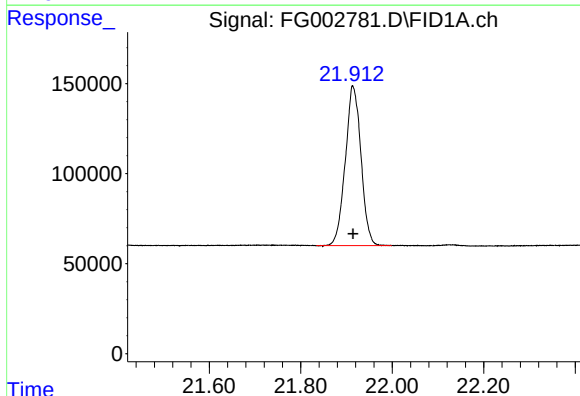

#15 N-TETRACONTANE

R.T.: 21.914 min
Delta R.T.: 0.000 min
Response: 2112572
Conc: 50.00 ug/ml

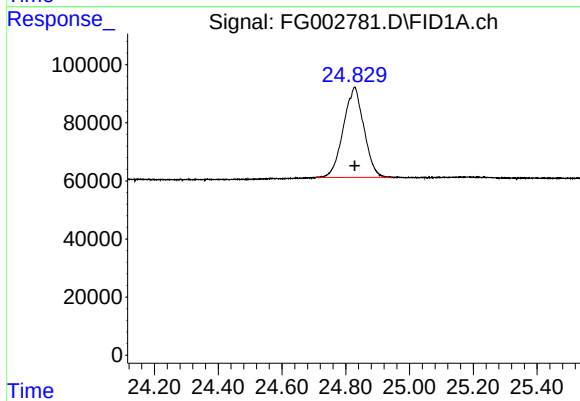

#16 N-TETRTETRACOOCTANE

R.T.: 24.828 min
Delta R.T.: 0.000 min
Response: 1388179
Conc: 50.00 ug/ml