

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110618\
 Data File : FG002790.D
 Signal(s) : FID1A.ch
 Acq On : 07 Nov 2018 02:50
 Operator : AJ\SJ
 Sample : J5827-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 07 10:41:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
 Quant Title :
 QLast Update : Wed Nov 07 10:34:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.759	1893804	15.410 ug/ml
Target Compounds			
6) N-TETRADECANE	8.354	731480	6.401 ug/ml
9) N-EICOSANE	12.720	846493	7.498 ug/ml
10) N-TETRACOSANE	14.945	453707	4.318 ug/ml
11) N-OCTACOSANE	16.942	547052	5.545 ug/ml
12) N-DOTRIACONTANE	18.666	505170	5.881 ug/ml
14) N-HEXATRIACONTANE	20.220	848814	12.805 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110618\
Data File : FG002790.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2018 02:50
Operator : AJ\SJ
Sample : J5827-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 10:41:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
Quant Title :
QLast Update : Wed Nov 07 10:34:24 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

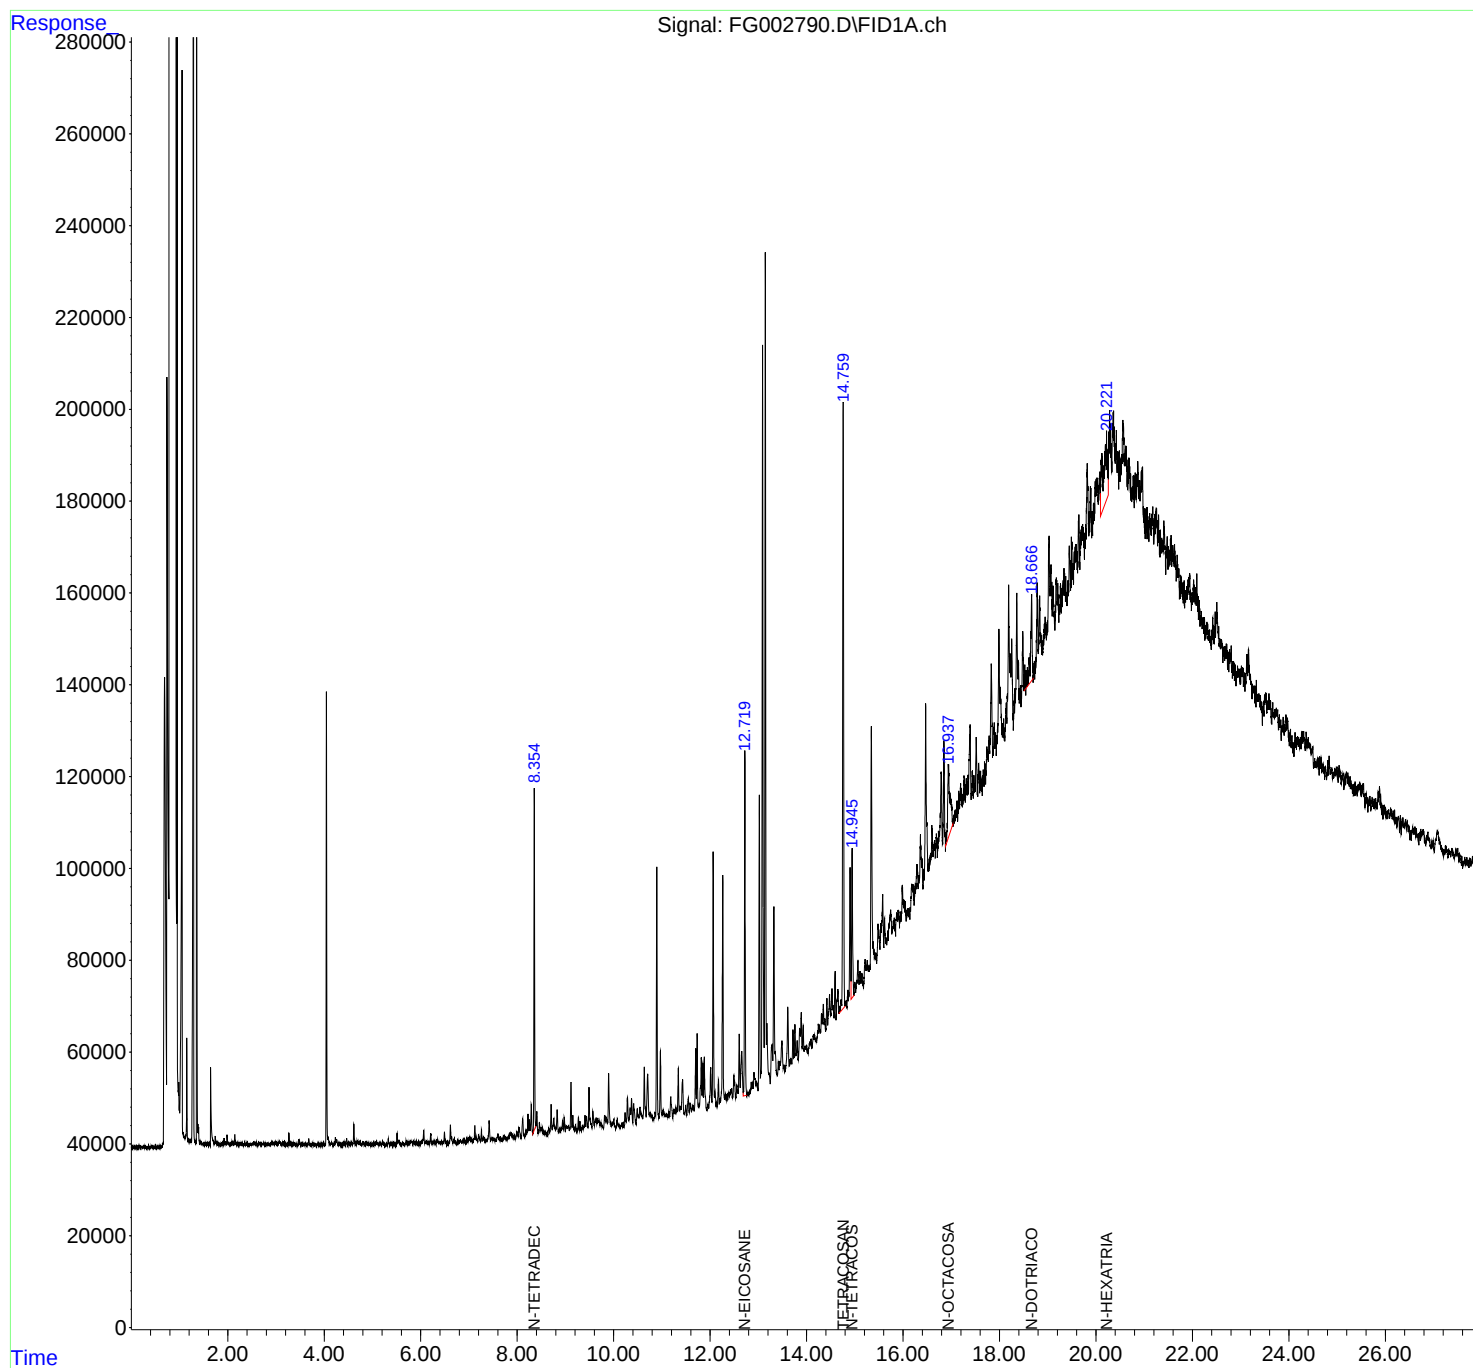

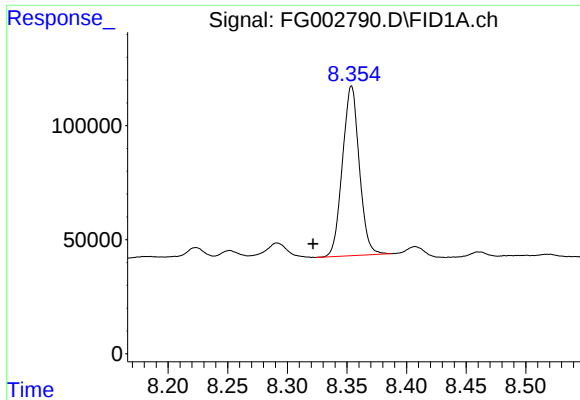


#6 N-TETRADECANE

R.T.: 8.354 min
Delta R.T.: 0.032 min
Response: 731480
Conc: 6.40 ug/ml

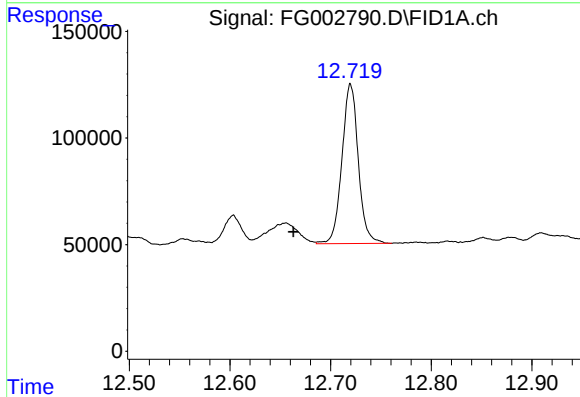


#9 N-EICOSANE

R.T.: 12.720 min
Delta R.T.: 0.057 min
Response: 846493
Conc: 7.50 ug/ml

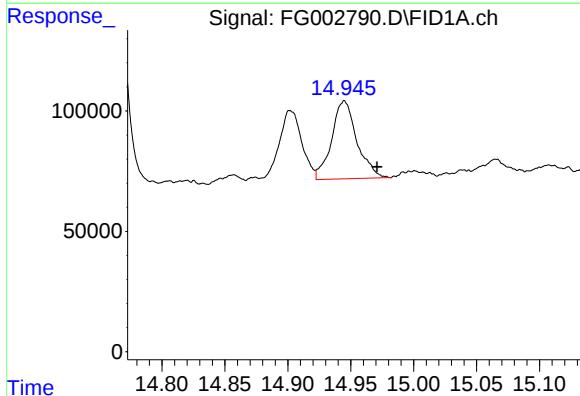


#10 N-TETRACOSANE

R.T.: 14.945 min
Delta R.T.: -0.026 min
Response: 453707
Conc: 4.32 ug/ml

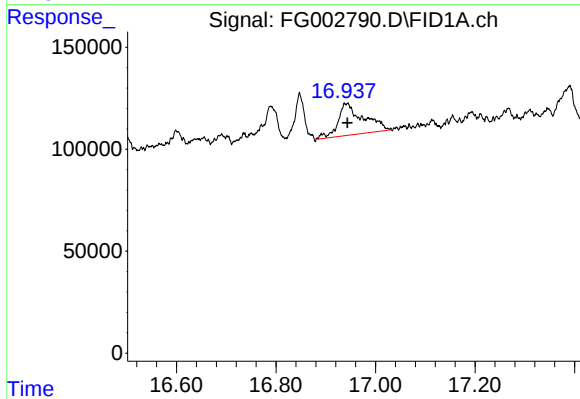


#11 N-OCTACOSANE

R.T.: 16.942 min
Delta R.T.: -0.002 min
Response: 547052
Conc: 5.54 ug/ml

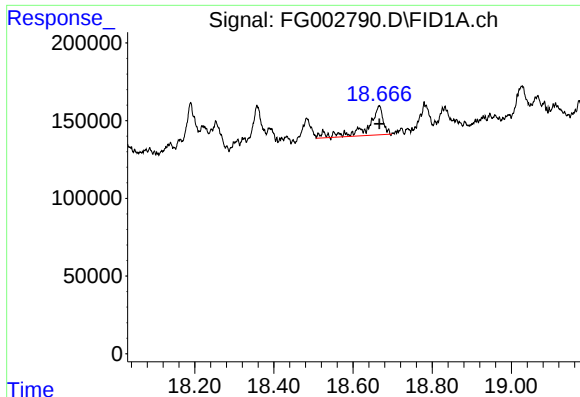


#12 N-DOTRIACONTANE

R.T.: 18.666 min
Delta R.T.: 0.000 min
Response: 505170
Conc: 5.88 ug/ml

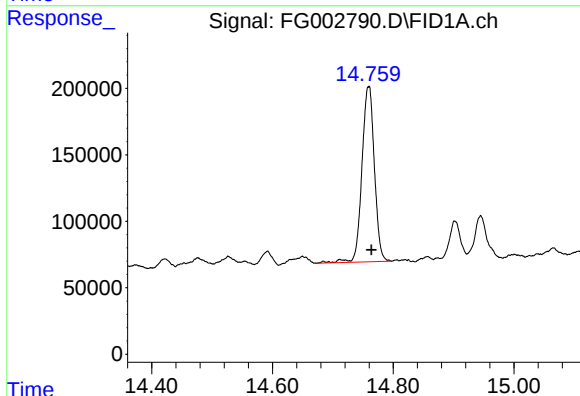

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.759 min
Delta R.T.: -0.005 min
Response: 1893804
Conc: 15.41 ug/ml

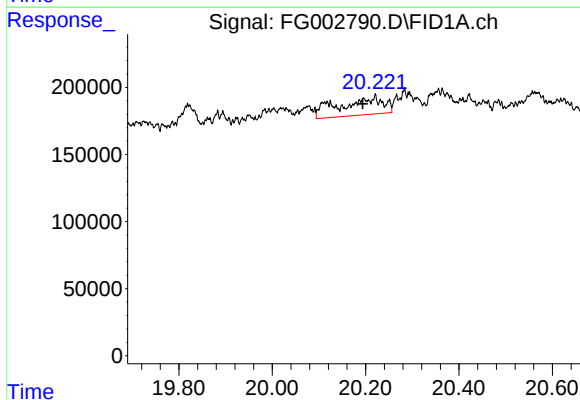

#14 N-HEXATRIACONTANE

R.T.: 20.220 min
Delta R.T.: 0.026 min
Response: 848814
Conc: 12.80 ug/ml