

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110618\
 Data File : FG002793.D
 Signal(s) : FID1A.ch
 Acq On : 07 Nov 2018 04:35
 Operator : AJ\SJ
 Sample : J5827-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 07 10:41:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
 Quant Title :
 QLast Update : Wed Nov 07 10:34:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.760	1493650	12.154 ug/ml
Target Compounds			
6) N-TETRADECANE	8.356	731854	6.404 ug/ml
9) N-EICOSANE	12.722	234228	2.075 ug/ml
10) N-TETRACOSANE	14.949	262600	2.499 ug/ml
11) N-OCTACOSANE	16.941	175321	1.777 ug/ml
12) N-DOTRIACONTANE	18.667	479898	5.587 ug/ml
14) N-HEXATRIACONTANE	20.196	340297	5.134 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110618\
Data File : FG002793.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2018 04:35
Operator : AJ\SJ
Sample : J5827-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 10:41:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
Quant Title :
QLast Update : Wed Nov 07 10:34:24 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

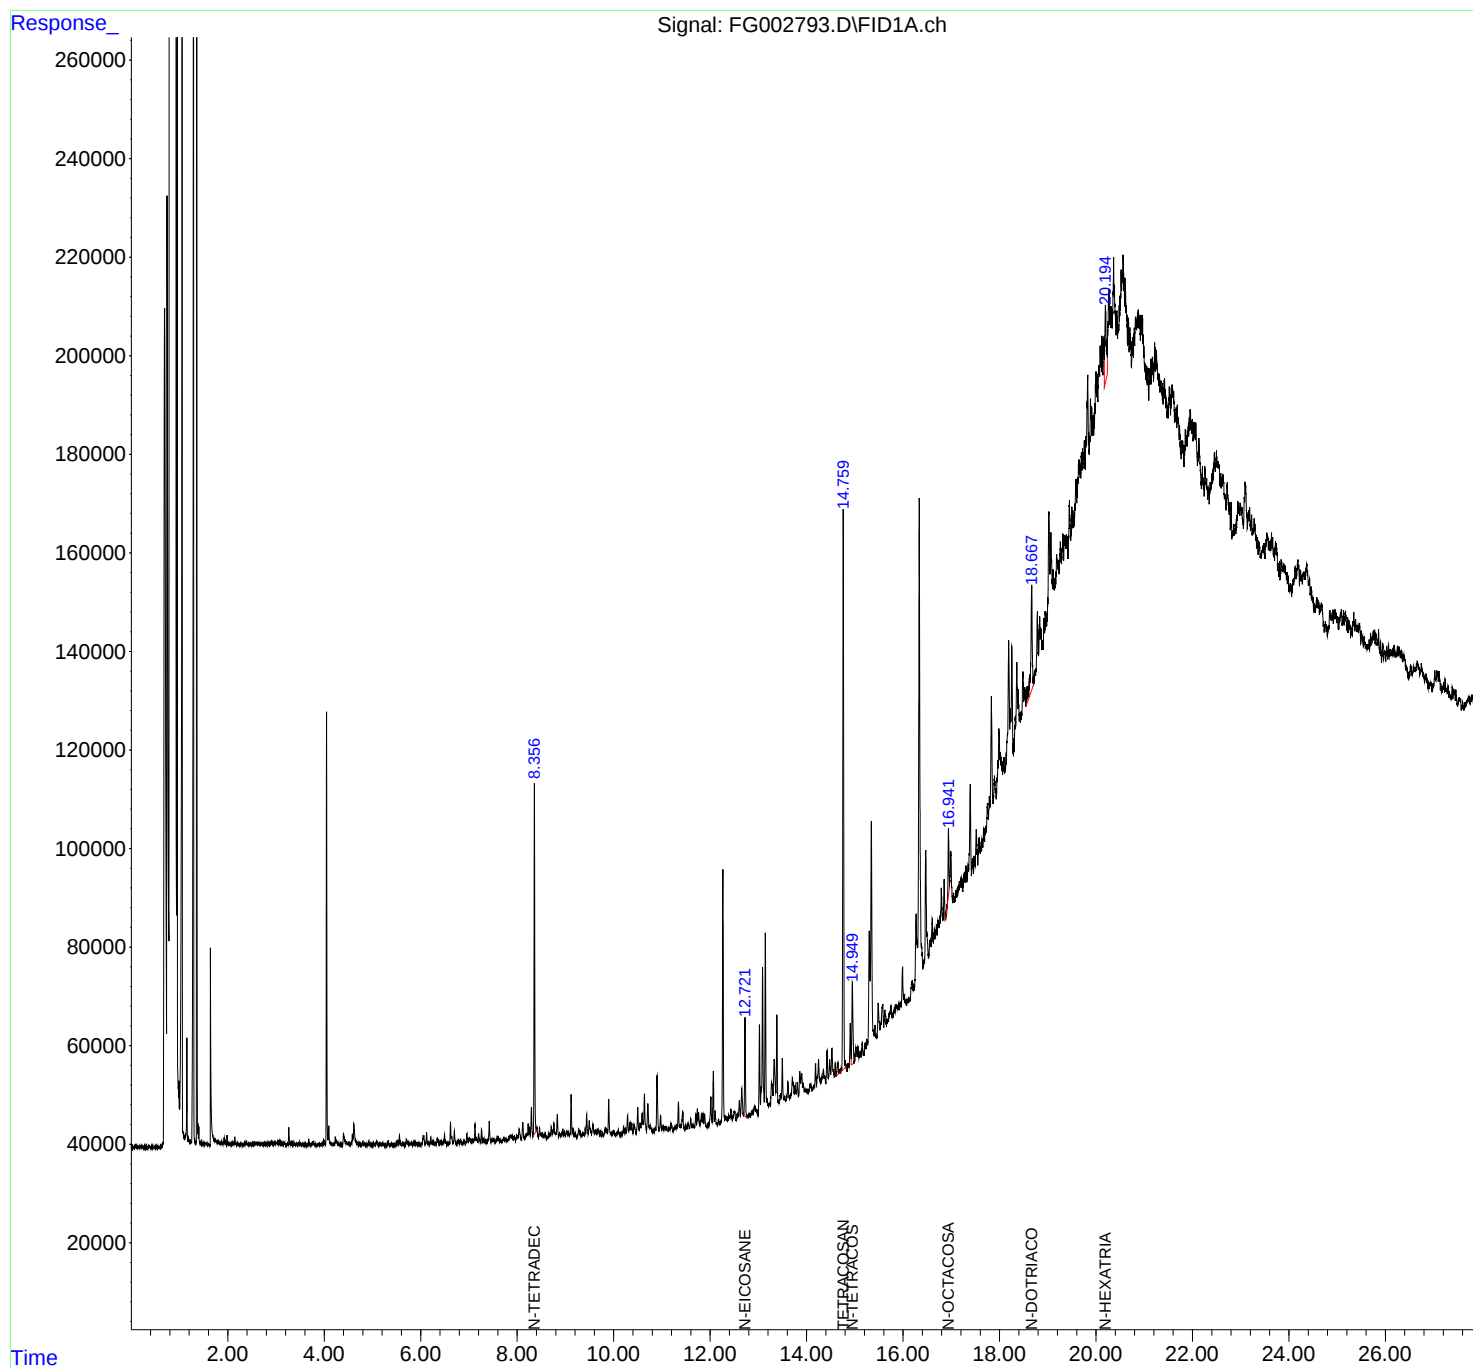

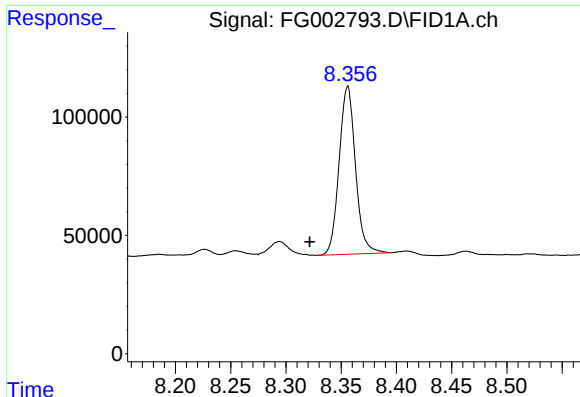


#6 N-TETRADECANE

R.T.: 8.356 min
Delta R.T.: 0.034 min
Response: 731854
Conc: 6.40 ug/ml

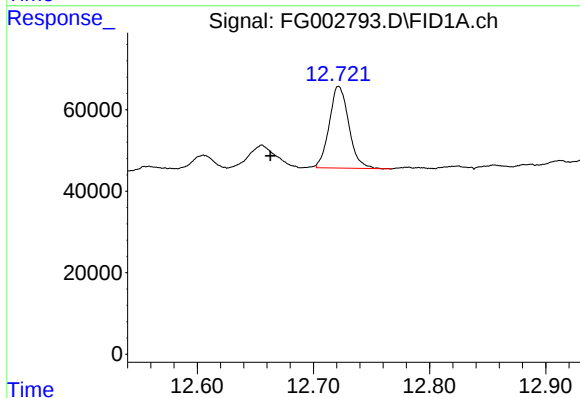


#9 N-EICOSANE

R.T.: 12.722 min
Delta R.T.: 0.059 min
Response: 234228
Conc: 2.07 ug/ml

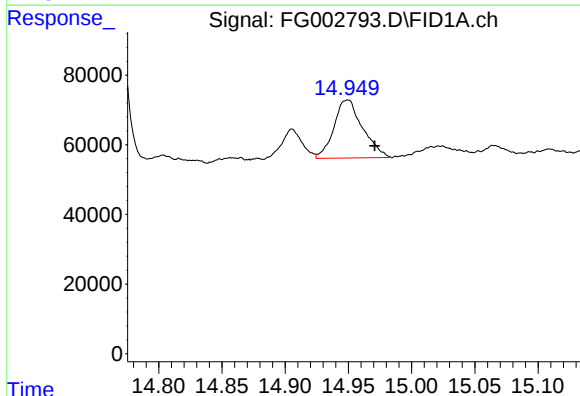


#10 N-TETRACOSANE

R.T.: 14.949 min
Delta R.T.: -0.022 min
Response: 262600
Conc: 2.50 ug/ml

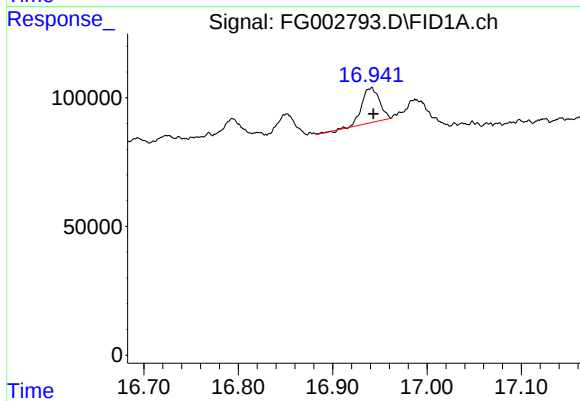


#11 N-OCTACOSANE

R.T.: 16.941 min
Delta R.T.: -0.003 min
Response: 175321
Conc: 1.78 ug/ml

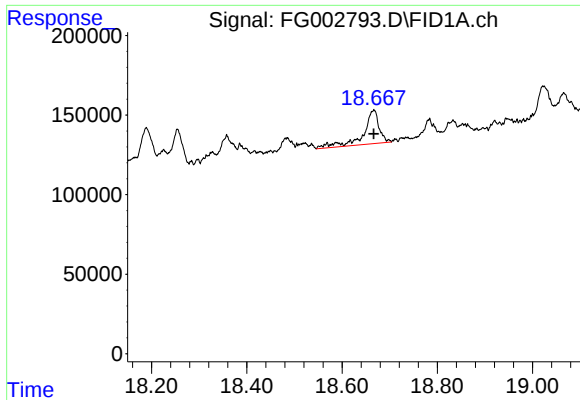


#12 N-DOTRIACONTANE

R.T.: 18.667 min
Delta R.T.: 0.000 min
Response: 479898
Conc: 5.59 ug/ml

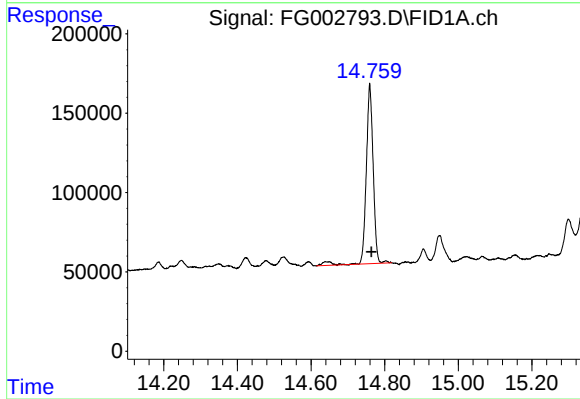

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.760 min
Delta R.T.: -0.004 min
Response: 1493650
Conc: 12.15 ug/ml

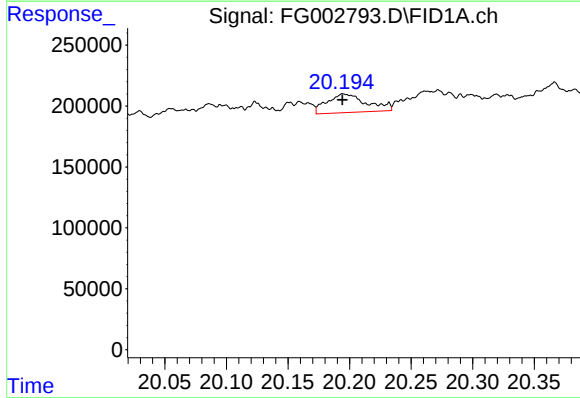

#14 N-HEXATRIACONTANE

R.T.: 20.196 min
Delta R.T.: 0.002 min
Response: 340297
Conc: 5.13 ug/ml