

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110618\
 Data File : FG002809.D
 Signal(s) : FID1A.ch
 Acq On : 07 Nov 2018 13:55
 Operator : AJ\SJ
 Sample : J5827-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 07 16:38:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
 Quant Title :
 QLast Update : Wed Nov 07 10:34:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.764	1824939	14.850 ug/ml
Target Compounds			
6) N-TETRADECANE	8.359	1046286	9.156 ug/ml
9) N-EICOSANE	12.730	401851	3.559 ug/ml
10) N-TETRACOSANE	14.956	302861	2.882 ug/ml
11) N-OCTACOSANE	16.944	314211	3.185 ug/ml
12) N-DOTRIACONTANE	18.668	275317	3.205 ug/ml
14) N-HEXATRIACONTANE	20.196	673764	10.164 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110618\
Data File : FG002809.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2018 13:55
Operator : AJ\SJ
Sample : J5827-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 16:38:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
Quant Title :
QLast Update : Wed Nov 07 10:34:24 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

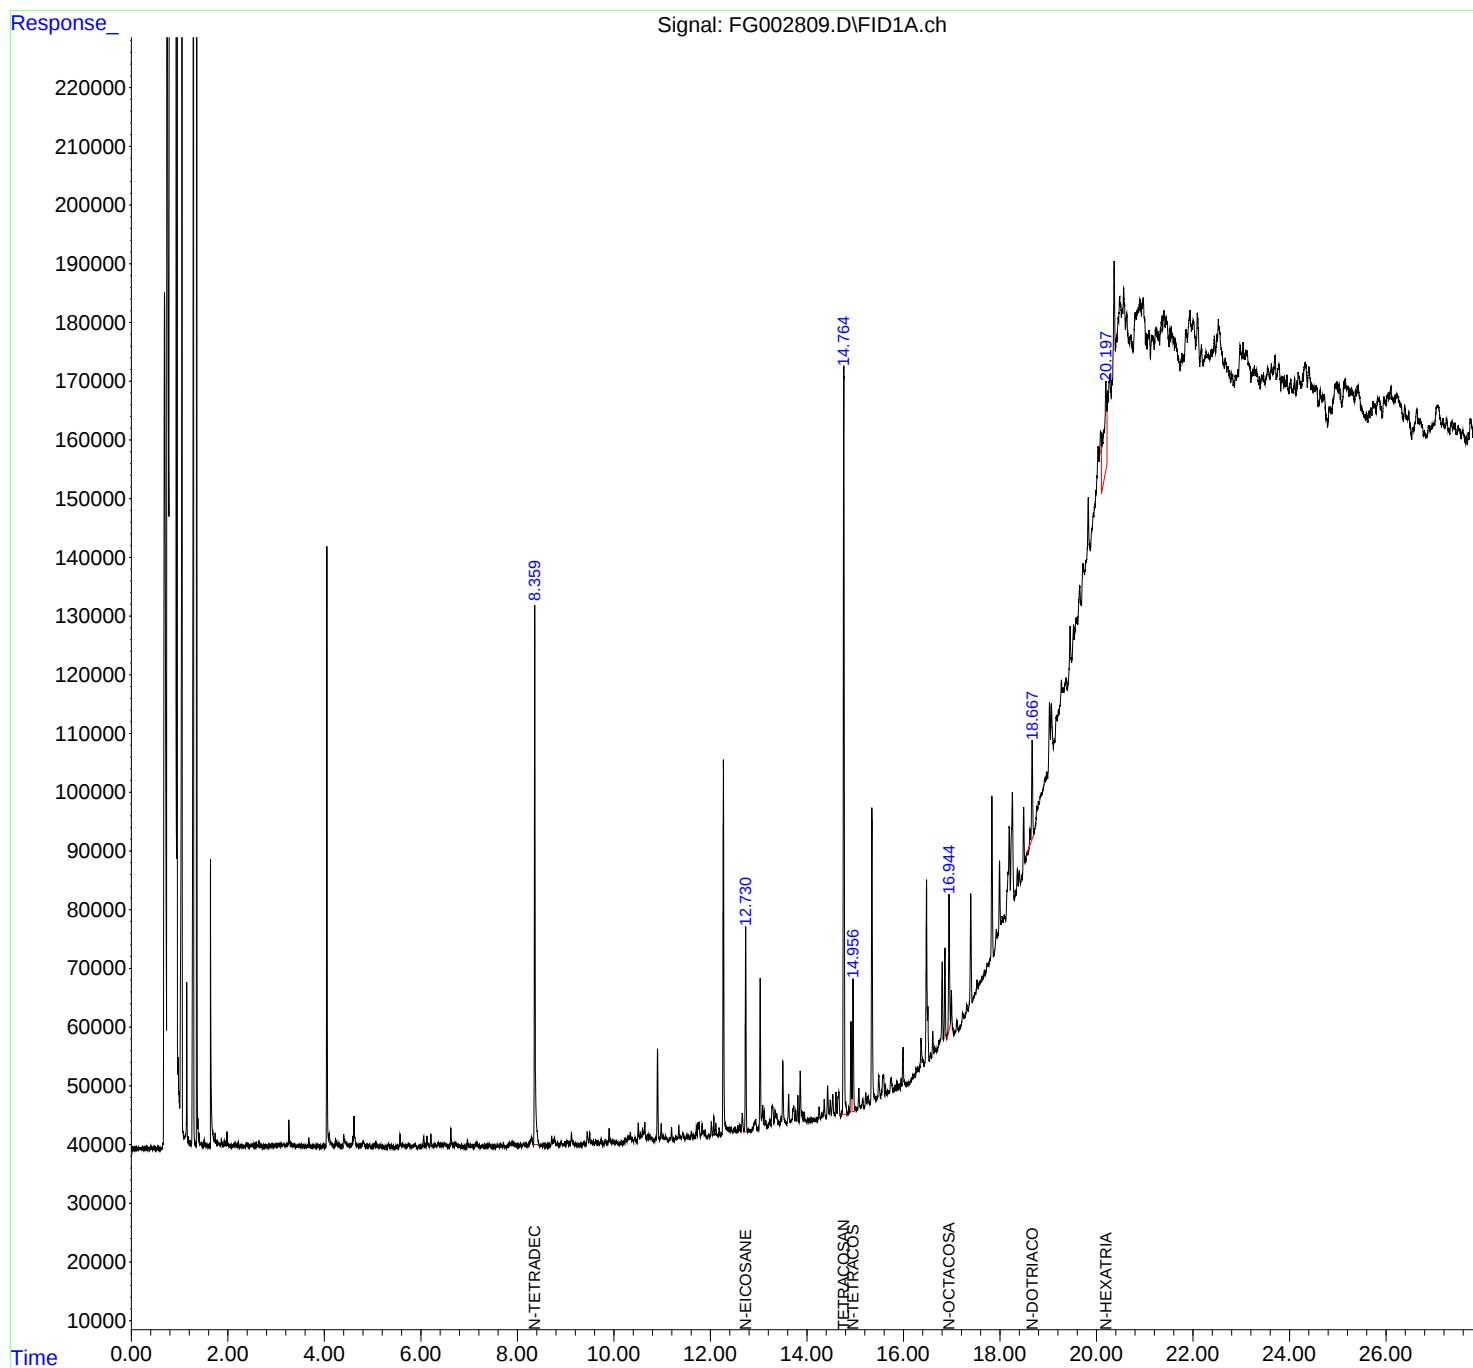

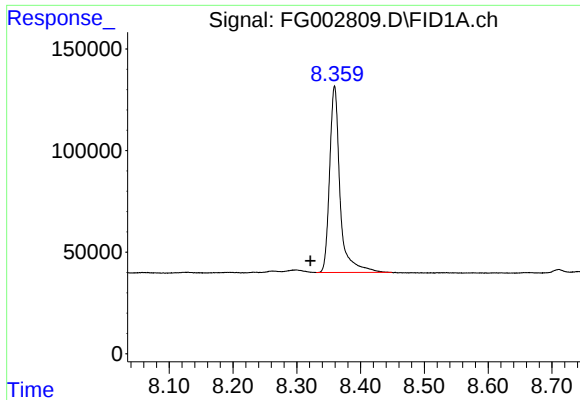


#6 N-TETRADECANE

R.T.: 8.359 min
Delta R.T.: 0.038 min
Response: 1046286
Conc: 9.16 ug/ml

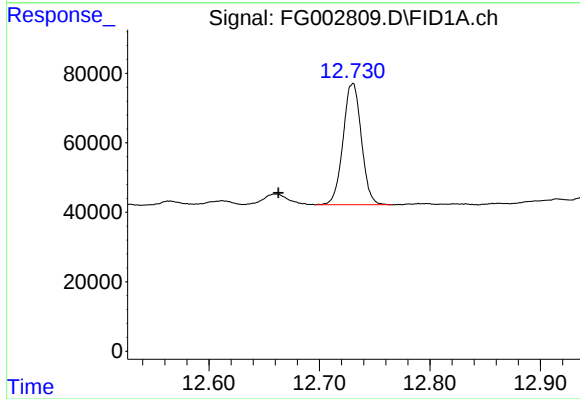


#9 N-EICOSANE

R.T.: 12.730 min
Delta R.T.: 0.067 min
Response: 401851
Conc: 3.56 ug/ml

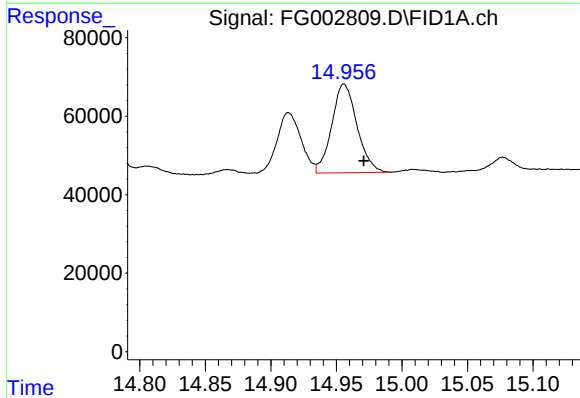


#10 N-TETRACOSANE

R.T.: 14.956 min
Delta R.T.: -0.015 min
Response: 302861
Conc: 2.88 ug/ml

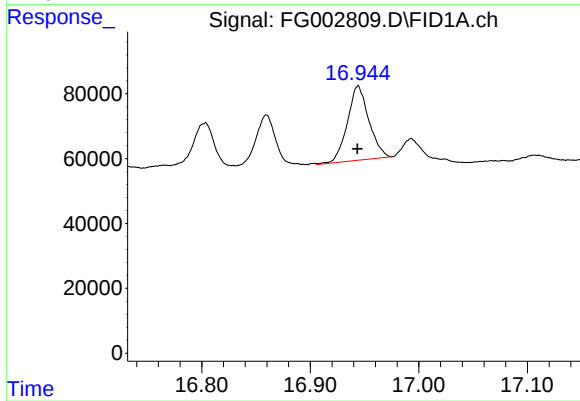


#11 N-OCTACOSANE

R.T.: 16.944 min
Delta R.T.: 0.000 min
Response: 314211
Conc: 3.18 ug/ml

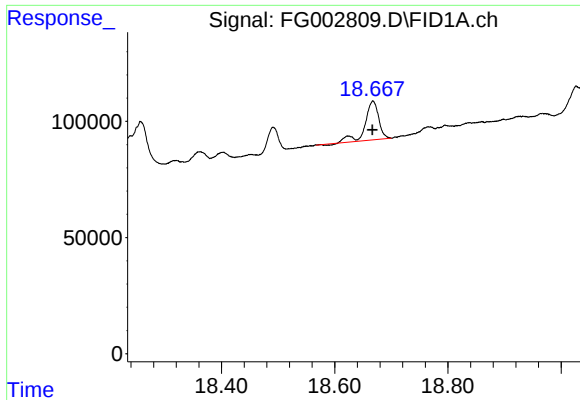


#12 N-DOTRIACONTANE

R.T.: 18.668 min
Delta R.T.: 0.000 min
Response: 275317
Conc: 3.21 ug/ml

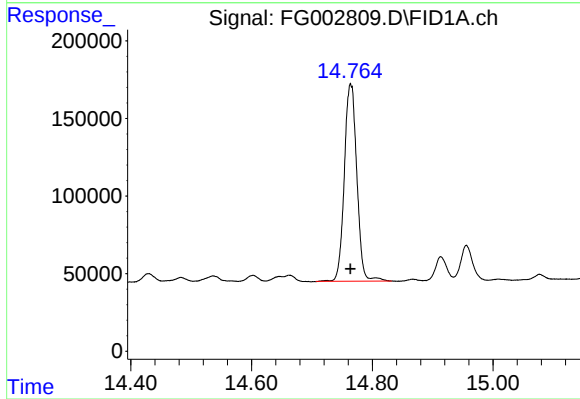

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.764 min
Delta R.T.: 0.000 min
Response: 1824939
Conc: 14.85 ug/ml

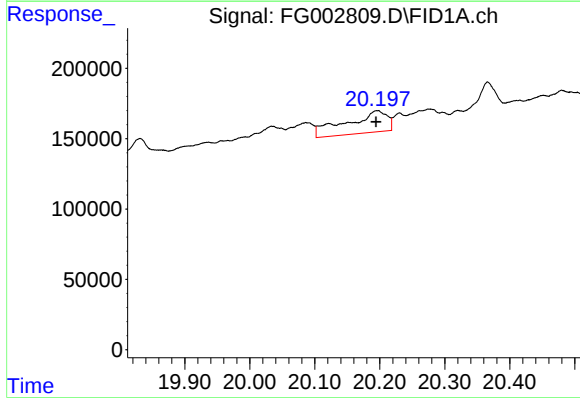

#14 N-HEXATRIACONTANE

R.T.: 20.196 min
Delta R.T.: 0.002 min
Response: 673764
Conc: 10.16 ug/ml