

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110618\
 Data File : FG002810.D
 Signal(s) : FID1A.ch
 Acq On : 07 Nov 2018 14:30
 Operator : AJ\SJ
 Sample : J5827-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 07 16:39:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
 Quant Title :
 QLast Update : Wed Nov 07 10:34:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.763	1817283	14.788 ug/ml
Target Compounds				
6)	N-TETRADECANE	8.359	1055969	9.241 ug/ml
9)	N-EICOSANE	12.729	398180	3.527 ug/ml
10)	N-TETRACOSANE	14.955	300257	2.857 ug/ml
11)	N-OCTACOSANE	16.944	308723	3.129 ug/ml
12)	N-DOTRIACONTANE	18.666	219055	2.550 ug/ml
14)	N-HEXATRIACONTANE	20.243	342707	5.170 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110618\
Data File : FG002810.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2018 14:30
Operator : AJ\SJ
Sample : J5827-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 16:39:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
Quant Title :
QLast Update : Wed Nov 07 10:34:24 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

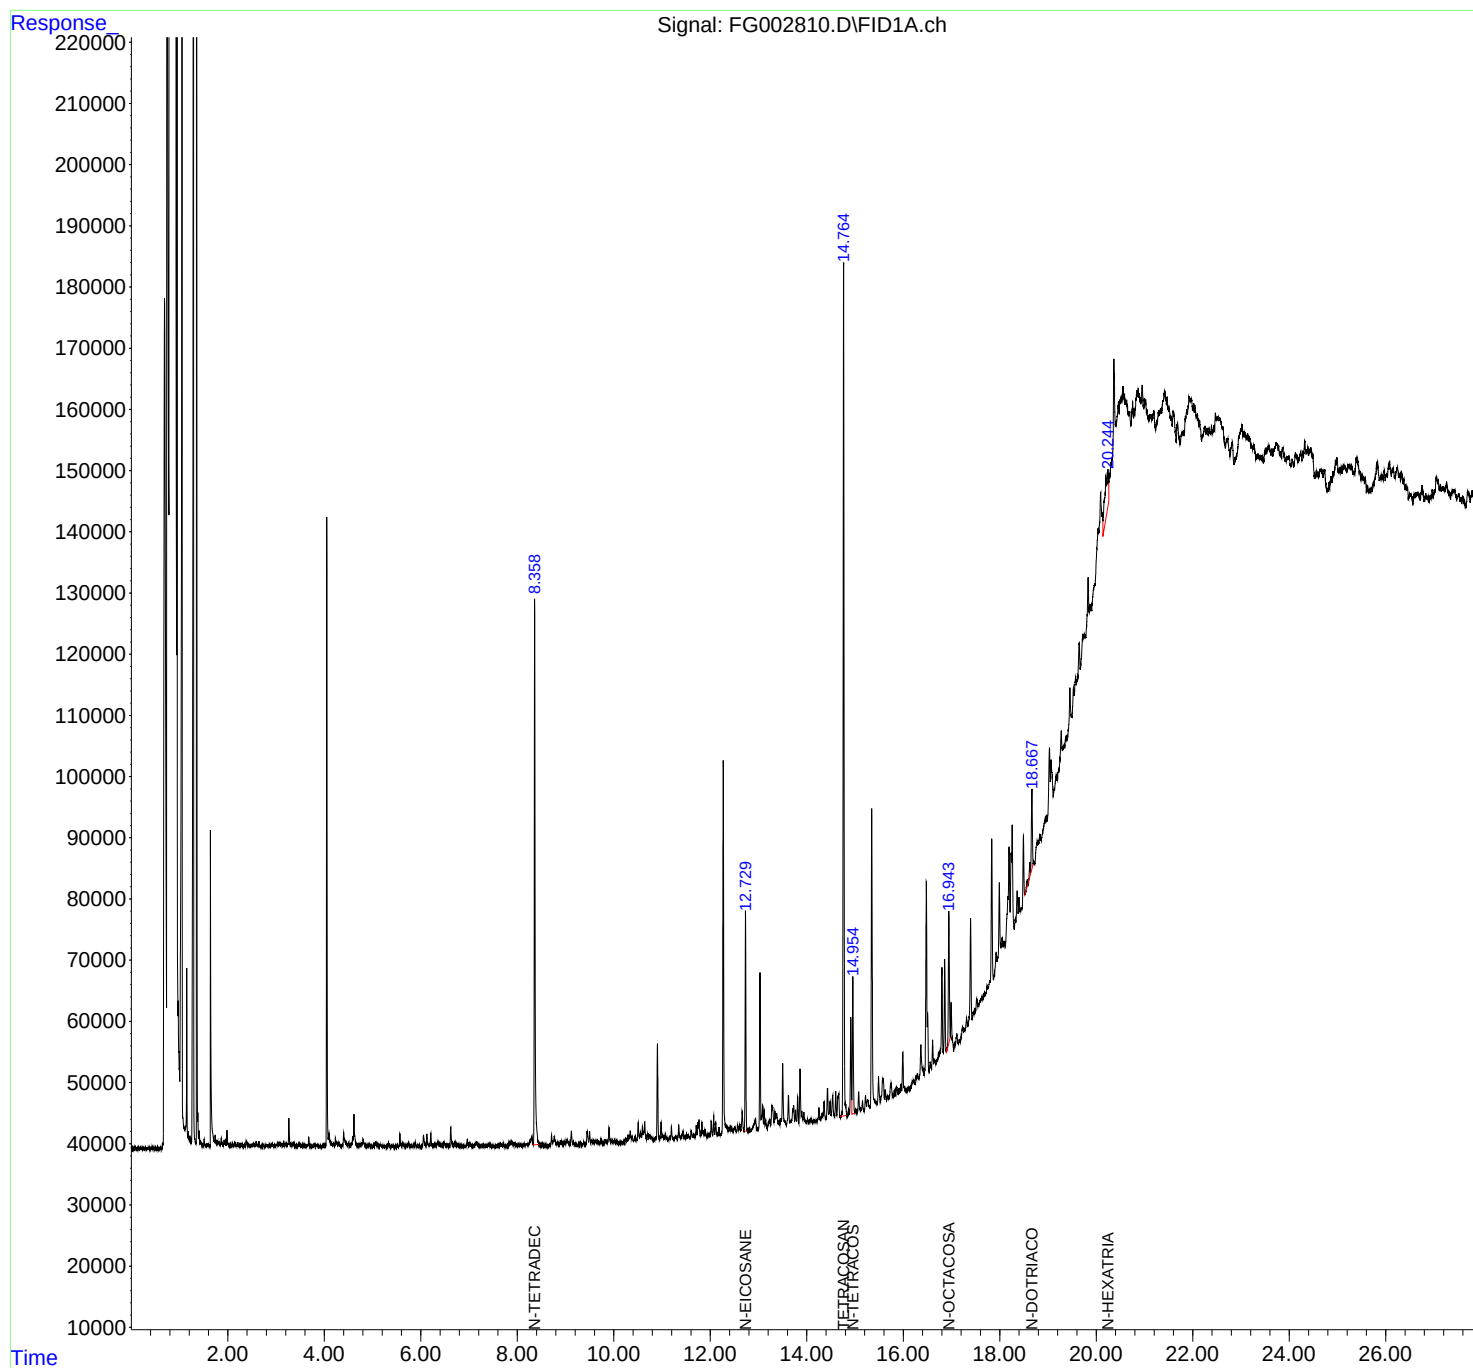

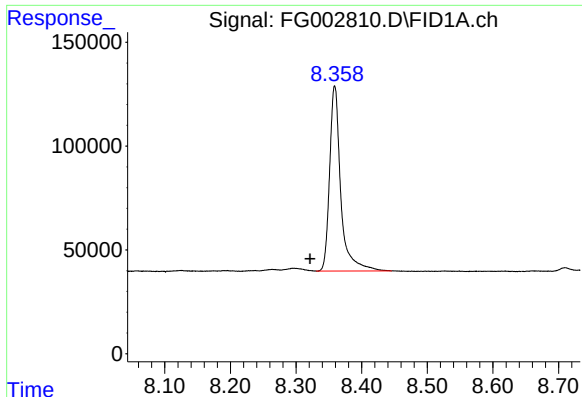


#6 N-TETRADECANE

R.T.: 8.359 min
Delta R.T.: 0.037 min
Response: 1055969
Conc: 9.24 ug/ml

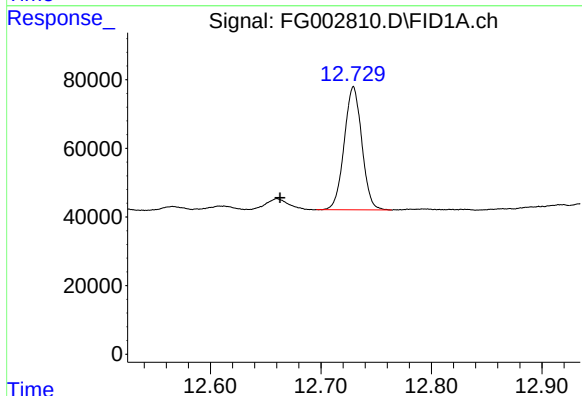


#9 N-EICOSANE

R.T.: 12.729 min
Delta R.T.: 0.066 min
Response: 398180
Conc: 3.53 ug/ml

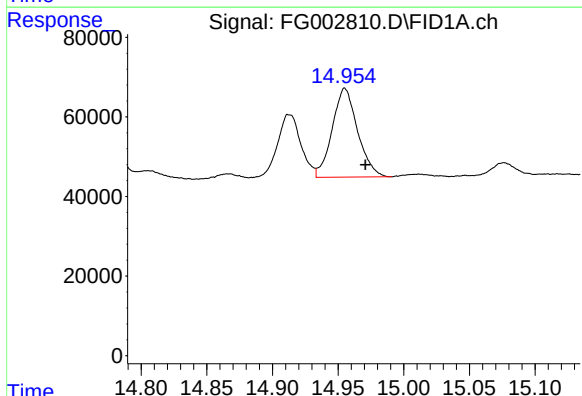


#10 N-TETRACOSANE

R.T.: 14.955 min
Delta R.T.: -0.016 min
Response: 300257
Conc: 2.86 ug/ml

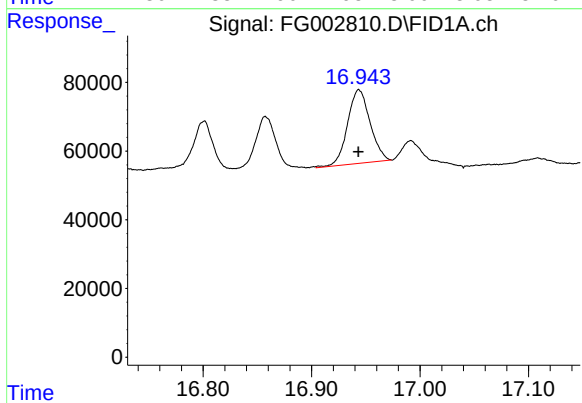


#11 N-OCTACOSANE

R.T.: 16.944 min
Delta R.T.: 0.000 min
Response: 308723
Conc: 3.13 ug/ml

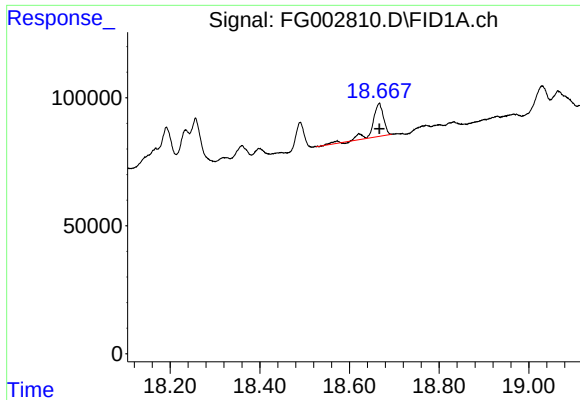


#12 N-DOTRIACONTANE

R.T.: 18.666 min
Delta R.T.: 0.000 min
Response: 219055
Conc: 2.55 ug/ml

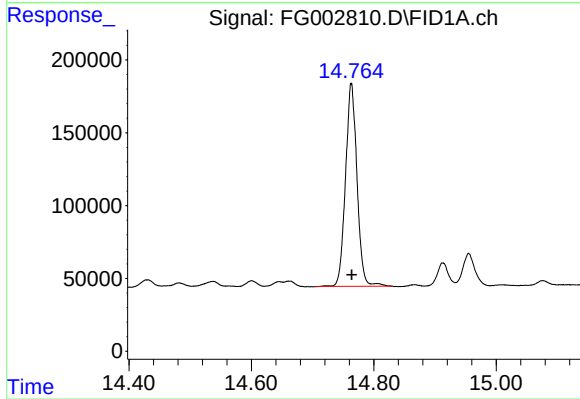

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.763 min
Delta R.T.: 0.000 min
Response: 1817283
Conc: 14.79 ug/ml

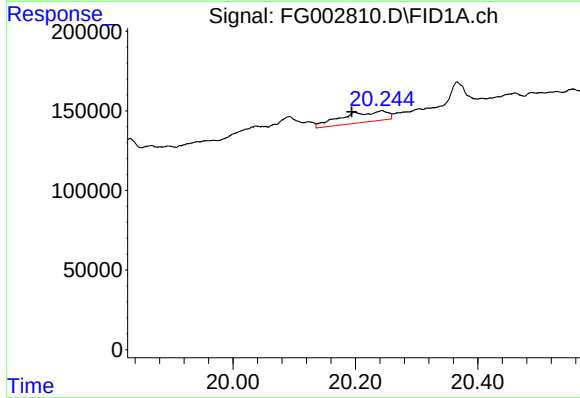

#14 N-HEXATRIACONTANE

R.T.: 20.243 min
Delta R.T.: 0.049 min
Response: 342707
Conc: 5.17 ug/ml