

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG110620\  
 Data File : FG007304.D  
 Signal(s) : FID1A.ch  
 Acq On : 07 Nov 2020 03:08  
 Operator : DD\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Nov 07 04:16:48 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG110220.M  
 Quant Title :  
 QLast Update : Tue Nov 03 02:04:00 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.473	3481252	24.855 ug/ml
12) N-OCTACOSANE	16.924	3089470	23.265 ug/ml
13) N-TRIACONTANE	17.812	181326	1.410 ug/ml
14) N-DOTRIACONTANE	18.646	228909	1.930 ug/ml
15) N-TETRATRIACONTANE	19.432	169010	1.749 ug/ml
16) N-HEXATRIACONTANE	20.172	100524	1.307 ug/ml
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG110620\  
 Data File : FG007304.D  
 Signal(s) : FID1A.ch  
 Acq On : 07 Nov 2020 03:08  
 Operator : DD\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampled :

Integration File: autoint1.e  
 Quant Time: Nov 07 04:16:48 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG110220.M  
 Quant Title :  
 QLast Update : Tue Nov 03 02:04:00 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation


Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

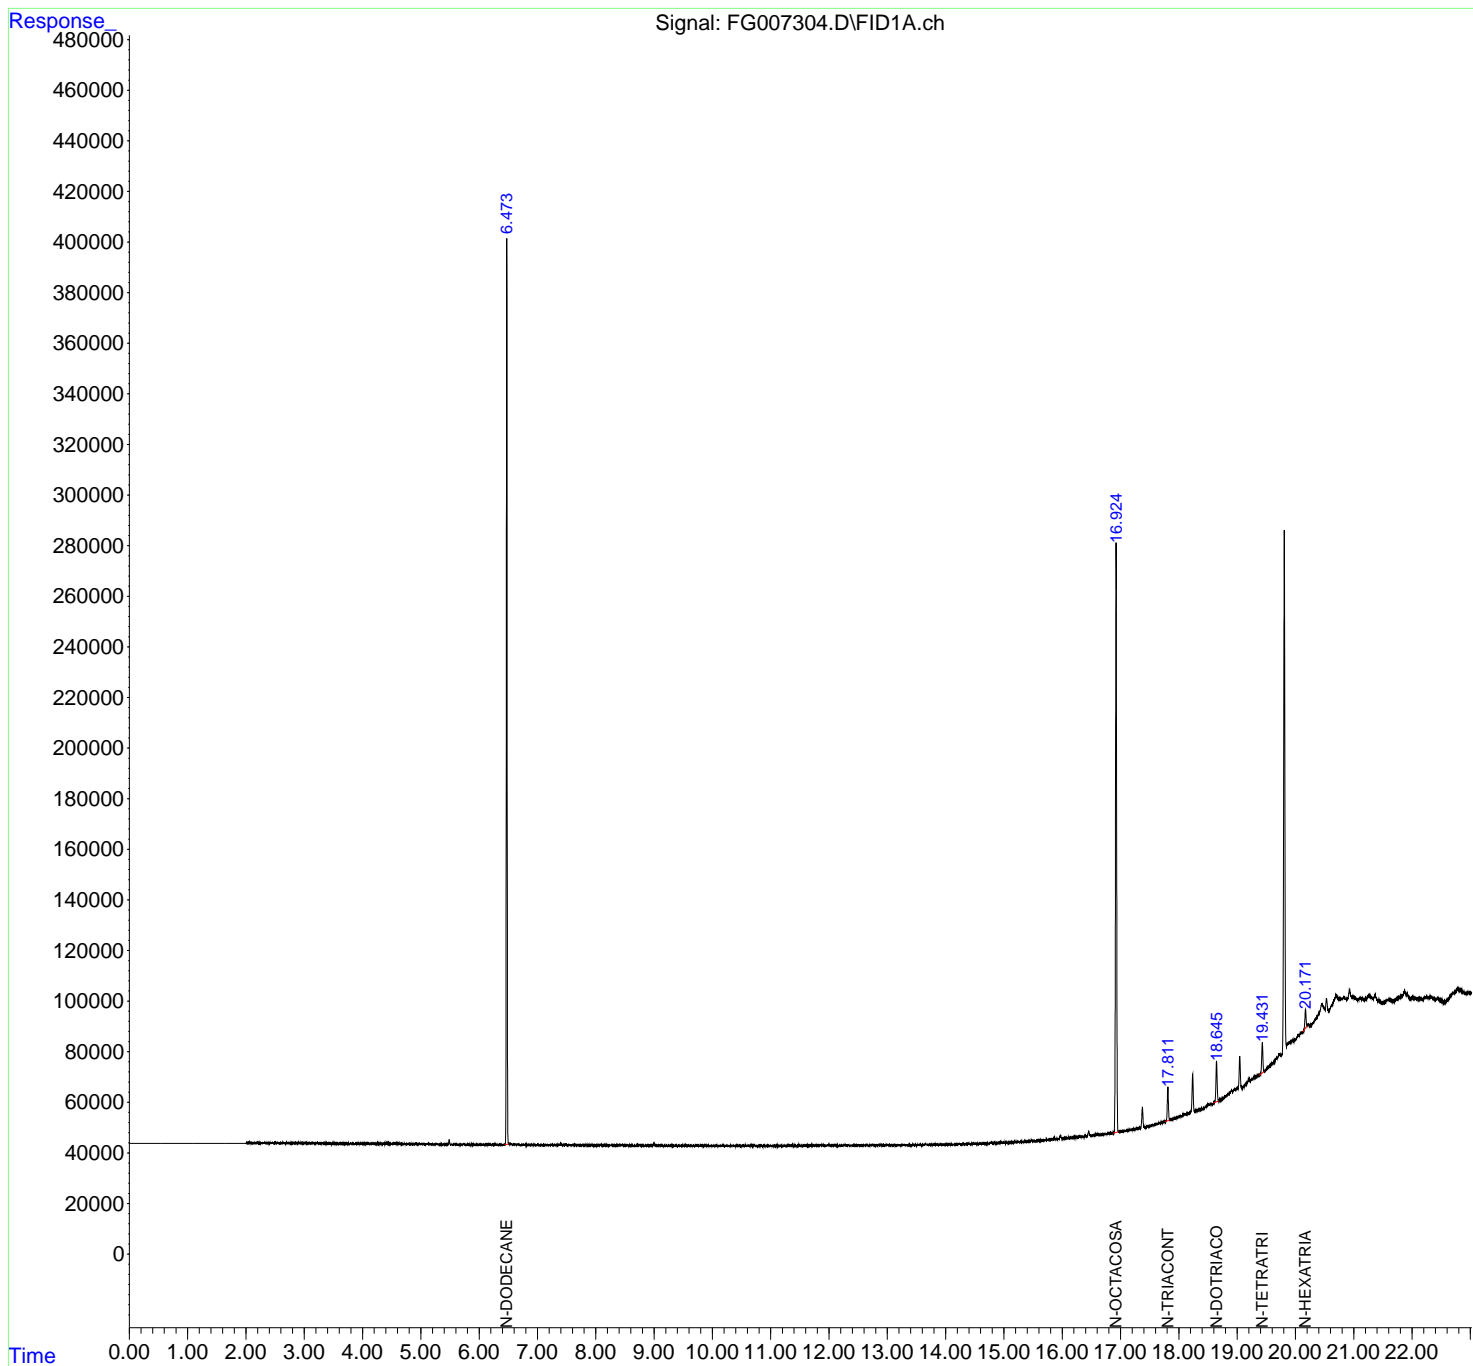

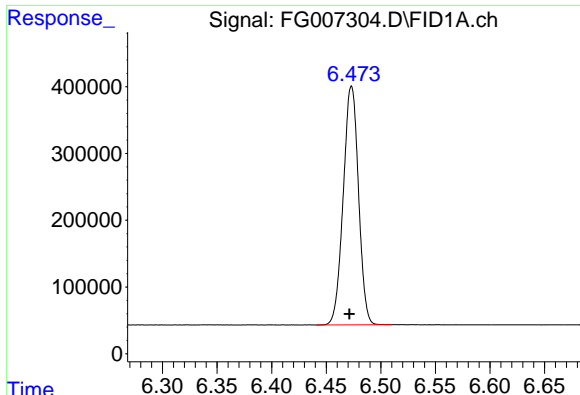


#3 N-DODECANE  
 R.T.: 6.473 min  
 Delta R.T.: 0.002 min  
 Response: 3481252  
 Conc: 24.85 ug/ml


Instrument :  
 FID\_G  
 ClientSampleId :

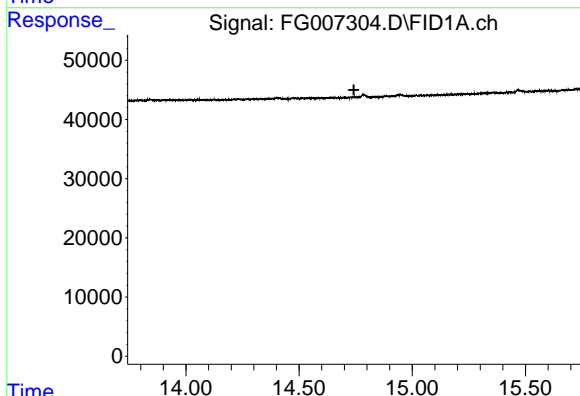


#9 TETRACOSANE-d50 (SURROGATE)  
 R.T.: 0.000 min  
 Exp R.T. : 14.742 min  
 Response: 0  
 Conc: N.D.

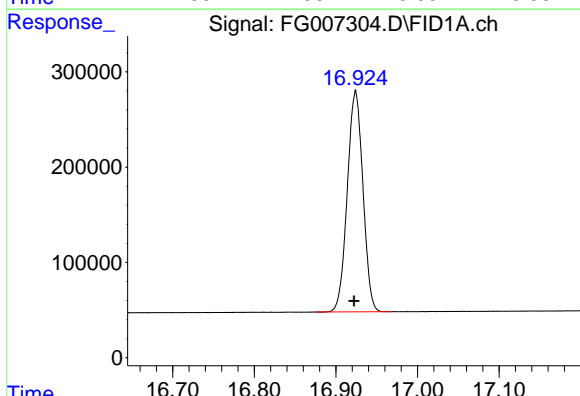

#12 N-OCTACOSANE  
 R.T.: 16.924 min  
 Delta R.T.: 0.002 min  
 Response: 3089470  
 Conc: 23.27 ug/ml

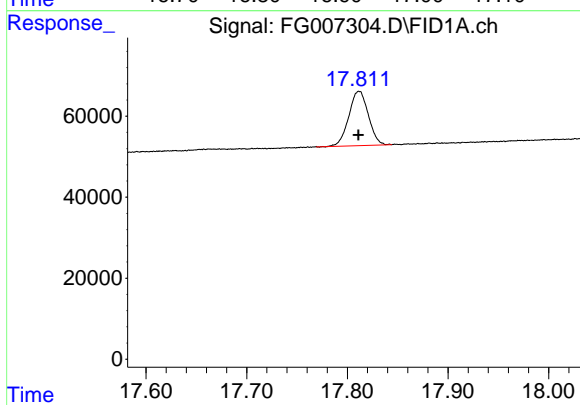


#13 N-TRIACONTANE  
 R.T.: 17.812 min  
 Delta R.T.: 0.000 min  
 Response: 181326  
 Conc: 1.41 ug/ml

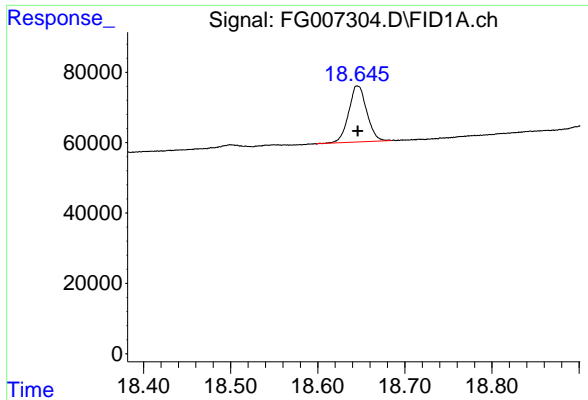

#14 N-DOTRIACONTANE


R.T.: 18.646 min  
Delta R.T.: 0.000 min  
Response: 228909  
Conc: 1.93 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

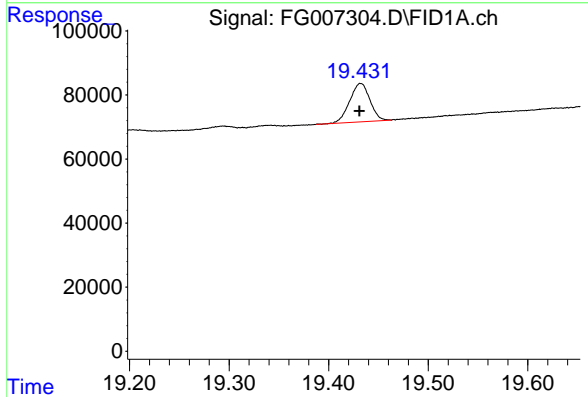

#15 N-TETRATRIACONTANE

R.T.: 19.432 min  
Delta R.T.: 0.001 min  
Response: 169010  
Conc: 1.75 ug/ml

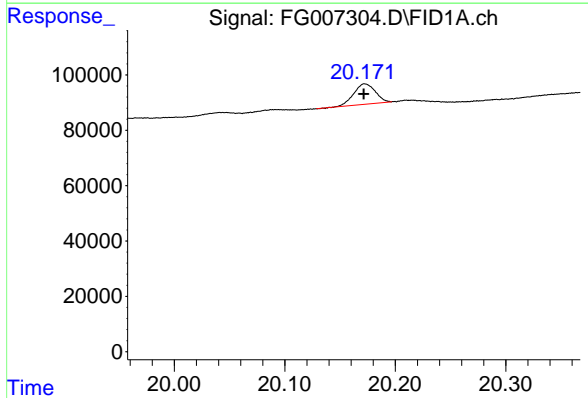

#16 N-HEXATRIACONTANE

R.T.: 20.172 min  
Delta R.T.: 0.001 min  
Response: 100524  
Conc: 1.31 ug/ml