

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110620\
 Data File : FG007305.D
 Signal(s) : FID1A.ch
 Acq On : 07 Nov 2020 03:39
 Operator : DD\AJ
 Sample : L4621-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 07 04:17:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
 Quant Title :
 QLast Update : Tue Nov 03 02:04:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.746	1891554	15.375 ug/ml
Target Compounds			
4) N-TETRADECANE	8.237	162562	1.153 ug/ml
7) N-EICOSANE	12.627	356064	2.483 ug/ml
8) N-DOCOSANE	13.876	1057701	7.533 ug/ml
10) N-TETRACOSANE	14.939	2983493	21.369 ug/ml
11) N-HEXACOSANE	15.969	207458	1.524 ug/ml
12) N-OCTACOSANE	16.910	244949	1.845 ug/ml
13) N-TRIACONTANE	17.816	962377	7.484 ug/ml
14) N-DOTRIACONTANE	18.640	408069	3.441 ug/ml
15) N-TETRATRIACONTANE	19.443	301977	3.125 ug/ml
16) N-HEXATRIACONTANE	20.172	543489	7.067 ug/ml
17) N-OCTATRIACONTANE	20.964	105720	1.603 ug/ml
18) N-TETRACONTANE	21.870	135788	2.115 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110620\
Data File : FG007305.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2020 03:39
Operator : DD\AJ
Sample : L4621-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 07 04:17:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
Quant Title :
QLast Update : Tue Nov 03 02:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

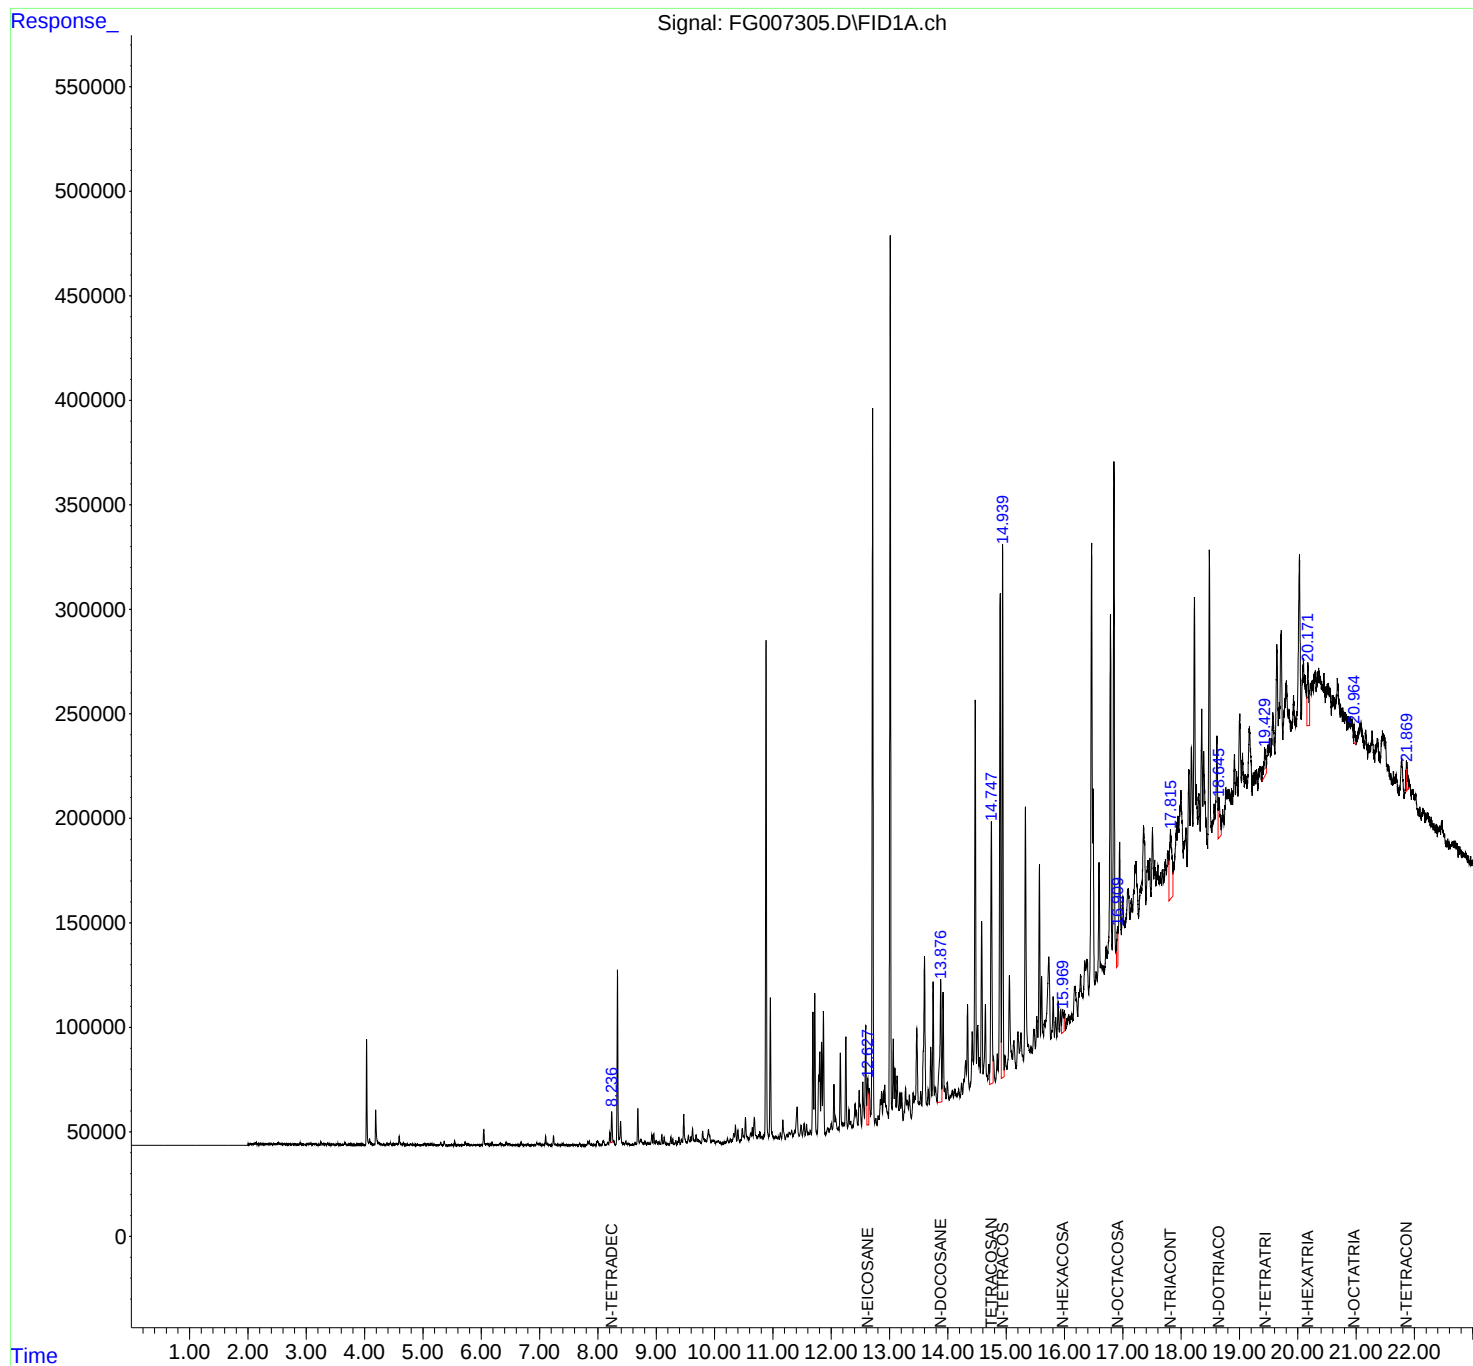


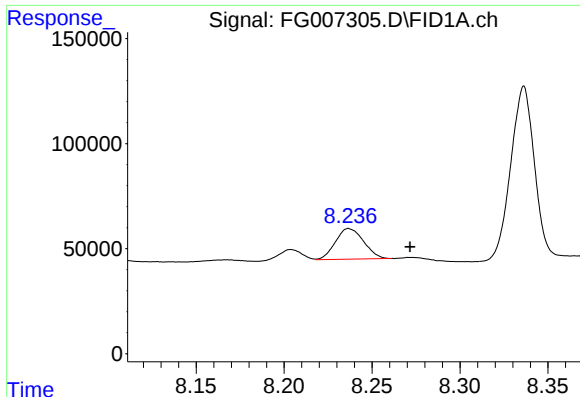

#4 N-TETRADECANE


R.T.: 8.237 min
Delta R.T.: -0.035 min
Response: 162562
Conc: 1.15 ug/ml

Instrument :
FID_G
ClientSampleId :

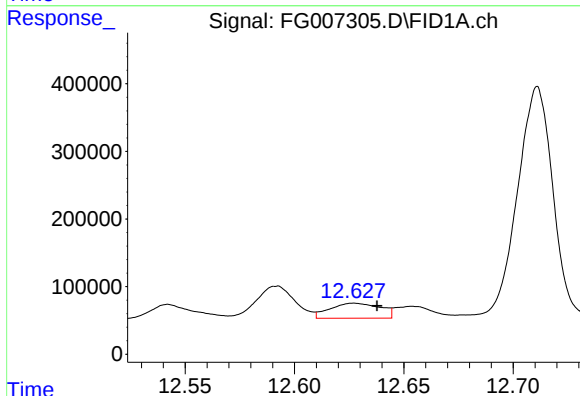


#7 N-EICOSANE

R.T.: 12.627 min
Delta R.T.: -0.010 min
Response: 356064
Conc: 2.48 ug/ml

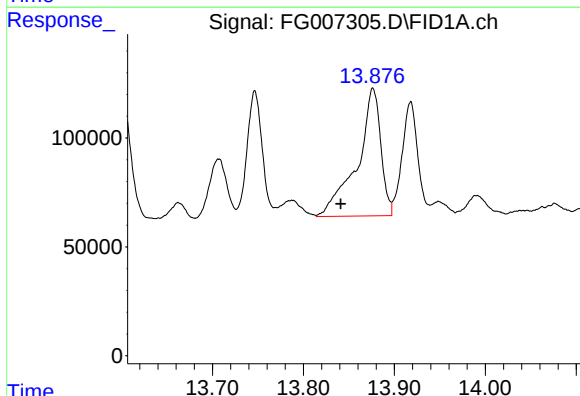


#8 N-DOCOSANE

R.T.: 13.876 min
Delta R.T.: 0.035 min
Response: 1057701
Conc: 7.53 ug/ml

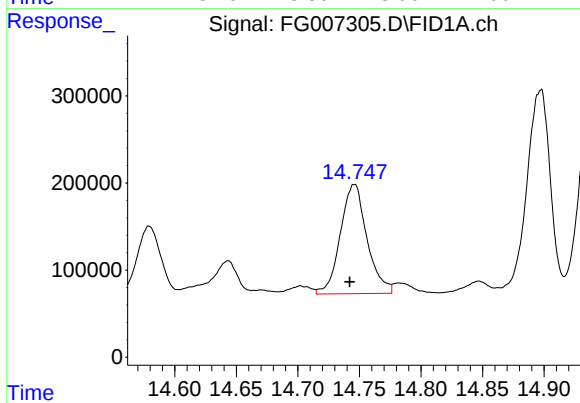

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.746 min
Delta R.T.: 0.004 min
Response: 1891554
Conc: 15.38 ug/ml

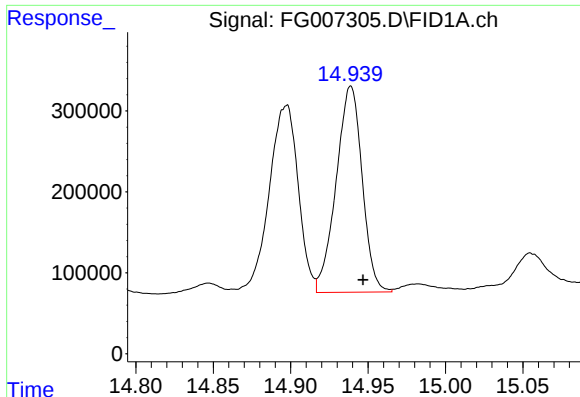

#10 N-TETRACOSANE


R.T.: 14.939 min
Delta R.T.: -0.008 min
Response: 2983493
Conc: 21.37 ug/ml

Instrument :
FID_G
ClientSampleId :

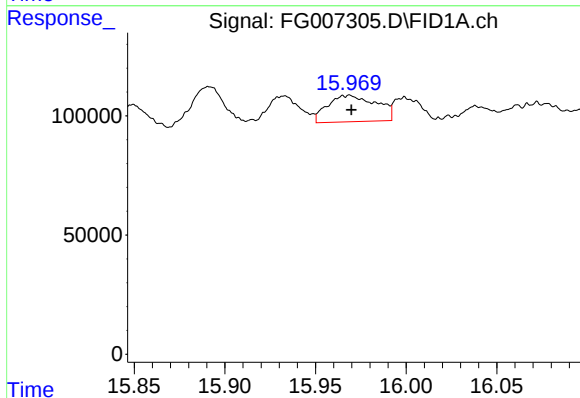


#11 N-HEXACOSANE

R.T.: 15.969 min
Delta R.T.: 0.000 min
Response: 207458
Conc: 1.52 ug/ml

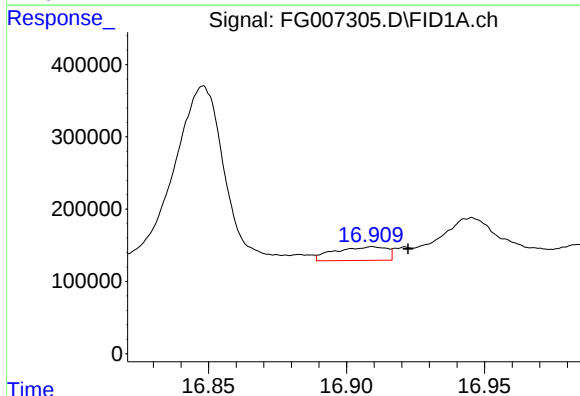


#12 N-OCTACOSANE

R.T.: 16.910 min
Delta R.T.: -0.013 min
Response: 244949
Conc: 1.84 ug/ml

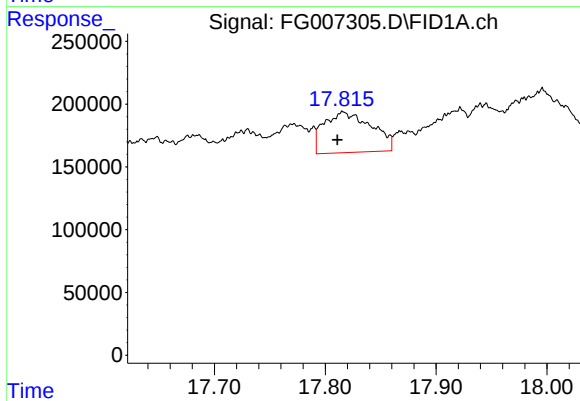

#13 N-TRIACONTANE


R.T.: 17.816 min
Delta R.T.: 0.005 min
Response: 962377
Conc: 7.48 ug/ml

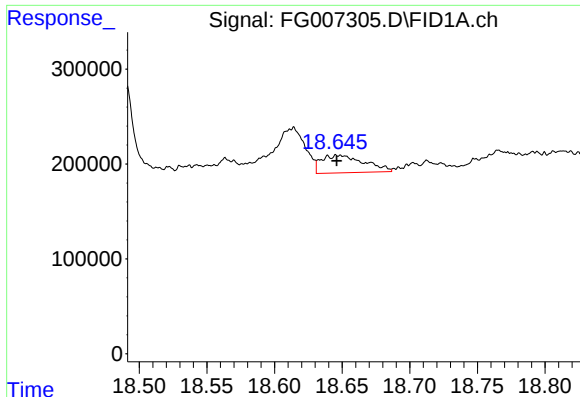

#14 N-DOTRIACONTANE


R.T.: 18.640 min
Delta R.T.: -0.006 min
Response: 408069
Conc: 3.44 ug/ml

Instrument :
FID_G
ClientSampleId :

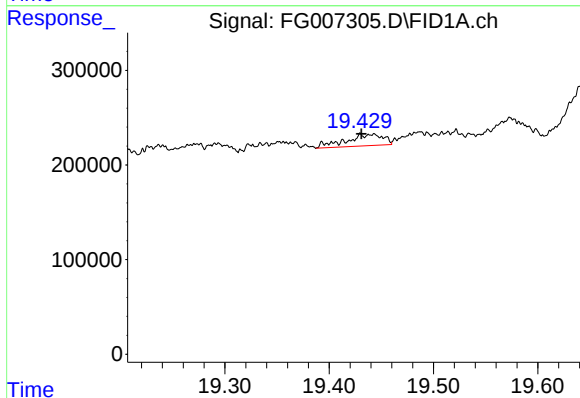


#15 N-TETRATRIACONTANE

R.T.: 19.443 min
Delta R.T.: 0.012 min
Response: 301977
Conc: 3.12 ug/ml

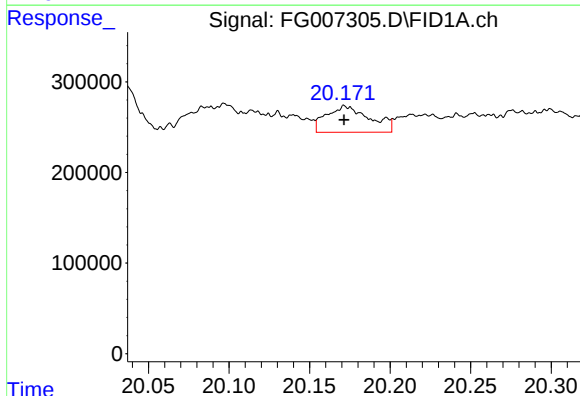


#16 N-HEXATRIACONTANE

R.T.: 20.172 min
Delta R.T.: 0.000 min
Response: 543489
Conc: 7.07 ug/ml

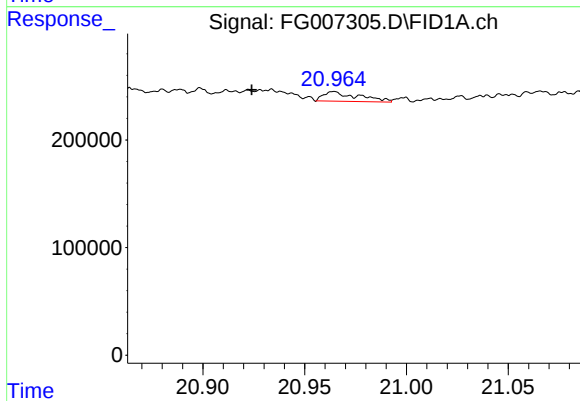

#17 N-OCTATRIACONTANE

R.T.: 20.964 min
Delta R.T.: 0.040 min
Response: 105720
Conc: 1.60 ug/ml

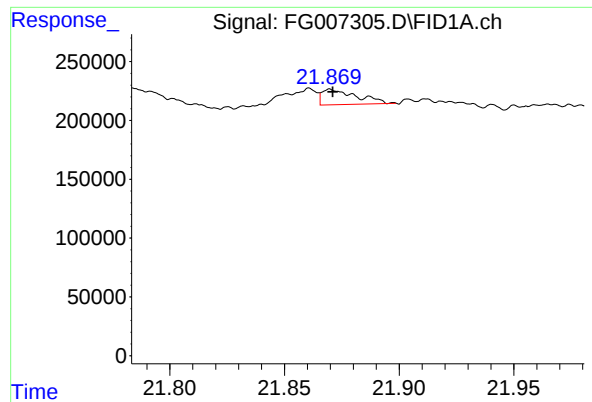

#18 N-TETRACONTANE

R.T.: 21.870 min
Delta R.T.: -0.001 min
Response: 135788
Conc: 2.11 ug/ml

Instrument :
FID_G
ClientSampleId :