

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110620\
 Data File : FG007306.D
 Signal(s) : FID1A.ch
 Acq On : 07 Nov 2020 04:10
 Operator : DD\AJ
 Sample : L4657-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 07 05:06:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
 Quant Title :
 QLast Update : Tue Nov 03 02:04:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.749	1738601	14.132 ug/ml
Target Compounds			
4) N-TETRADECANE	8.337f	507156	3.597 ug/ml
7) N-EICOSANE	12.591	63633	0.444 ug/ml
8) N-DOCOSANE	13.856	299977	2.137 ug/ml
10) N-TETRACOSANE	14.936	630562	4.516 ug/ml
11) N-HEXACOSANE	15.983	591010	4.342 ug/ml
12) N-OCTACOSANE	16.908	859454	6.472 ug/ml
13) N-TRIACONTANE	17.832	8127484	63.200 ug/ml
14) N-DOTRIACONTANE	18.646	6562995	55.347 ug/ml
15) N-TETRATRIACONTANE	19.446	4625004	47.859 ug/ml
16) N-HEXATRIACONTANE	20.163	1683996	21.896 ug/ml
17) N-OCTATRIACONTANE	20.915	2320175	35.181 ug/ml
18) N-TETRACONTANE	21.867	434674	6.769 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110620\
Data File : FG007306.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2020 04:10
Operator : DD\AJ
Sample : L4657-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 07 05:06:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
Quant Title :
QLast Update : Tue Nov 03 02:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

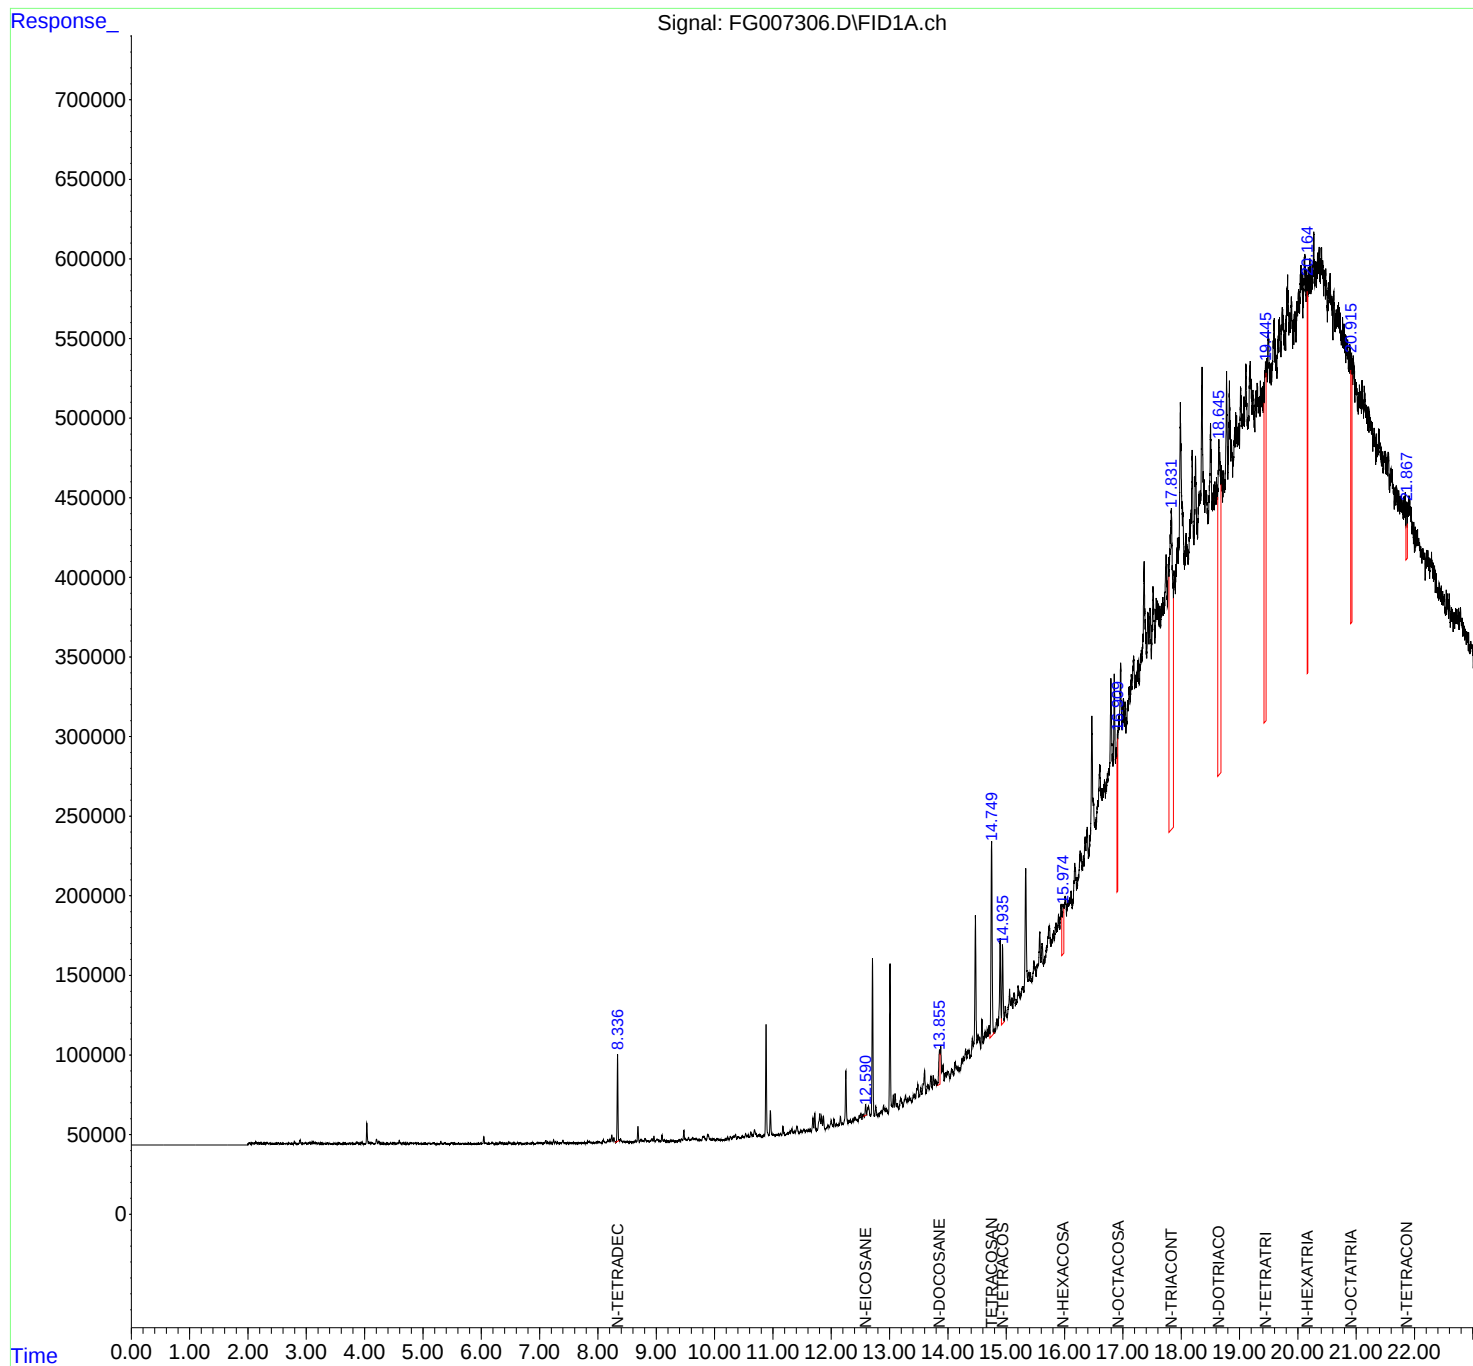


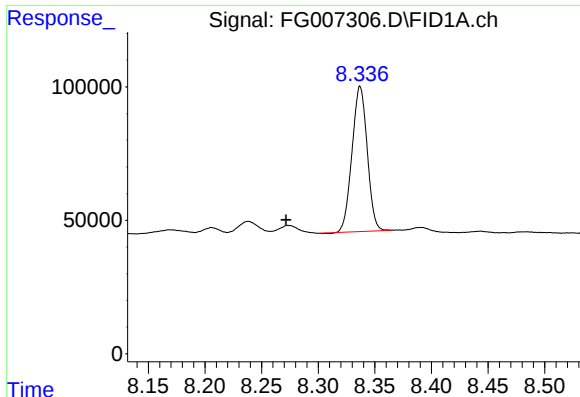

#4 N-TETRADECANE


R.T.: 8.337 min
Delta R.T.: 0.065 min
Response: 507156
Conc: 3.60 ug/ml

Instrument :
FID_G
ClientSampleId :

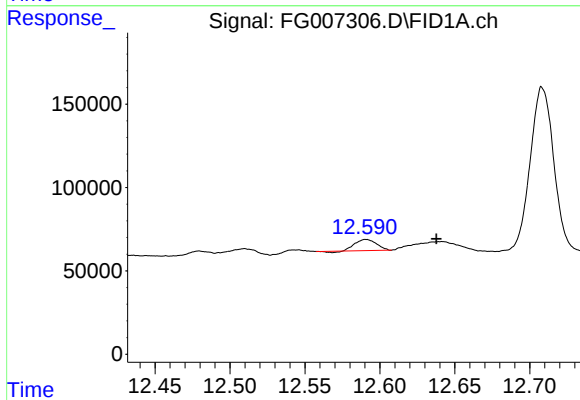


#7 N-EICOSANE

R.T.: 12.591 min
Delta R.T.: -0.047 min
Response: 63633
Conc: 0.44 ug/ml

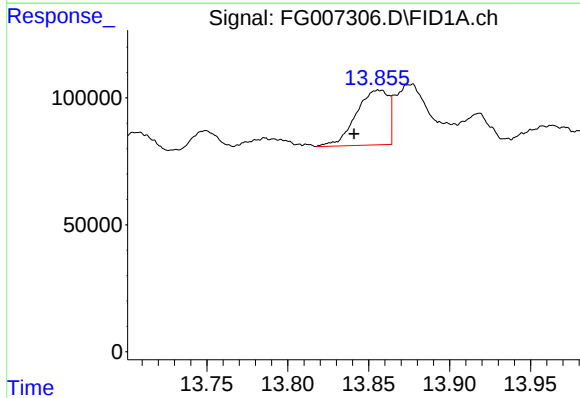


#8 N-DOCOSANE

R.T.: 13.856 min
Delta R.T.: 0.015 min
Response: 299977
Conc: 2.14 ug/ml

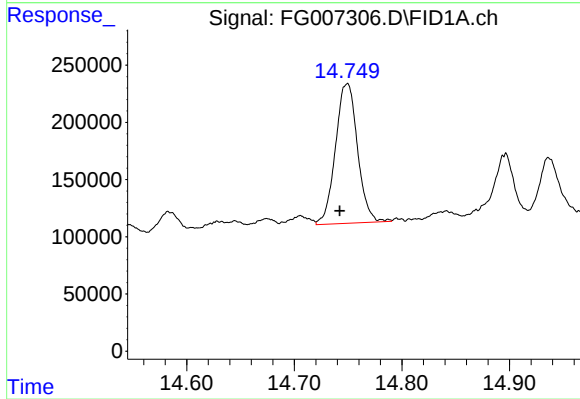

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.749 min
Delta R.T.: 0.007 min
Response: 1738601
Conc: 14.13 ug/ml

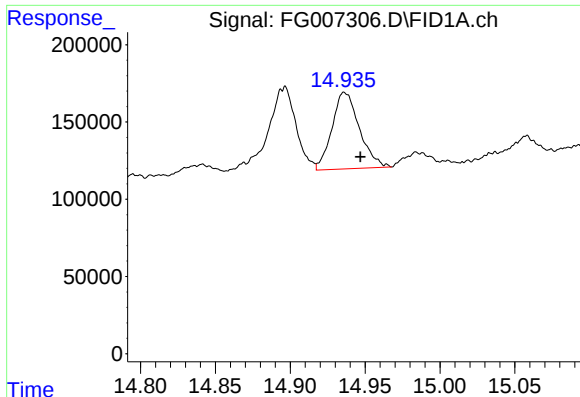

#10 N-TETRACOSANE


R.T.: 14.936 min
Delta R.T.: -0.011 min
Response: 630562
Conc: 4.52 ug/ml

Instrument :
FID_G
ClientSampleId :

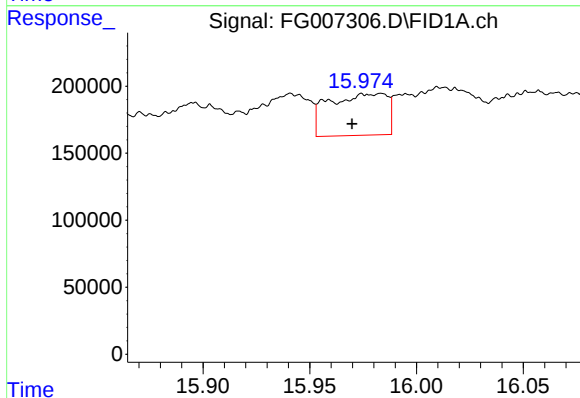


#11 N-HEXACOSANE

R.T.: 15.983 min
Delta R.T.: 0.014 min
Response: 591010
Conc: 4.34 ug/ml

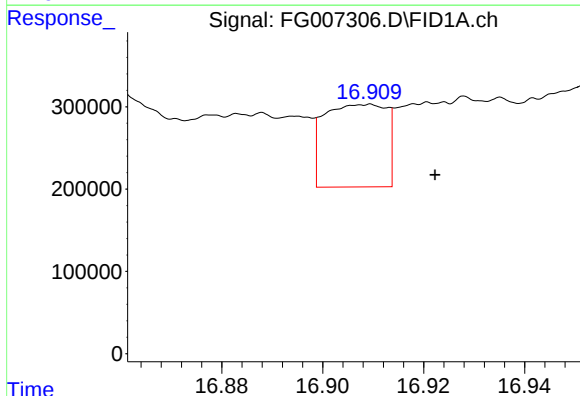


#12 N-OCTACOSANE

R.T.: 16.908 min
Delta R.T.: -0.014 min
Response: 859454
Conc: 6.47 ug/ml

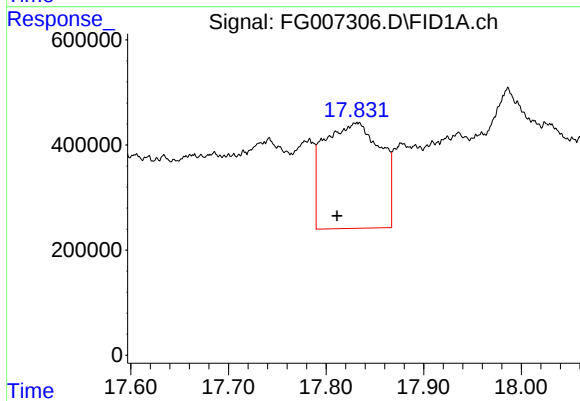

#13 N-TRIACONTANE


R.T.: 17.832 min
Delta R.T.: 0.021 min
Response: 8127484
Conc: 63.20 ug/ml

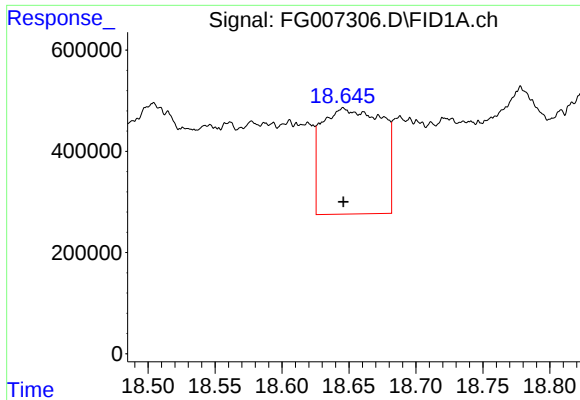

#14 N-DOTRIACONTANE


R.T.: 18.646 min
Delta R.T.: 0.000 min
Response: 6562995
Conc: 55.35 ug/ml

Instrument :
FID_G
ClientSampleId :

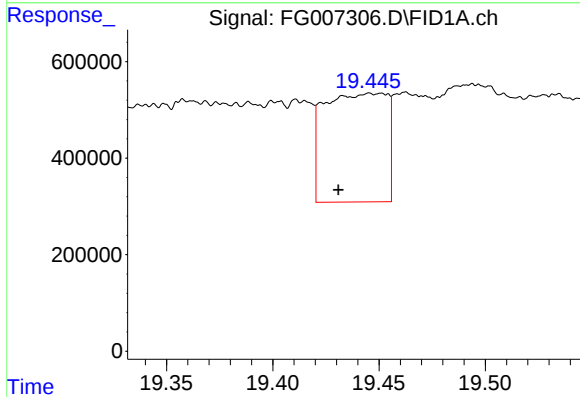


#15 N-TETRATRIACONTANE

R.T.: 19.446 min
Delta R.T.: 0.015 min
Response: 4625004
Conc: 47.86 ug/ml

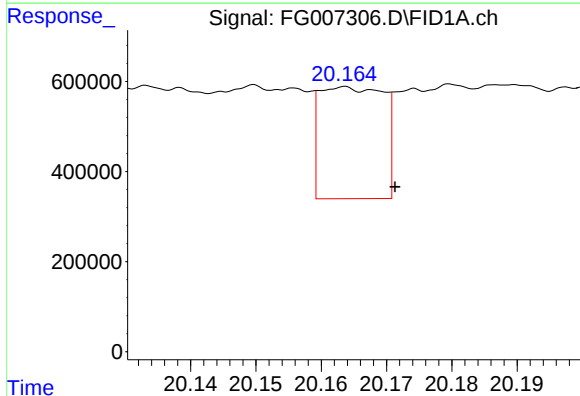


#16 N-HEXATRIACONTANE

R.T.: 20.163 min
Delta R.T.: -0.008 min
Response: 1683996
Conc: 21.90 ug/ml

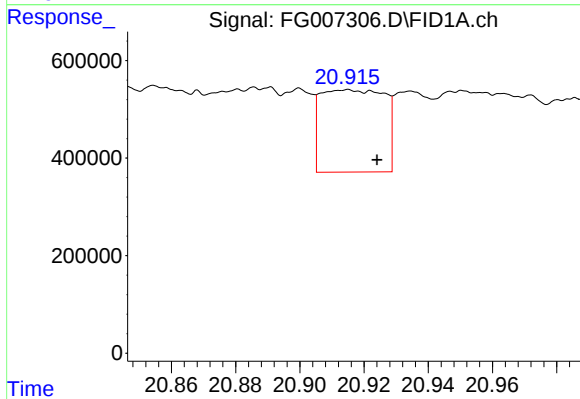

#17 N-OCTATRIACONTANE

R.T.: 20.915 min
Delta R.T.: -0.009 min
Response: 2320175
Conc: 35.18 ug/ml

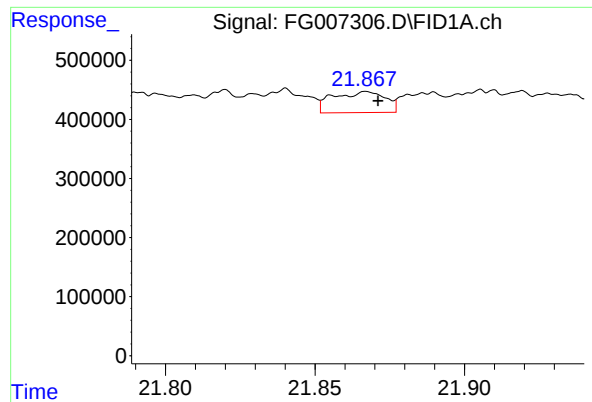

#18 N-TETRACONTANE

R.T.: 21.867 min
Delta R.T.: -0.004 min
Response: 434674
Conc: 6.77 ug/ml

Instrument :
FID_G
ClientSampleId :