

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110620\
 Data File : FG007308.D
 Signal(s) : FID1A.ch
 Acq On : 07 Nov 2020 05:11
 Operator : DD\AJ
 Sample : L4657-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 07 07:33:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
 Quant Title :
 QLast Update : Tue Nov 03 02:04:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.749	2440164	19.834 ug/ml
Target Compounds			
4) N-TETRADECANE	8.339f	899918	6.382 ug/ml
10) N-TETRACOSANE	14.939	110419	0.791 ug/ml
12) N-OCTACOSANE	16.929	84896	0.639 ug/ml
13) N-TRIACONTANE	17.818	155831	1.212 ug/ml
14) N-DOTRIACONTANE	18.645	267169	2.253 ug/ml
15) N-TETRATRIACONTANE	19.437	59013	0.611 ug/ml
16) N-HEXATRIACONTANE	20.161	45600	0.593 ug/ml
18) N-TETRACONTANE	21.892	199572	3.108 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110620\
Data File : FG007308.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2020 05:11
Operator : DD\AJ
Sample : L4657-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 07 07:33:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
Quant Title :
QLast Update : Tue Nov 03 02:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

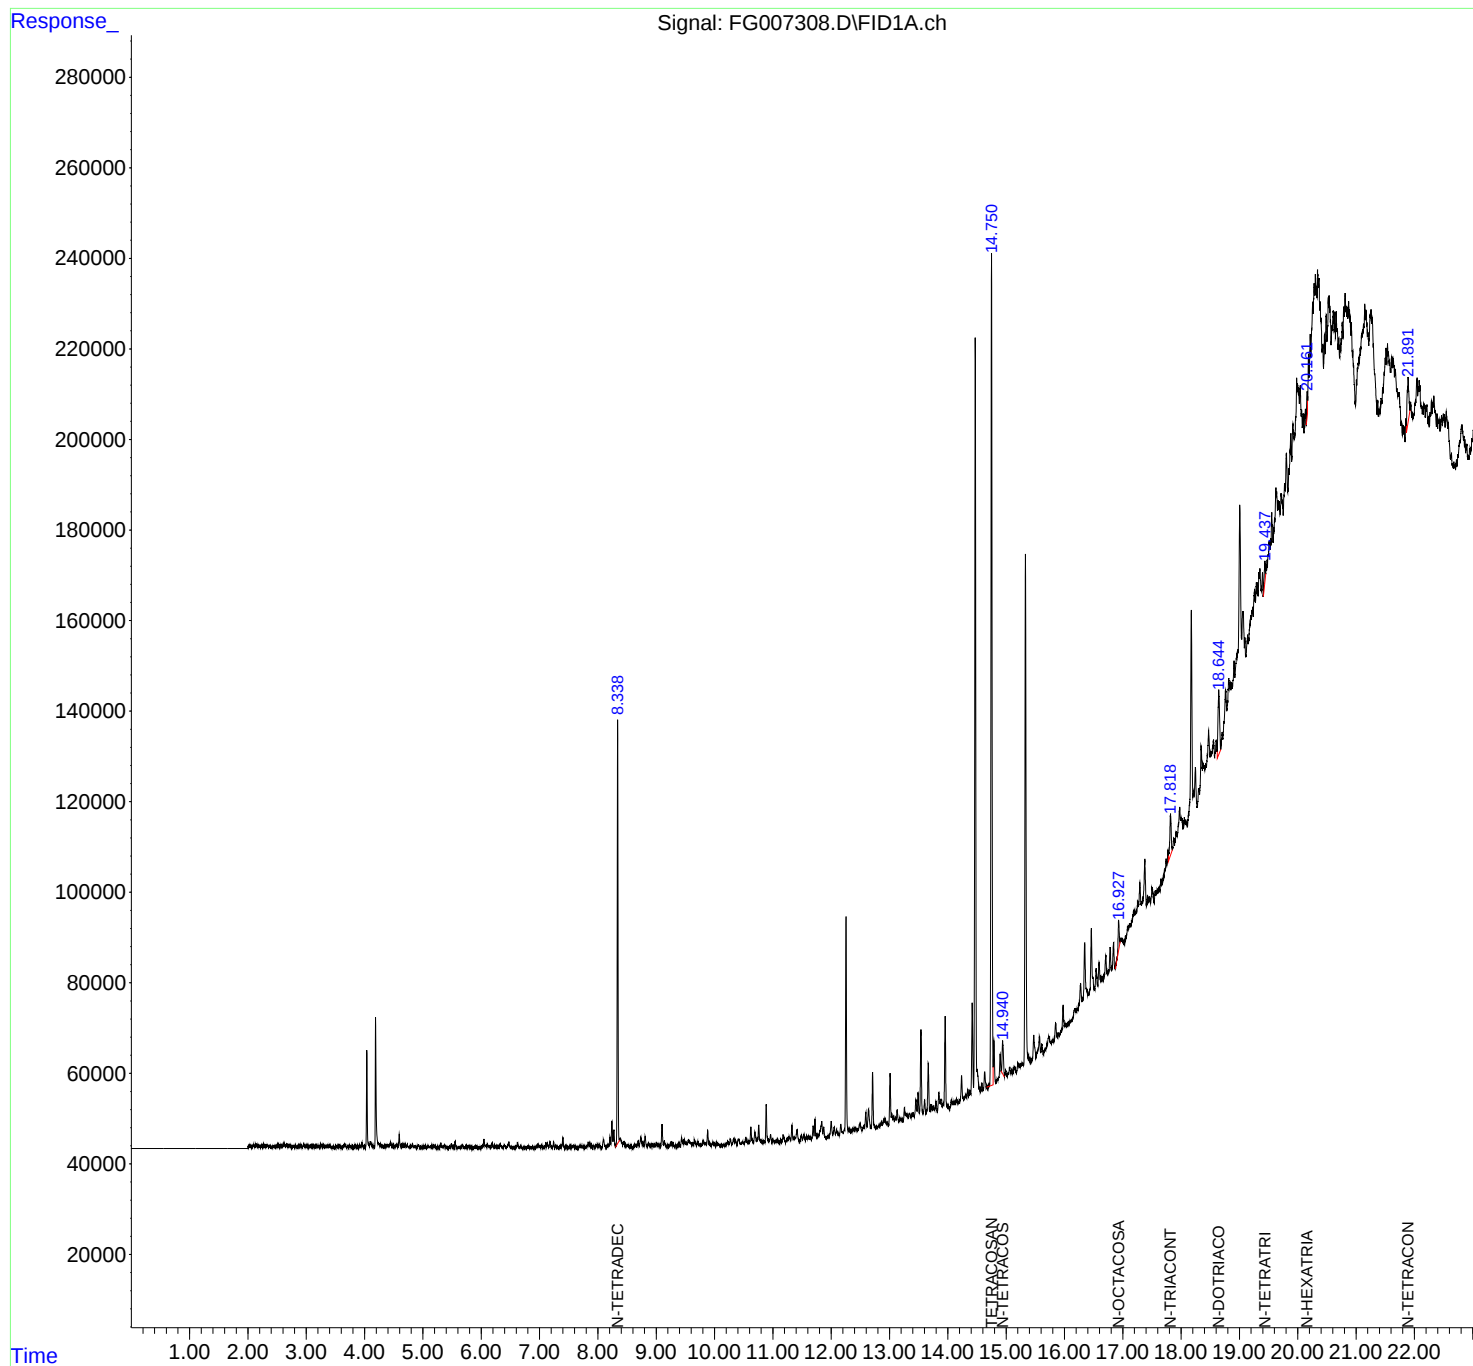


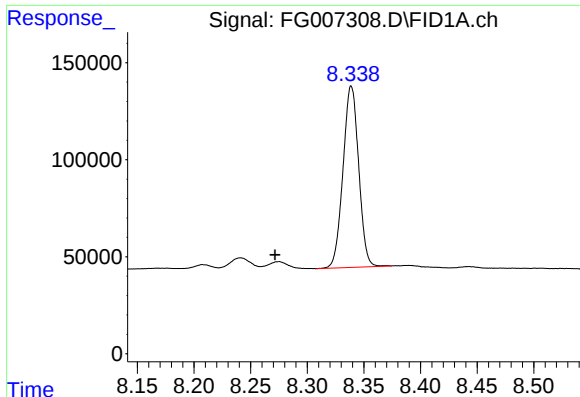

#4 N-TETRADECANE


R.T.: 8.339 min
Delta R.T.: 0.067 min
Response: 899918
Conc: 6.38 ug/ml

Instrument :
FID_G
ClientSampleId :

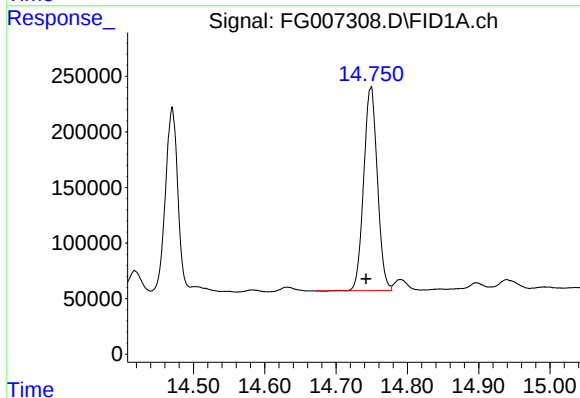


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.749 min
Delta R.T.: 0.007 min
Response: 2440164
Conc: 19.83 ug/ml

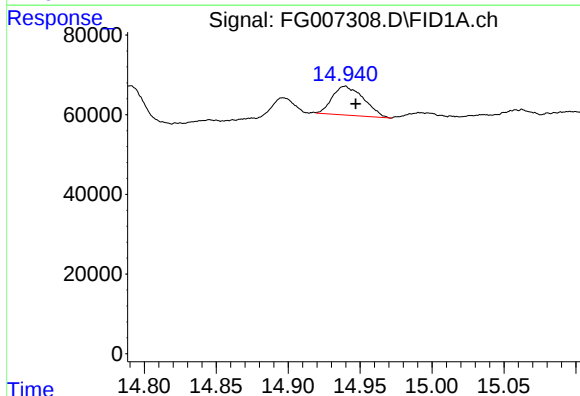


#10 N-TETRACOSANE

R.T.: 14.939 min
Delta R.T.: -0.008 min
Response: 110419
Conc: 0.79 ug/ml

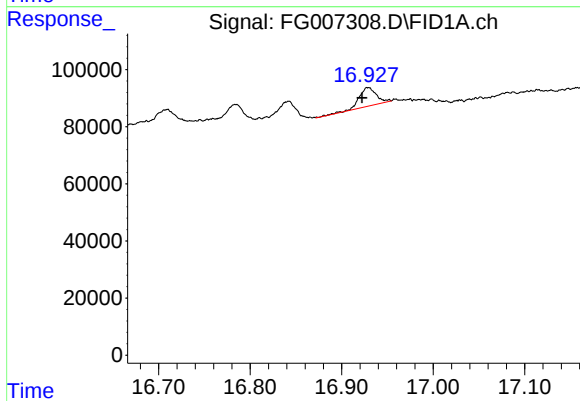

#12 N-OCTACOSANE


R.T.: 16.929 min
Delta R.T.: 0.007 min
Response: 84896
Conc: 0.64 ug/ml

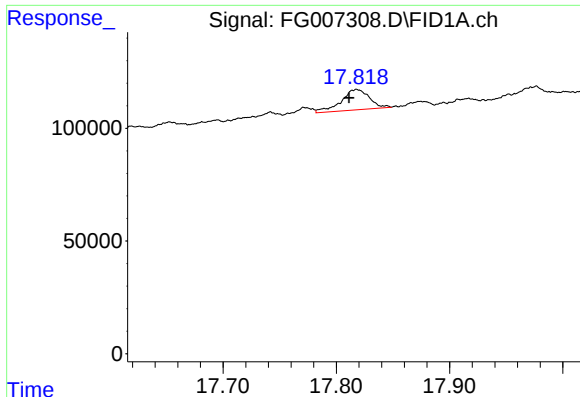

#13 N-TRIACONTANE


R.T.: 17.818 min
Delta R.T.: 0.007 min
Response: 155831
Conc: 1.21 ug/ml

Instrument :
FID_G
ClientSampleId :

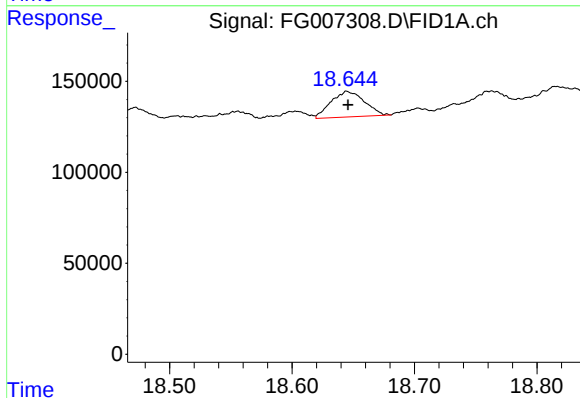


#14 N-DOTRIACONTANE

R.T.: 18.645 min
Delta R.T.: 0.000 min
Response: 267169
Conc: 2.25 ug/ml

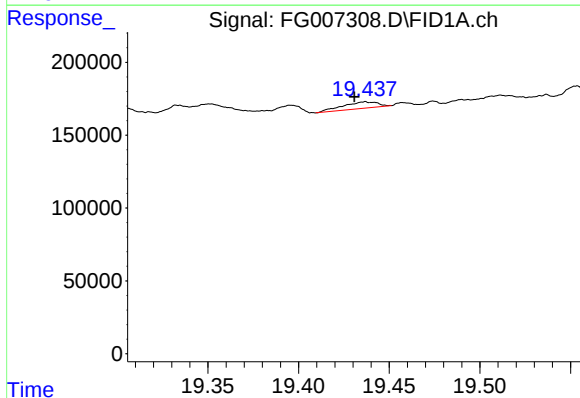


#15 N-TETRATRIACONTANE

R.T.: 19.437 min
Delta R.T.: 0.006 min
Response: 59013
Conc: 0.61 ug/ml

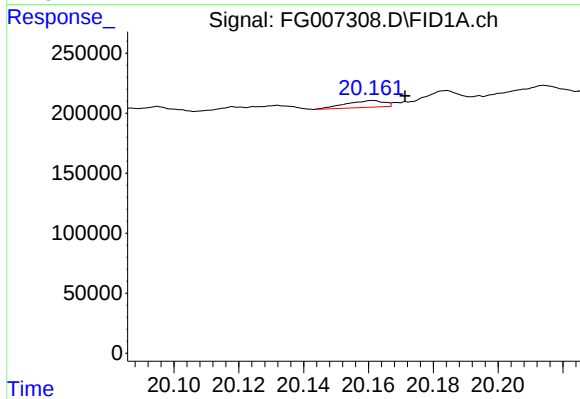

#16 N-HEXATRIACONTANE

R.T.: 20.161 min
Delta R.T.: -0.010 min
Response: 45600
Conc: 0.59 ug/ml

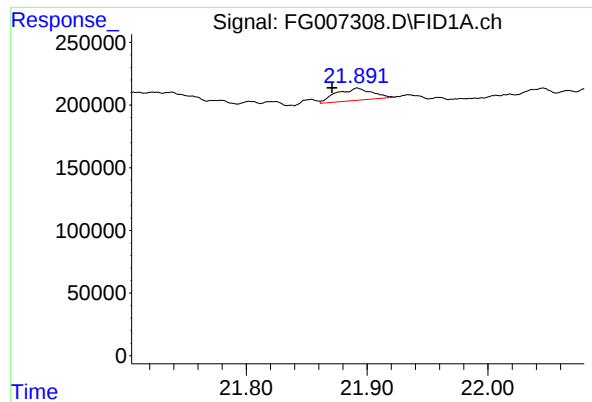

#18 N-TETRACONTANE

R.T.: 21.892 min
Delta R.T.: 0.021 min
Response: 199572
Conc: 3.11 ug/ml

Instrument :
FID_G
ClientSampleId :