

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110620\
 Data File : FG007309.D
 Signal(s) : FID1A.ch
 Acq On : 07 Nov 2020 05:42
 Operator : DD\AJ
 Sample : L4621-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 07 07:33:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
 Quant Title :
 QLast Update : Tue Nov 03 02:04:00 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.746	1651889	13.427 ug/ml
Target Compounds			
4) N-TETRADECANE	8.242	245019	1.738 ug/ml
8) N-DOCOSANE	13.853	102605	0.731 ug/ml
10) N-TETRACOSANE	14.938	331115	2.372 ug/ml
13) N-TRIACONTANE	17.817	112340	0.874 ug/ml
14) N-DOTRIACONTANE	18.648	293674	2.477 ug/ml
15) N-TETRATRIACONTANE	19.440	66801	0.691 ug/ml
16) N-HEXATRIACONTANE	20.178	397648	5.170 ug/ml
18) N-TETRACONTANE	21.922f	489776	7.627 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110620\
Data File : FG007309.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2020 05:42
Operator : DD\AJ
Sample : L4621-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 07 07:33:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110220.M
Quant Title :
QLast Update : Tue Nov 03 02:04:00 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

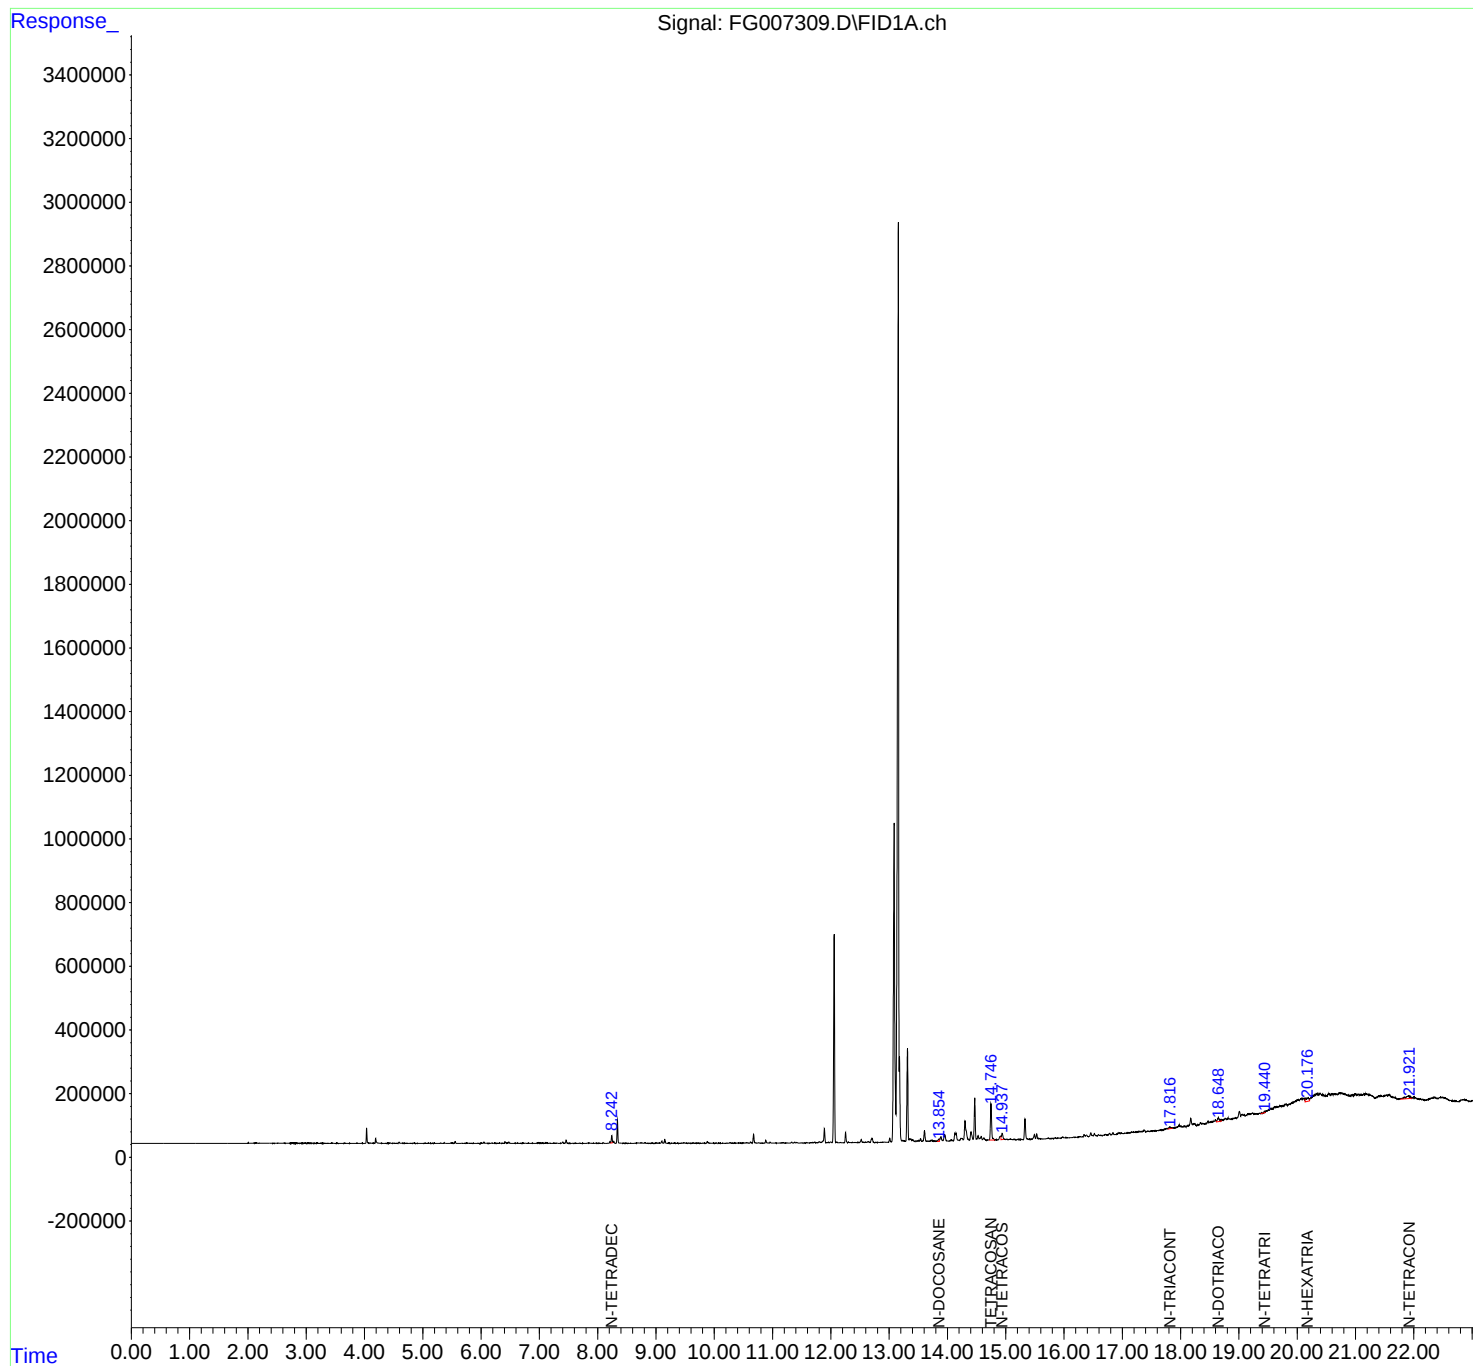


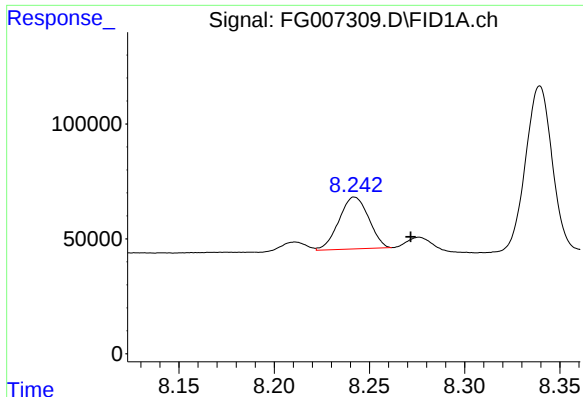

#4 N-TETRADECANE


R.T.: 8.242 min
Delta R.T.: -0.029 min
Response: 245019
Conc: 1.74 ug/ml

Instrument :
FID_G
ClientSampleId :

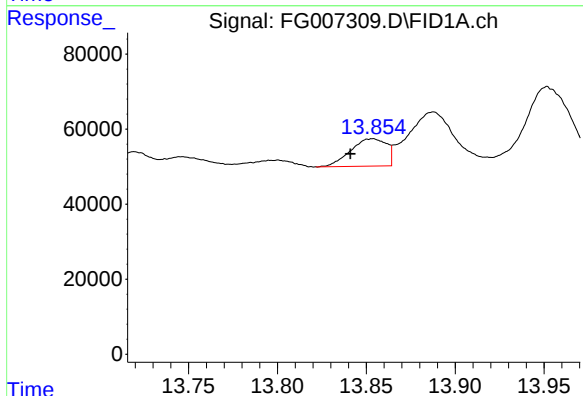


#8 N-DOCOSANE

R.T.: 13.853 min
Delta R.T.: 0.012 min
Response: 102605
Conc: 0.73 ug/ml

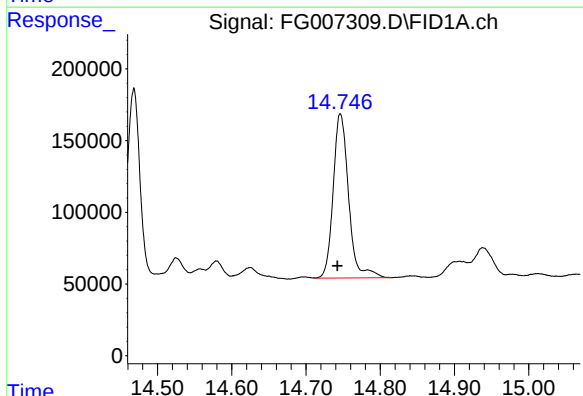


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.746 min
Delta R.T.: 0.004 min
Response: 1651889
Conc: 13.43 ug/ml

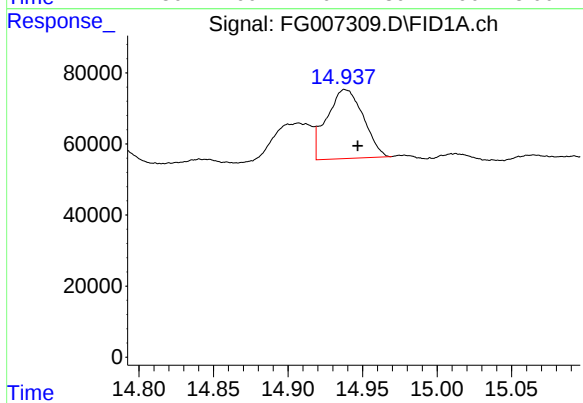

#10 N-TETRACOSANE


R.T.: 14.938 min
Delta R.T.: -0.008 min
Response: 331115
Conc: 2.37 ug/ml

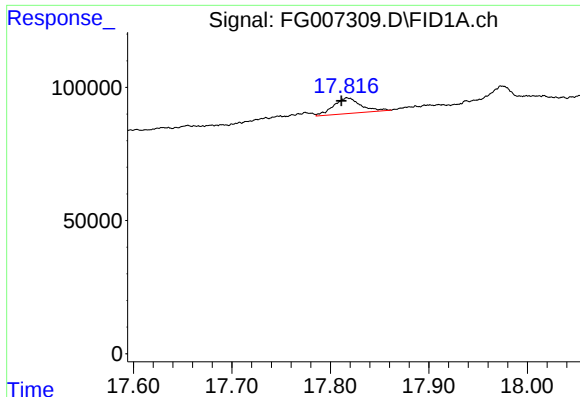

#13 N-TRIACONTANE


R.T.: 17.817 min
Delta R.T.: 0.006 min
Response: 112340
Conc: 0.87 ug/ml

Instrument :
FID_G
ClientSampleId :

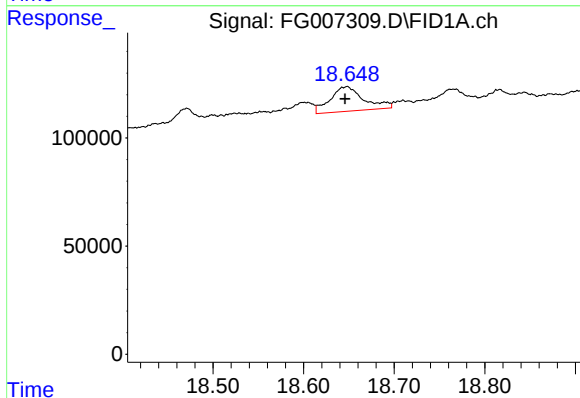


#14 N-DOTRIACONTANE

R.T.: 18.648 min
Delta R.T.: 0.002 min
Response: 293674
Conc: 2.48 ug/ml

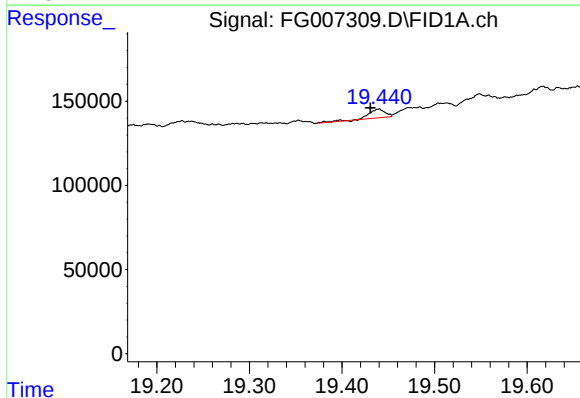


#15 N-TETRATRIACONTANE

R.T.: 19.440 min
Delta R.T.: 0.009 min
Response: 66801
Conc: 0.69 ug/ml

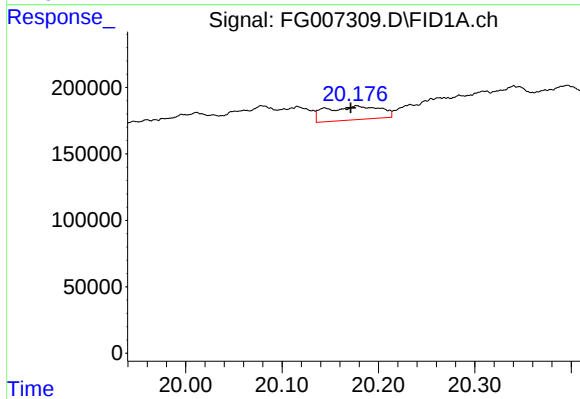

#16 N-HEXATRIACONTANE

R.T.: 20.178 min
Delta R.T.: 0.006 min
Response: 397648
Conc: 5.17 ug/ml

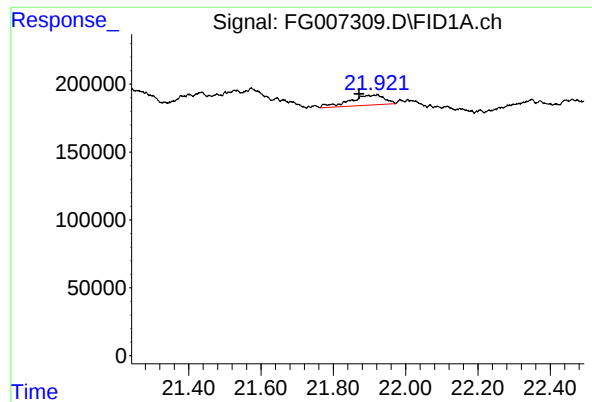

#18 N-TETRACONTANE

R.T.: 21.922 min
Delta R.T.: 0.051 min
Response: 489776
Conc: 7.63 ug/ml

Instrument :
FID_G
ClientSampleId :