

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110724\
Data File : FG014693.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2024 02:48
Operator : YP\AJ
Sample : P4721-15 10X
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 05:28:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102124.M
Quant Title :
QLast Update : Mon Oct 21 17:03:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.046	123950	1.036 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.943	30291	0.229 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110724\
Data File : FG014693.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2024 02:48
Operator : YP\AJ
Sample : P4721-15 10X
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 05:28:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102124.M
Quant Title :
QLast Update : Mon Oct 21 17:03:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

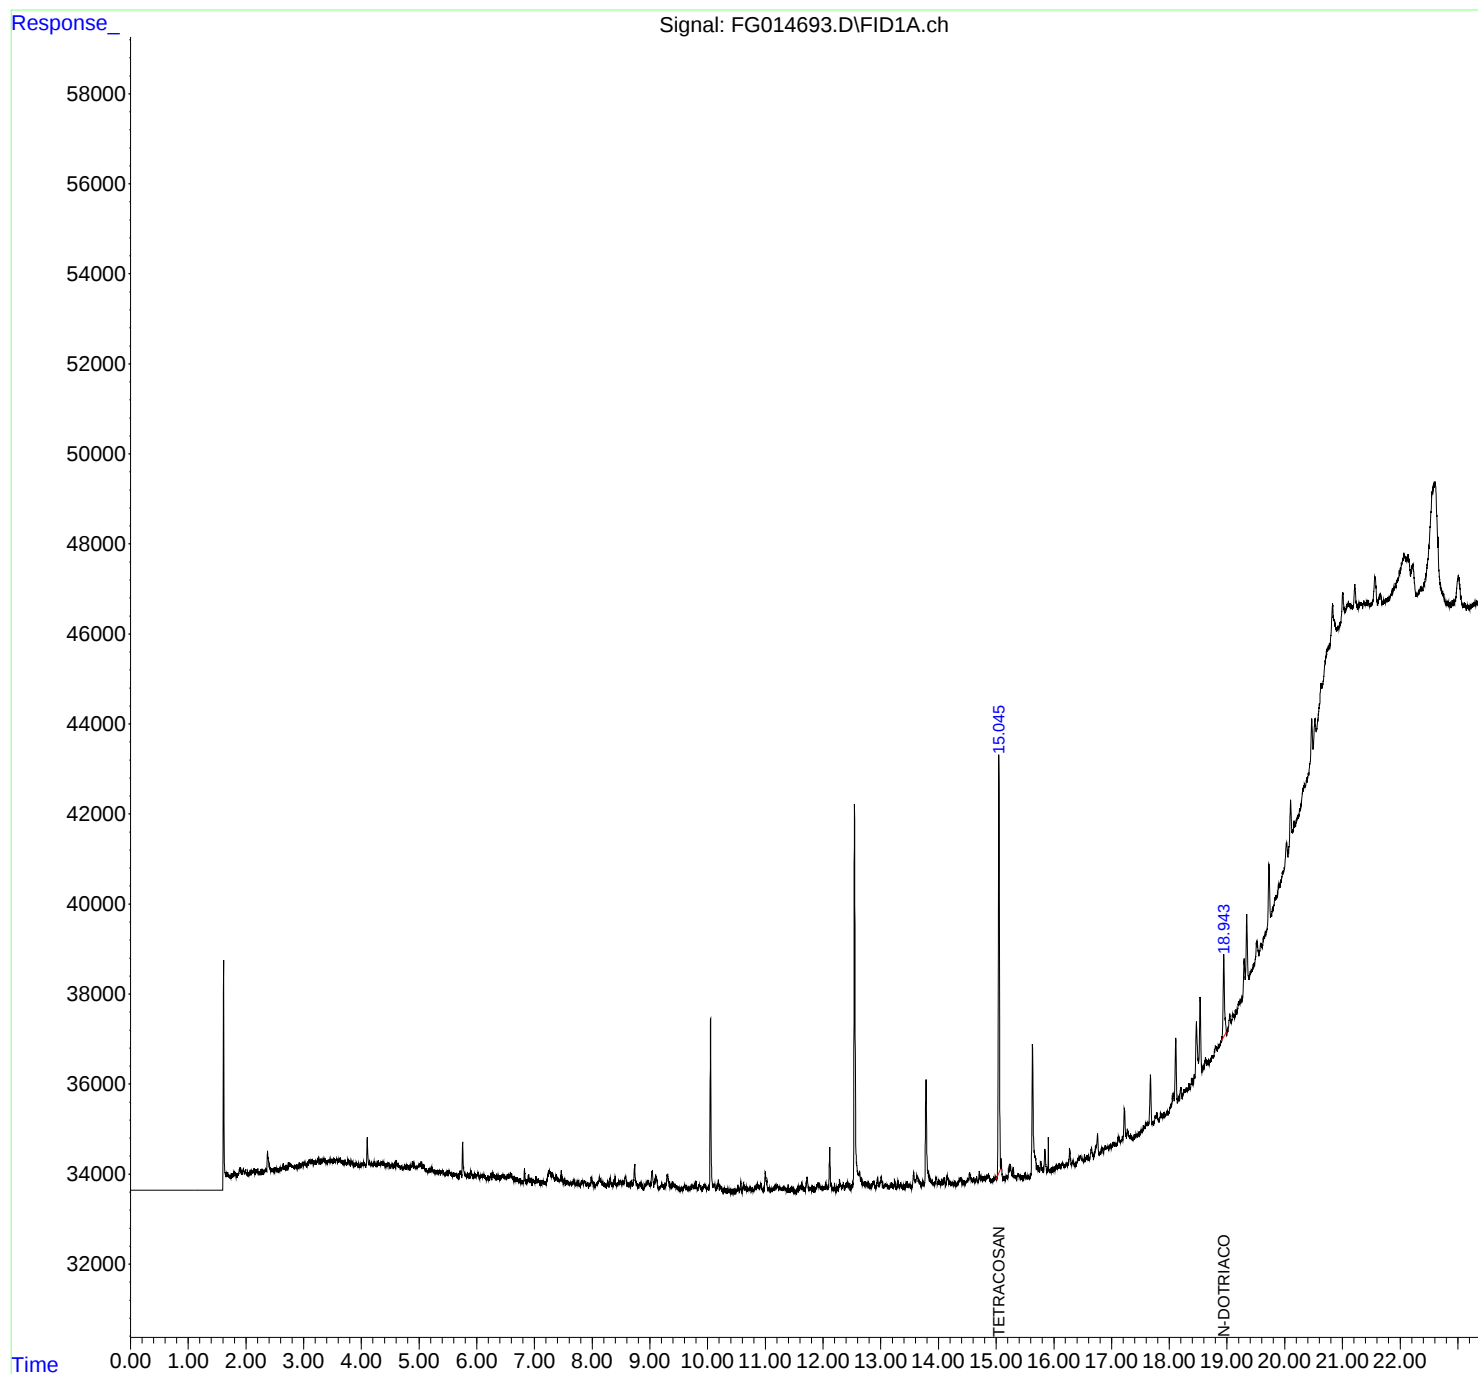

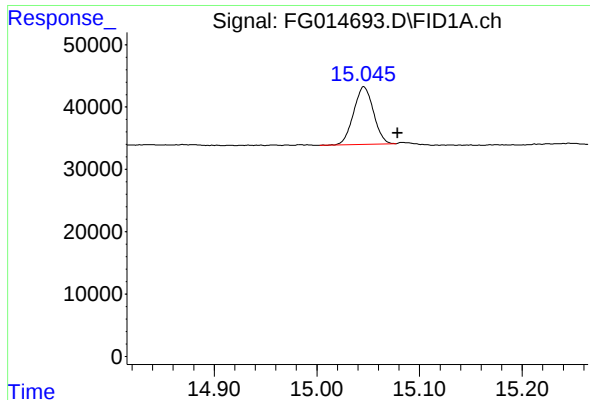


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.046 min
Delta R.T.: -0.033 min
Response: 123950
Conc: 1.04 ug/ml

Instrument :

FID_G

ClientSampleId :

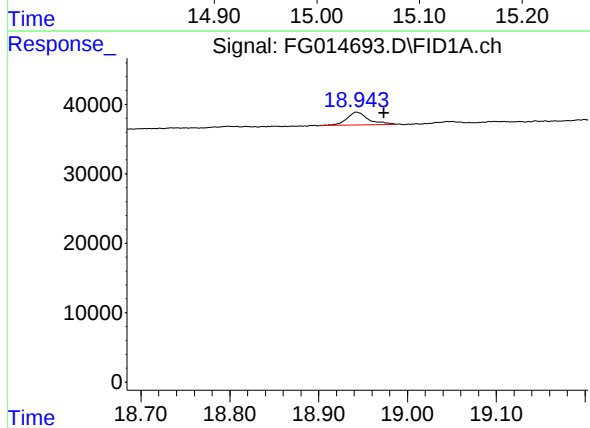

#14 N-DOTRIACONTANE

R.T.: 18.943 min
Delta R.T.: -0.031 min
Response: 30291
Conc: 0.23 ug/ml