

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110724\
 Data File : FG014697.D
 Signal(s) : FID1A.ch
 Acq On : 08 Nov 2024 04:41
 Operator : YP\AJ
 Sample : P4721-04 250X
 Misc :
 ALS Vial : 83 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 08 05:50:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102124.M
 Quant Title :
 QLast Update : Mon Oct 21 17:03:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.762	70732	0.561 ug/ml
4) N-TETRADECANE	8.619	30864	0.240 ug/ml
5) N-HEXADECANE	10.191	112161	0.861 ug/ml
6) N-OCTADECANE	11.724f	257534	1.919 ug/ml
7) N-EICOSANE	12.998	14833	0.109 ug/ml
13) N-TRIACONTANE	18.111	38903	0.291 ug/ml
14) N-DOTRIACONTANE	18.940	30972	0.234 ug/ml
15) N-TETRATRIACONTANE	19.727	36208	0.287 ug/ml
16) N-HEXATRIACONTANE	20.467	23939	0.207 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110724\
Data File : FG014697.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2024 04:41
Operator : YP\AJ
Sample : P4721-04 250X
Misc :
ALS Vial : 83 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 05:50:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102124.M
Quant Title :
QLast Update : Mon Oct 21 17:03:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

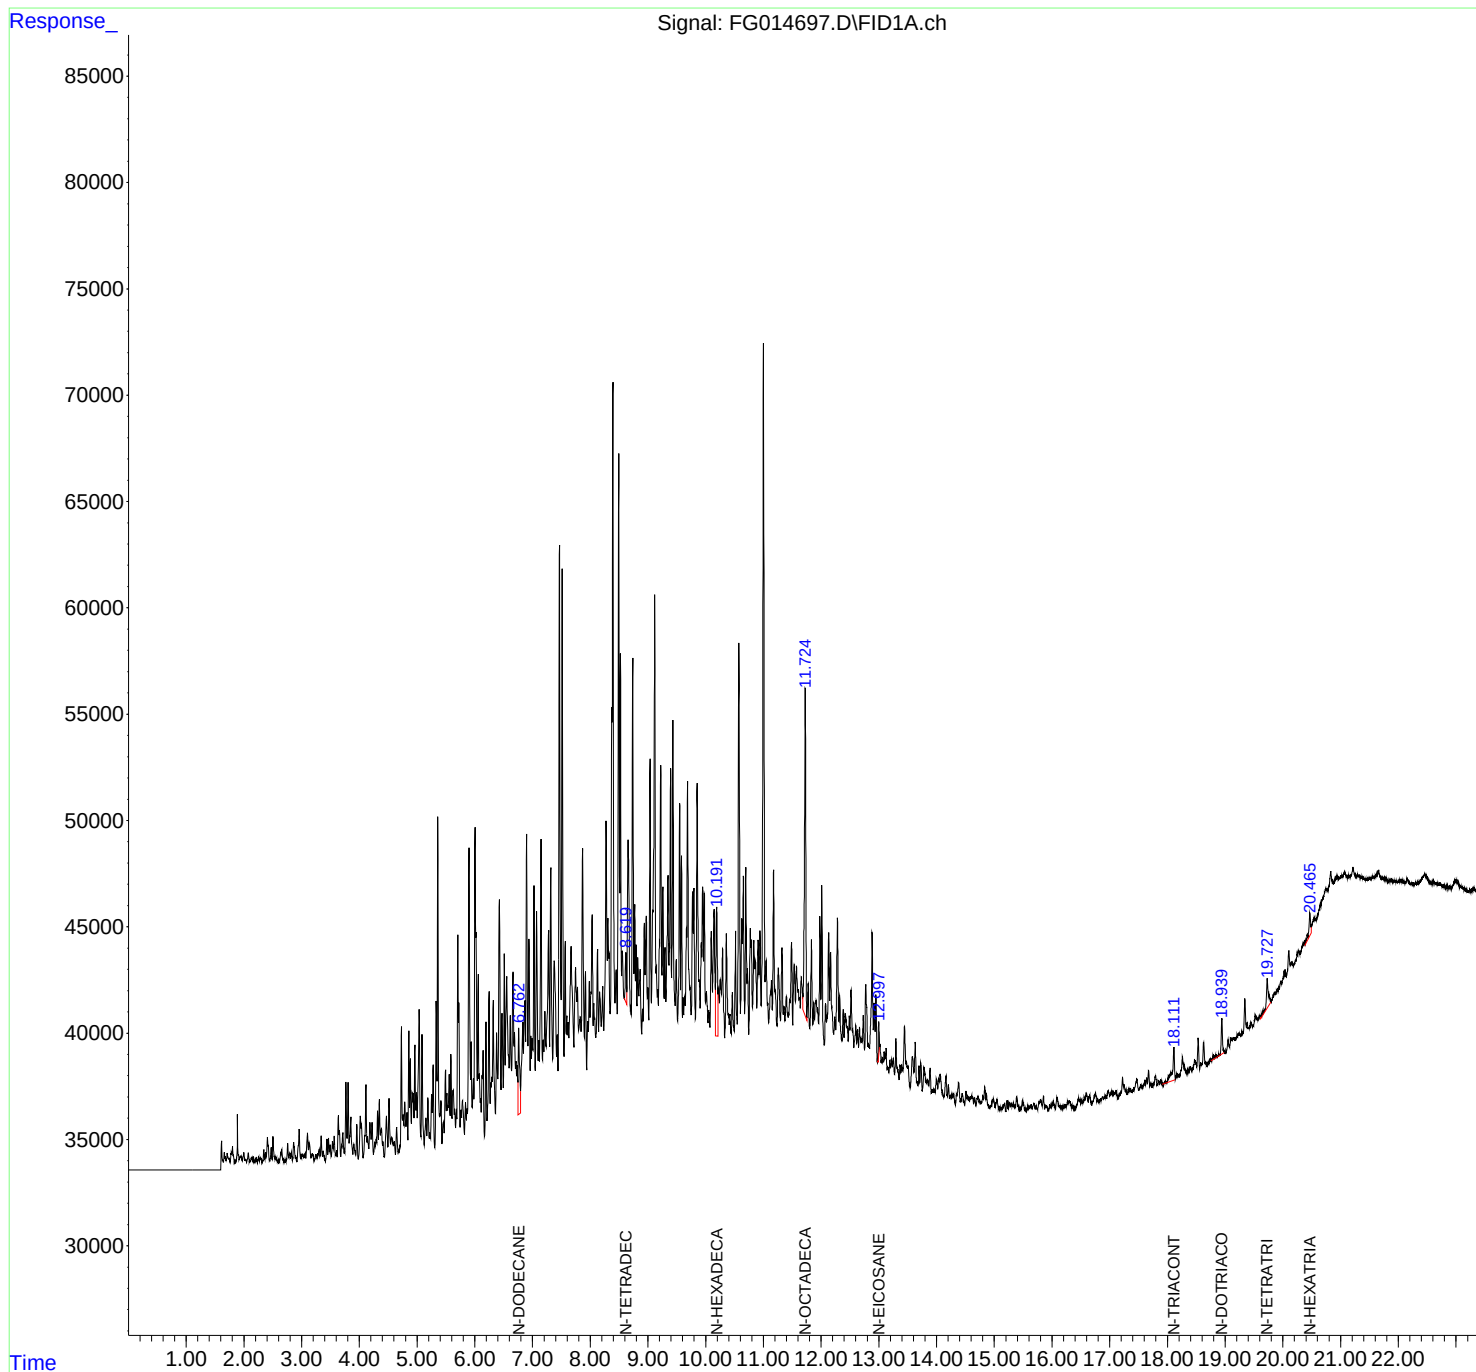


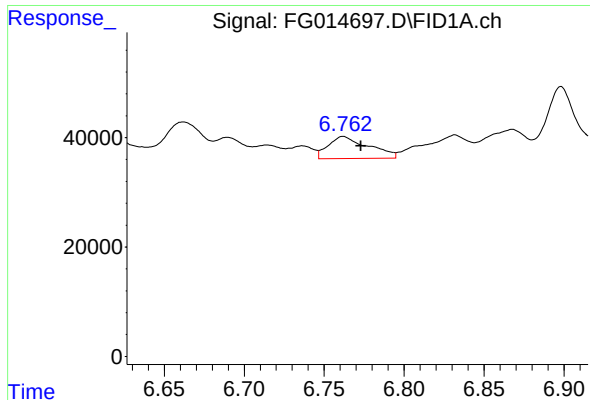

#3 N-DODECANE


R.T.: 6.762 min
Delta R.T.: -0.011 min
Response: 70732
Conc: 0.56 ug/ml

Instrument :
FID_G
ClientSampleId :

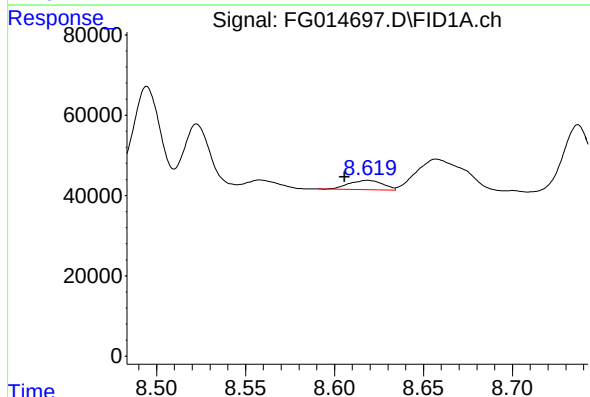


#4 N-TETRADECANE

R.T.: 8.619 min
Delta R.T.: 0.013 min
Response: 30864
Conc: 0.24 ug/ml

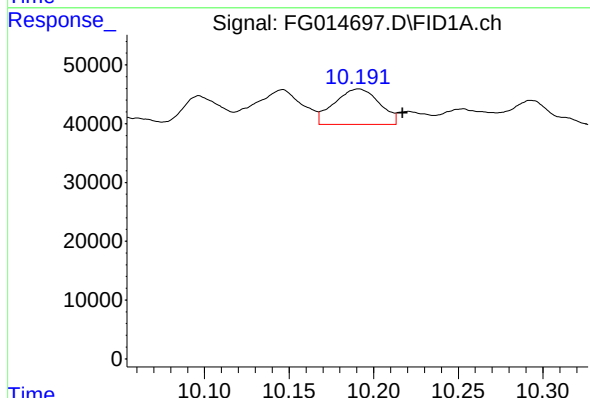


#5 N-HEXADECANE

R.T.: 10.191 min
Delta R.T.: -0.026 min
Response: 112161
Conc: 0.86 ug/ml

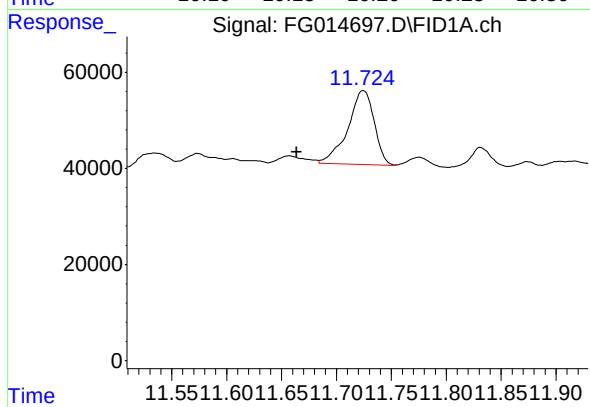

#6 N-OCTADECANE

R.T.: 11.724 min
Delta R.T.: 0.061 min
Response: 257534
Conc: 1.92 ug/ml

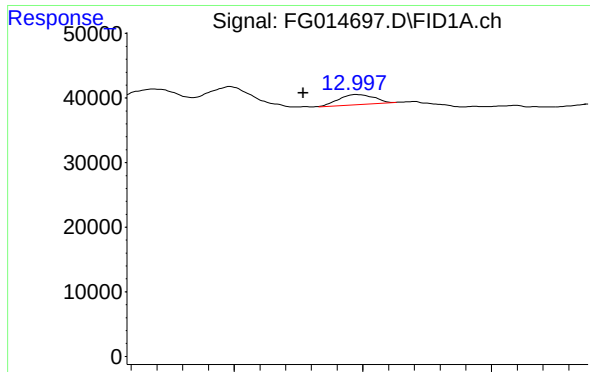


#7 N-EICOSANE

R.T.: 12.998 min
Delta R.T.: 0.021 min
Response: 14833
Conc: 0.11 ug/ml

Instrument :


FID_G

ClientSampleId :

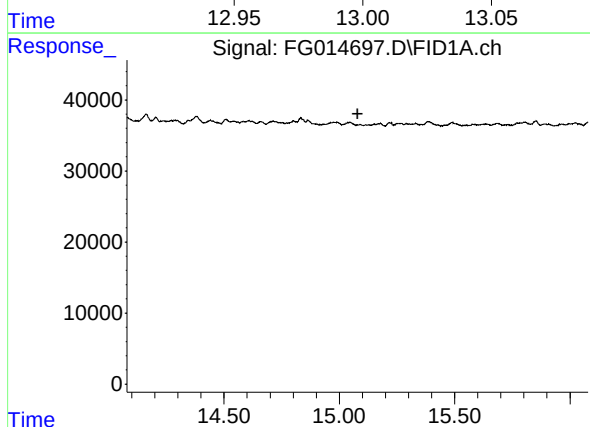


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.079 min
Response: 0
Conc: N.D.

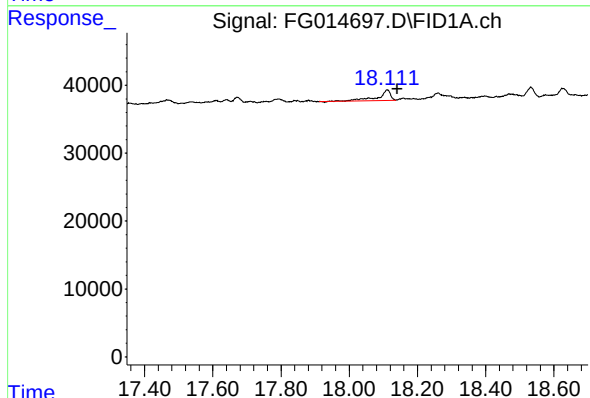


#13 N-TRIACONTANE

R.T.: 18.111 min
Delta R.T.: -0.030 min
Response: 38903
Conc: 0.29 ug/ml

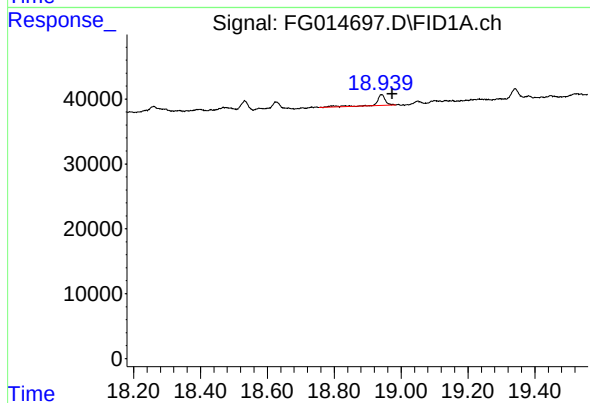

#14 N-DOTRIACONTANE


R.T.: 18.940 min
Delta R.T.: -0.033 min
Response: 30972
Conc: 0.23 ug/ml

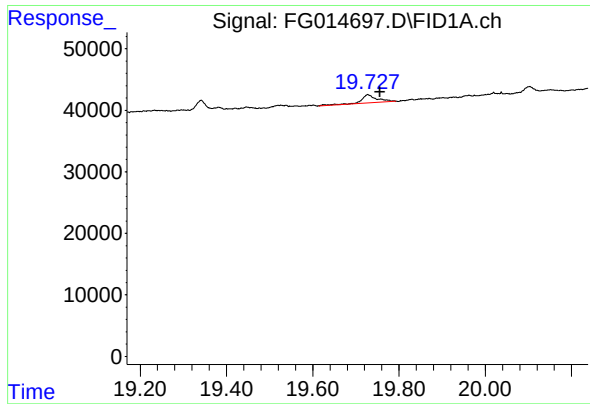

#15 N-TETRATRIACONTANE

R.T.: 19.727 min
Delta R.T.: -0.028 min
Response: 36208
Conc: 0.29 ug/ml

Instrument :
FID_G
ClientSampleId :

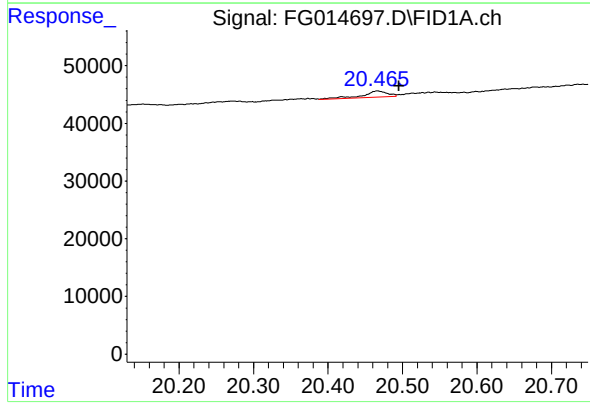

#16 N-HEXATRIACONTANE

R.T.: 20.467 min
Delta R.T.: -0.029 min
Response: 23939
Conc: 0.21 ug/ml