

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110724\
 Data File : FG014682.D
 Signal(s) : FID1A.ch
 Acq On : 07 Nov 2024 20:11
 Operator : YP\AJ
 Sample : PB164744BS
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 PB164744BS

Integration File: autoint1.e
 Quant Time: Nov 08 05:27:07 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102124.M
 Quant Title :
 QLast Update : Mon Oct 21 17:03:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.048	1961445	16.399 ug/ml
Target Compounds			
2) N-DECANE	4.575	2767494	22.351 ug/ml
3) N-DODECANE	6.746	2914163	23.122 ug/ml
4) N-TETRADECANE	8.578	2850283	22.182 ug/ml
5) N-HEXADECANE	10.189	2930059	22.502 ug/ml
6) N-OCTADECANE	11.636	3046978	22.708 ug/ml
7) N-EICOSANE	12.947	2995391	21.970 ug/ml
8) N-DOCOSANE	14.148	2956585	22.270 ug/ml
10) N-TETRACOSANE	15.252	2927990	21.966 ug/ml
11) N-HEXACOSANE	16.273	2852488	21.430 ug/ml
12) N-OCTACOSANE	17.225	2773115	20.911 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110724\
Data File : FG014682.D
Signal(s) : FID1A.ch
Acq On : 07 Nov 2024 20:11
Operator : YP\AJ
Sample : PB164744BS
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB164744BS

Integration File: autoint1.e
Quant Time: Nov 08 05:27:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102124.M
Quant Title :
QLast Update : Mon Oct 21 17:03:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

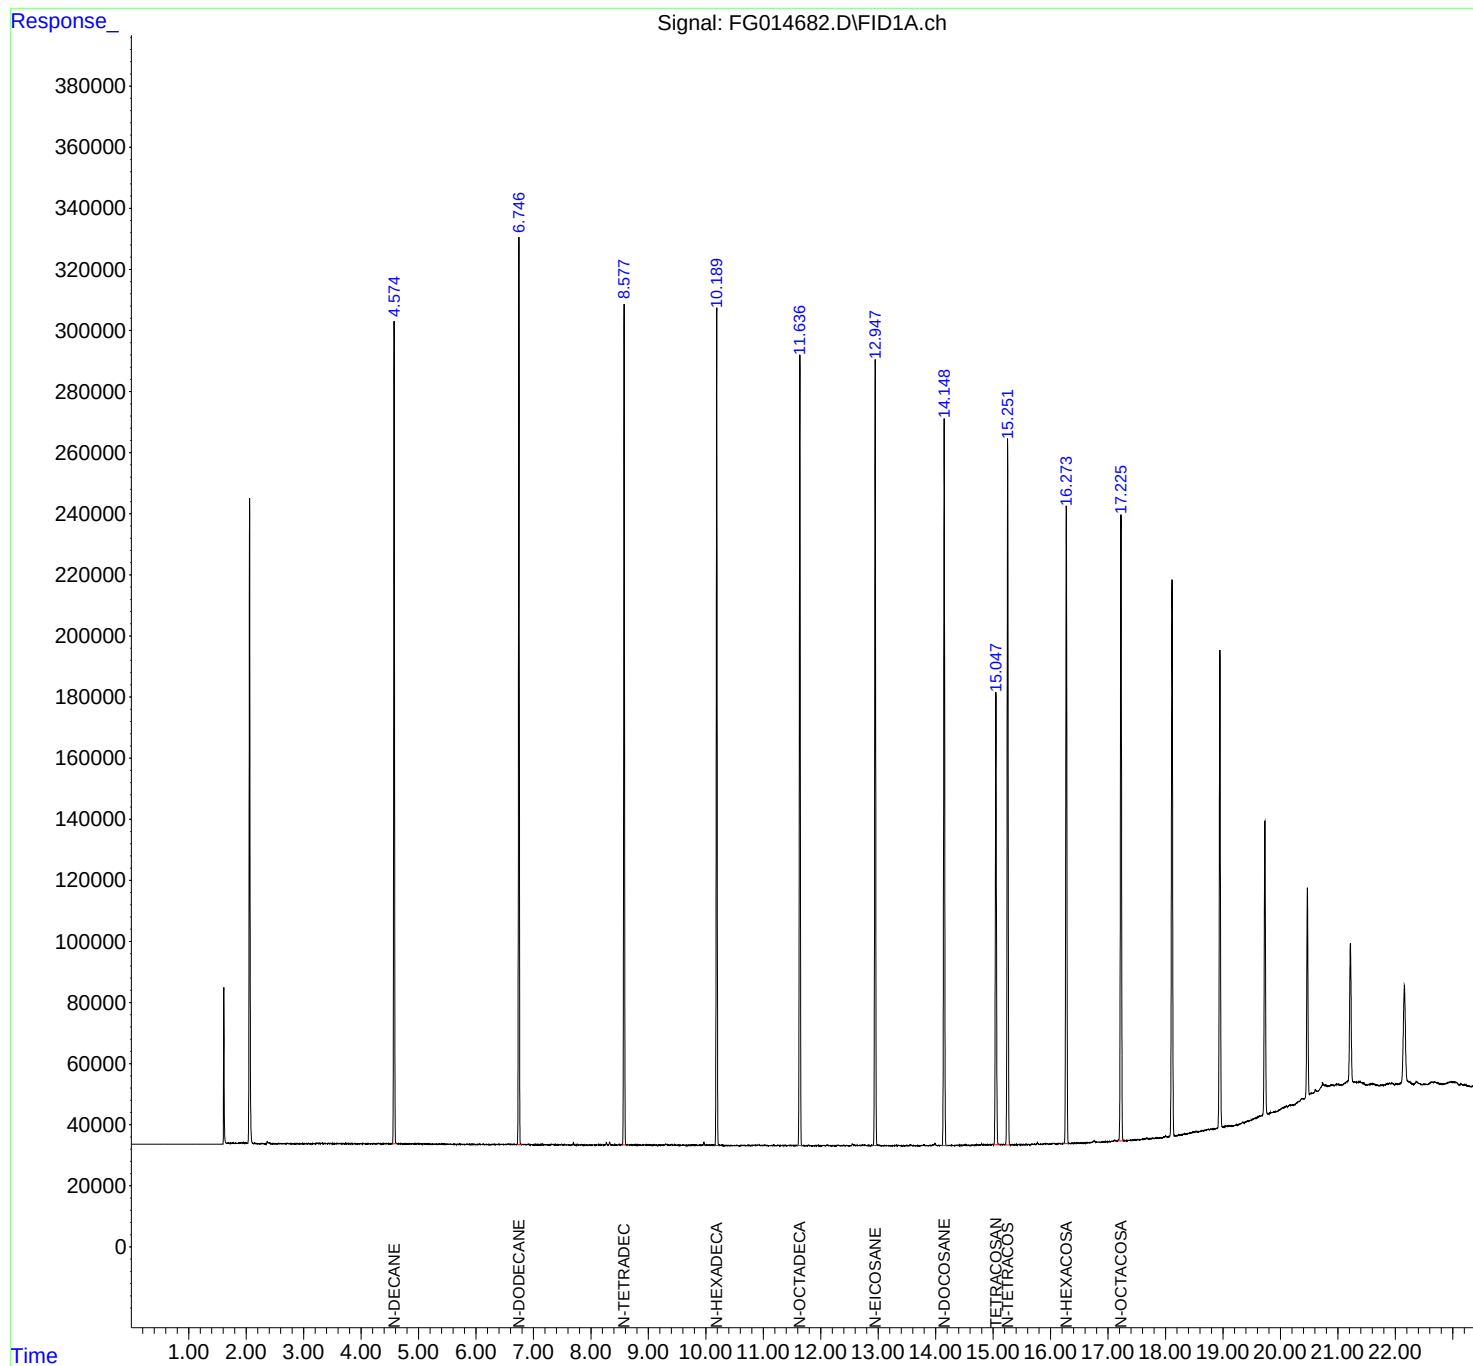


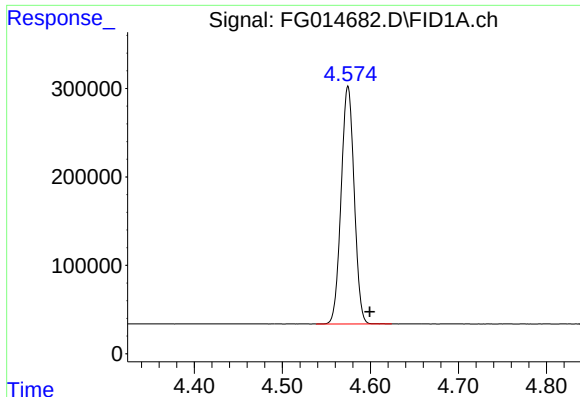

#2 N-DECANE


R.T.: 4.575 min
Delta R.T.: -0.025 min
Response: 2767494
Conc: 22.35 ug/ml

Instrument :
FID_G
ClientSampleId :
PB164744BS

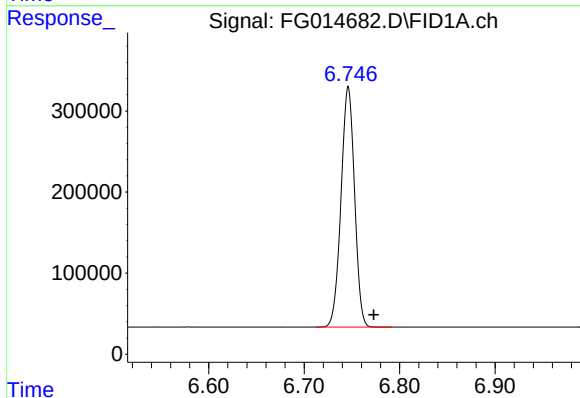


#3 N-DODECANE

R.T.: 6.746 min
Delta R.T.: -0.027 min
Response: 2914163
Conc: 23.12 ug/ml

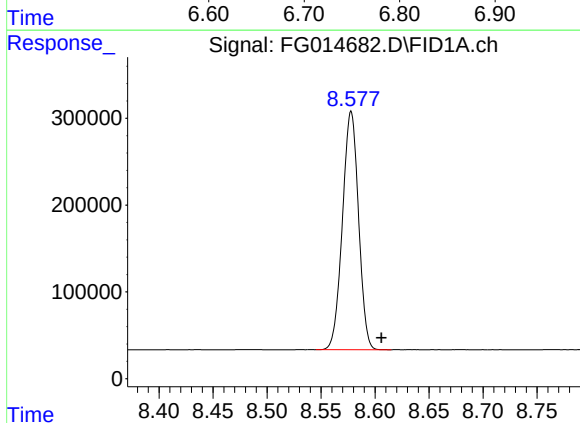


#4 N-TETRADECANE

R.T.: 8.578 min
Delta R.T.: -0.028 min
Response: 2850283
Conc: 22.18 ug/ml

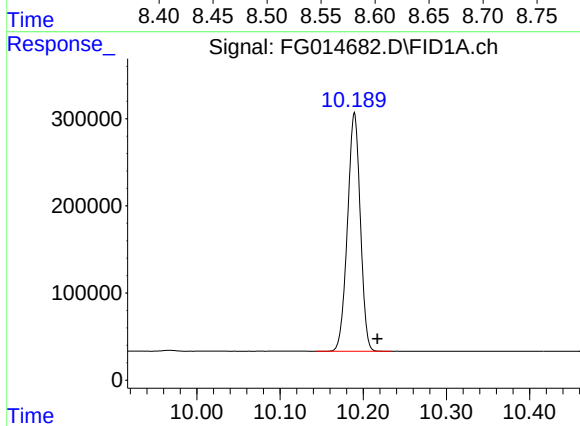

#5 N-HEXADECANE


R.T.: 10.189 min
Delta R.T.: -0.028 min
Response: 2930059
Conc: 22.50 ug/ml

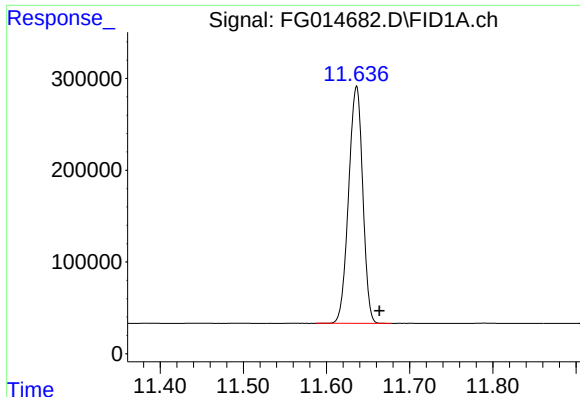

#6 N-OCTADECANE


R.T.: 11.636 min
Delta R.T.: -0.028 min
Response: 3046978
Conc: 22.71 ug/ml

Instrument :
FID_G
ClientSampleId :
PB164744BS

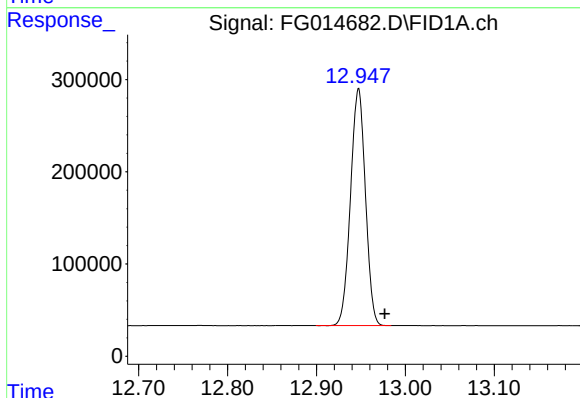


#7 N-EICOSANE

R.T.: 12.947 min
Delta R.T.: -0.030 min
Response: 2995391
Conc: 21.97 ug/ml

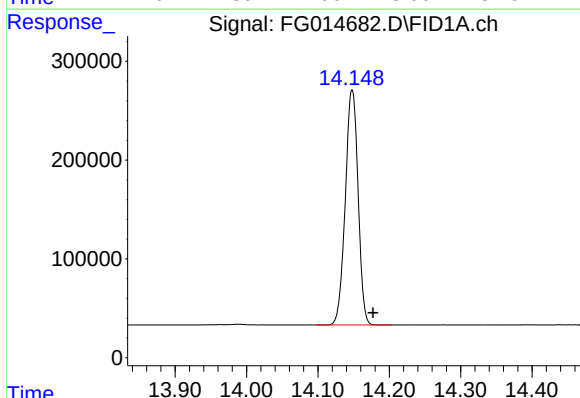


#8 N-DOCOSANE

R.T.: 14.148 min
Delta R.T.: -0.029 min
Response: 2956585
Conc: 22.27 ug/ml

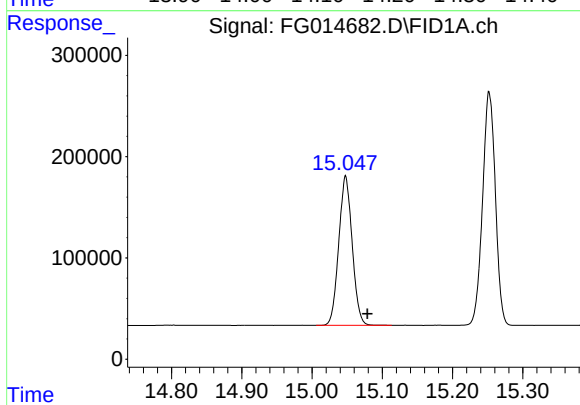

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.048 min
Delta R.T.: -0.031 min
Response: 1961445
Conc: 16.40 ug/ml

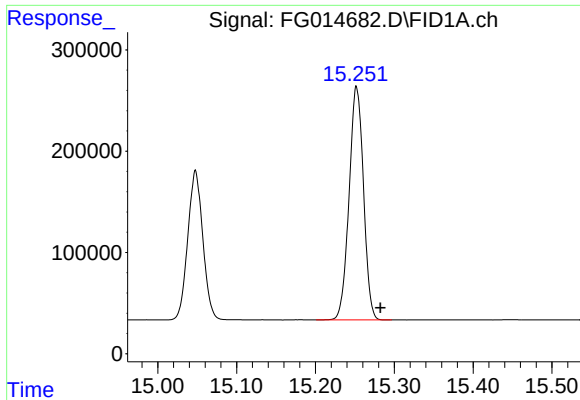

#10 N-TETRACOSANE


R.T.: 15.252 min
Delta R.T.: -0.030 min
Response: 2927990
Conc: 21.97 ug/ml

Instrument :
FID_G
ClientSampleId :
PB164744BS

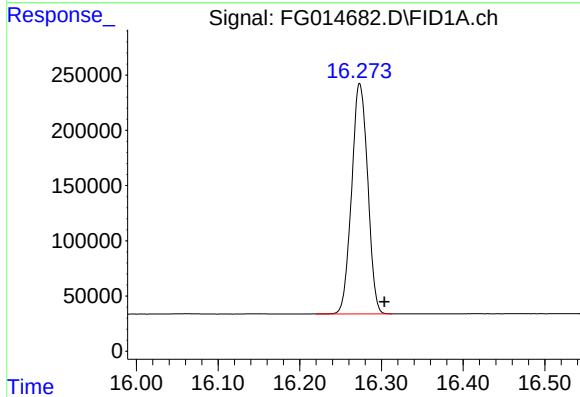

#11 N-HEXACOSANE

R.T.: 16.273 min
Delta R.T.: -0.030 min
Response: 2852488
Conc: 21.43 ug/ml

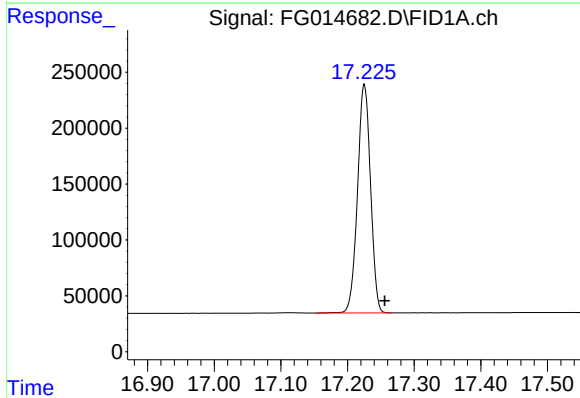

#12 N-OCTACOSANE

R.T.: 17.225 min
Delta R.T.: -0.030 min
Response: 2773115
Conc: 20.91 ug/ml