

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110818\
 Data File : FG002813.D
 Signal(s) : FID1A.ch
 Acq On : 08 Nov 2018 09:25
 Operator : AJ\SJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 08 14:19:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
 Quant Title :
 QLast Update : Wed Nov 07 10:34:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
9) N-EICOSANE	12.645	1022665	9.058 ug/ml
10) N-TETRACOSANE	14.957	1174610	11.178 ug/ml
11) N-OCTACOSANE	16.944	595792	6.039 ug/ml
12) N-DOTRIACONTANE	18.670	782112	9.105 ug/ml
14) N-HEXATRIACONTANE	20.207	353248	5.329 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110818\
Data File : FG002813.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2018 09:25
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 14:19:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
Quant Title :
QLast Update : Wed Nov 07 10:34:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

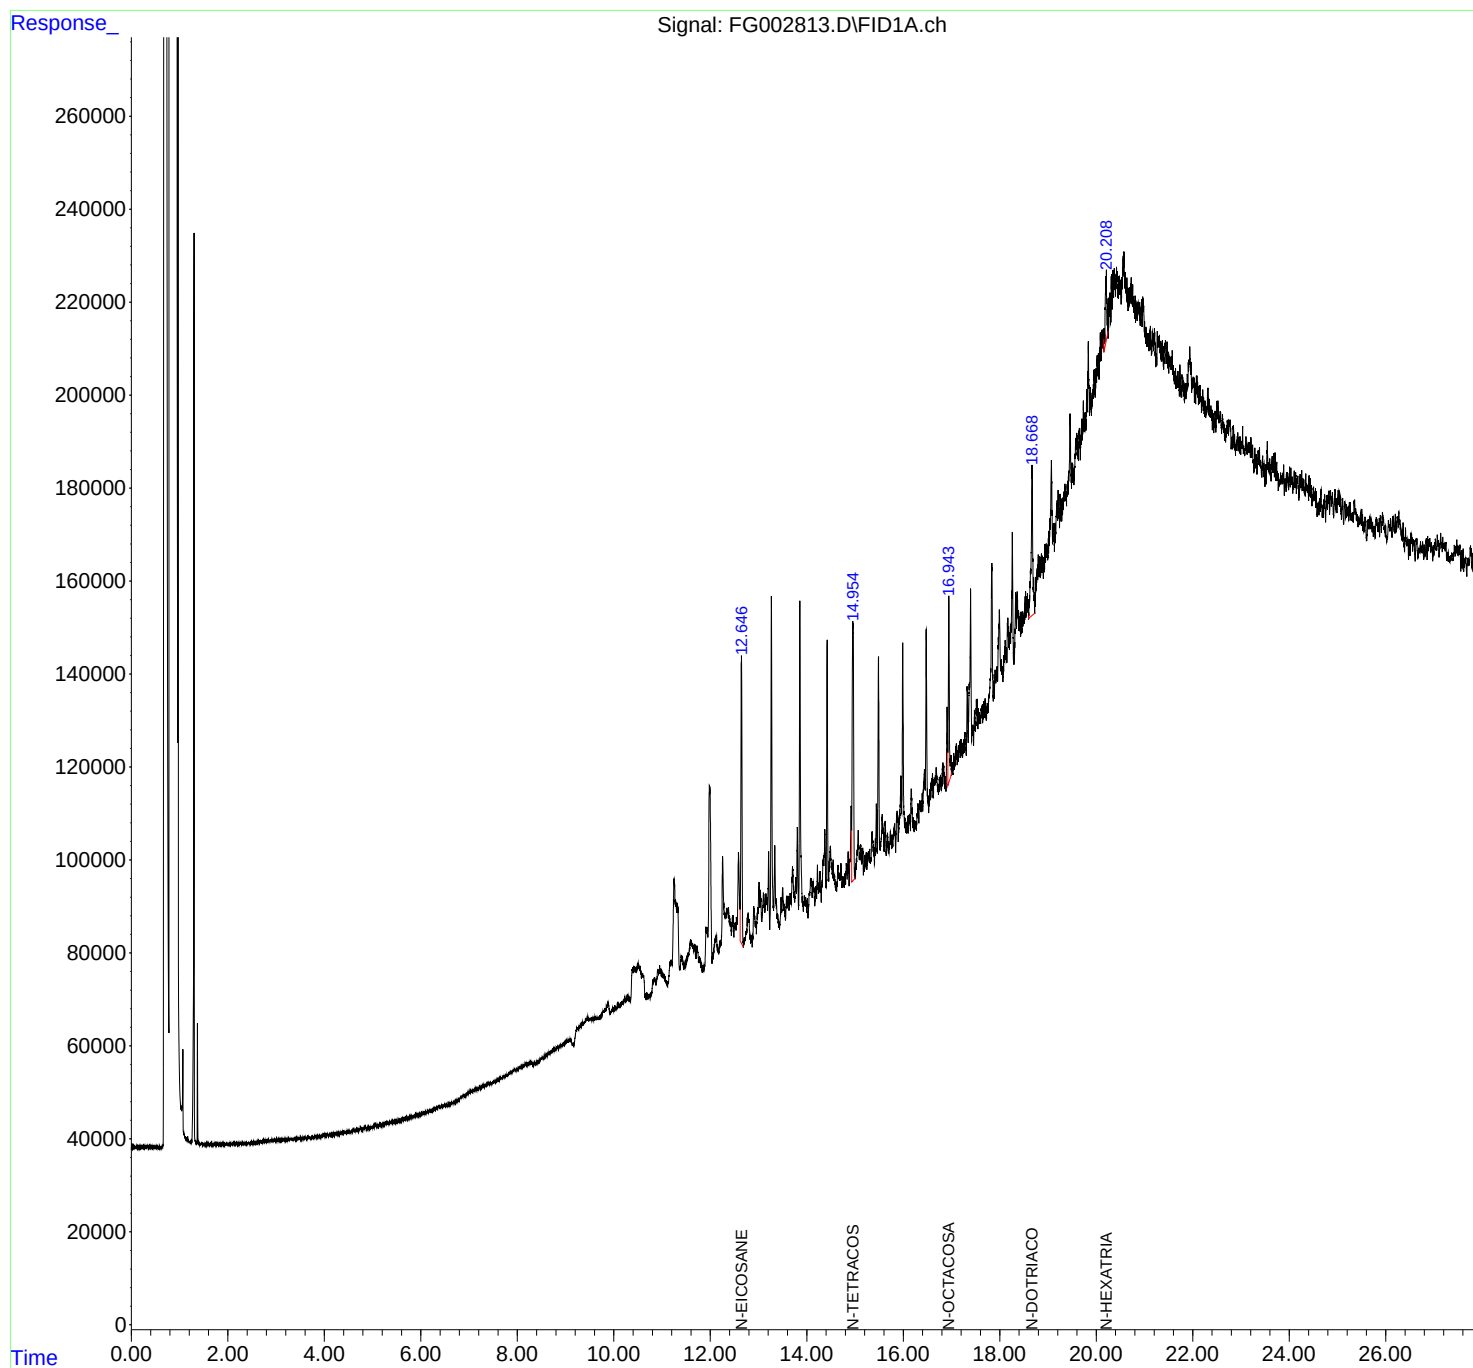


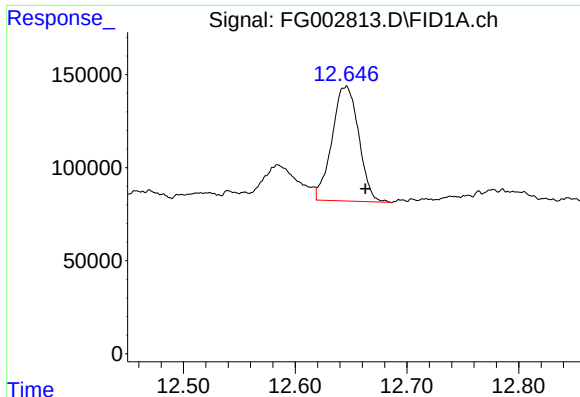

#9 N-EICOSANE


R.T.: 12.645 min
Delta R.T.: -0.018 min
Response: 1022665
Conc: 9.06 ug/ml

Instrument :
FID_G
ClientSampleId :

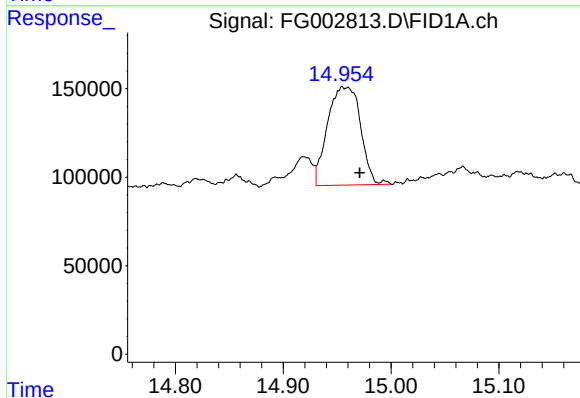


#10 N-TETRACOSANE

R.T.: 14.957 min
Delta R.T.: -0.014 min
Response: 1174610
Conc: 11.18 ug/ml

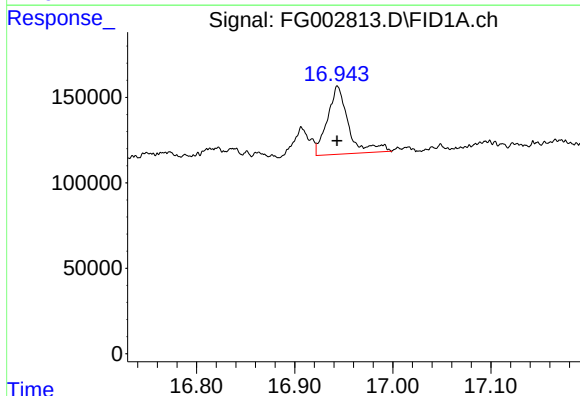


#11 N-OCTACOSANE

R.T.: 16.944 min
Delta R.T.: 0.000 min
Response: 595792
Conc: 6.04 ug/ml

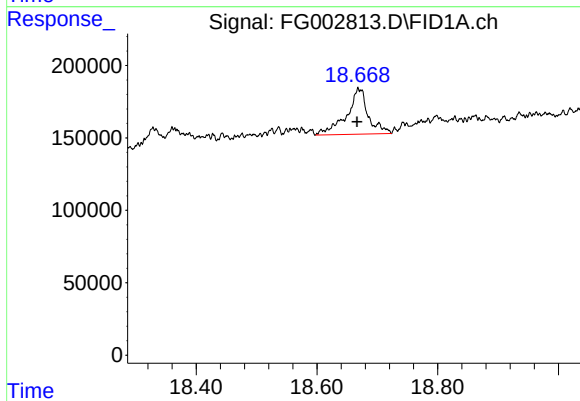

#12 N-DOTRIACONTANE


R.T.: 18.670 min
Delta R.T.: 0.004 min
Response: 782112
Conc: 9.11 ug/ml

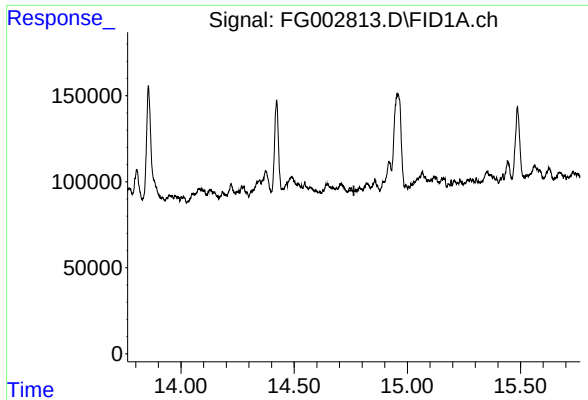

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.764 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

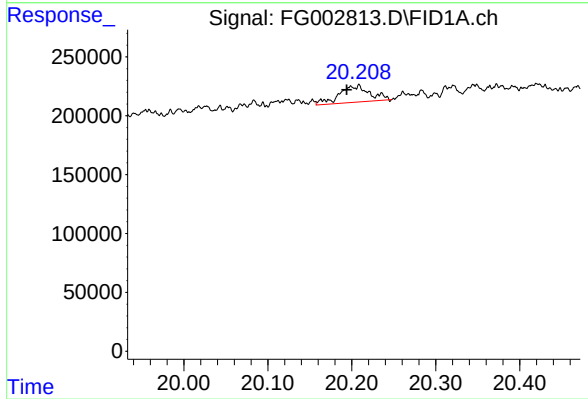

#14 N-HEXATRIACONTANE

R.T.: 20.207 min
Delta R.T.: 0.013 min
Response: 353248
Conc: 5.33 ug/ml