

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110818\
 Data File : FG002817.D
 Signal(s) : FID1A.ch
 Acq On : 08 Nov 2018 11:44
 Operator : AJ\SJ
 Sample : J5827-22 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 08 14:19:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
 Quant Title :
 QLast Update : Wed Nov 07 10:34:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.767	476145	3.874 ug/ml
Target Compounds			
6) N-TETRADECANE	8.361	182919	1.601 ug/ml
9) N-EICOSANE	12.620	338265	2.996 ug/ml
10) N-TETRACOSANE	14.964	682680	6.497 ug/ml
11) N-OCTACOSANE	16.948	177592	1.800 ug/ml
12) N-DOTRIACONTANE	18.675	418083	4.867 ug/ml
14) N-HEXATRIACONTANE	20.203	281900	4.253 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110818\
Data File : FG002817.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2018 11:44
Operator : AJ\SJ
Sample : J5827-22 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 14:19:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
Quant Title :
QLast Update : Wed Nov 07 10:34:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

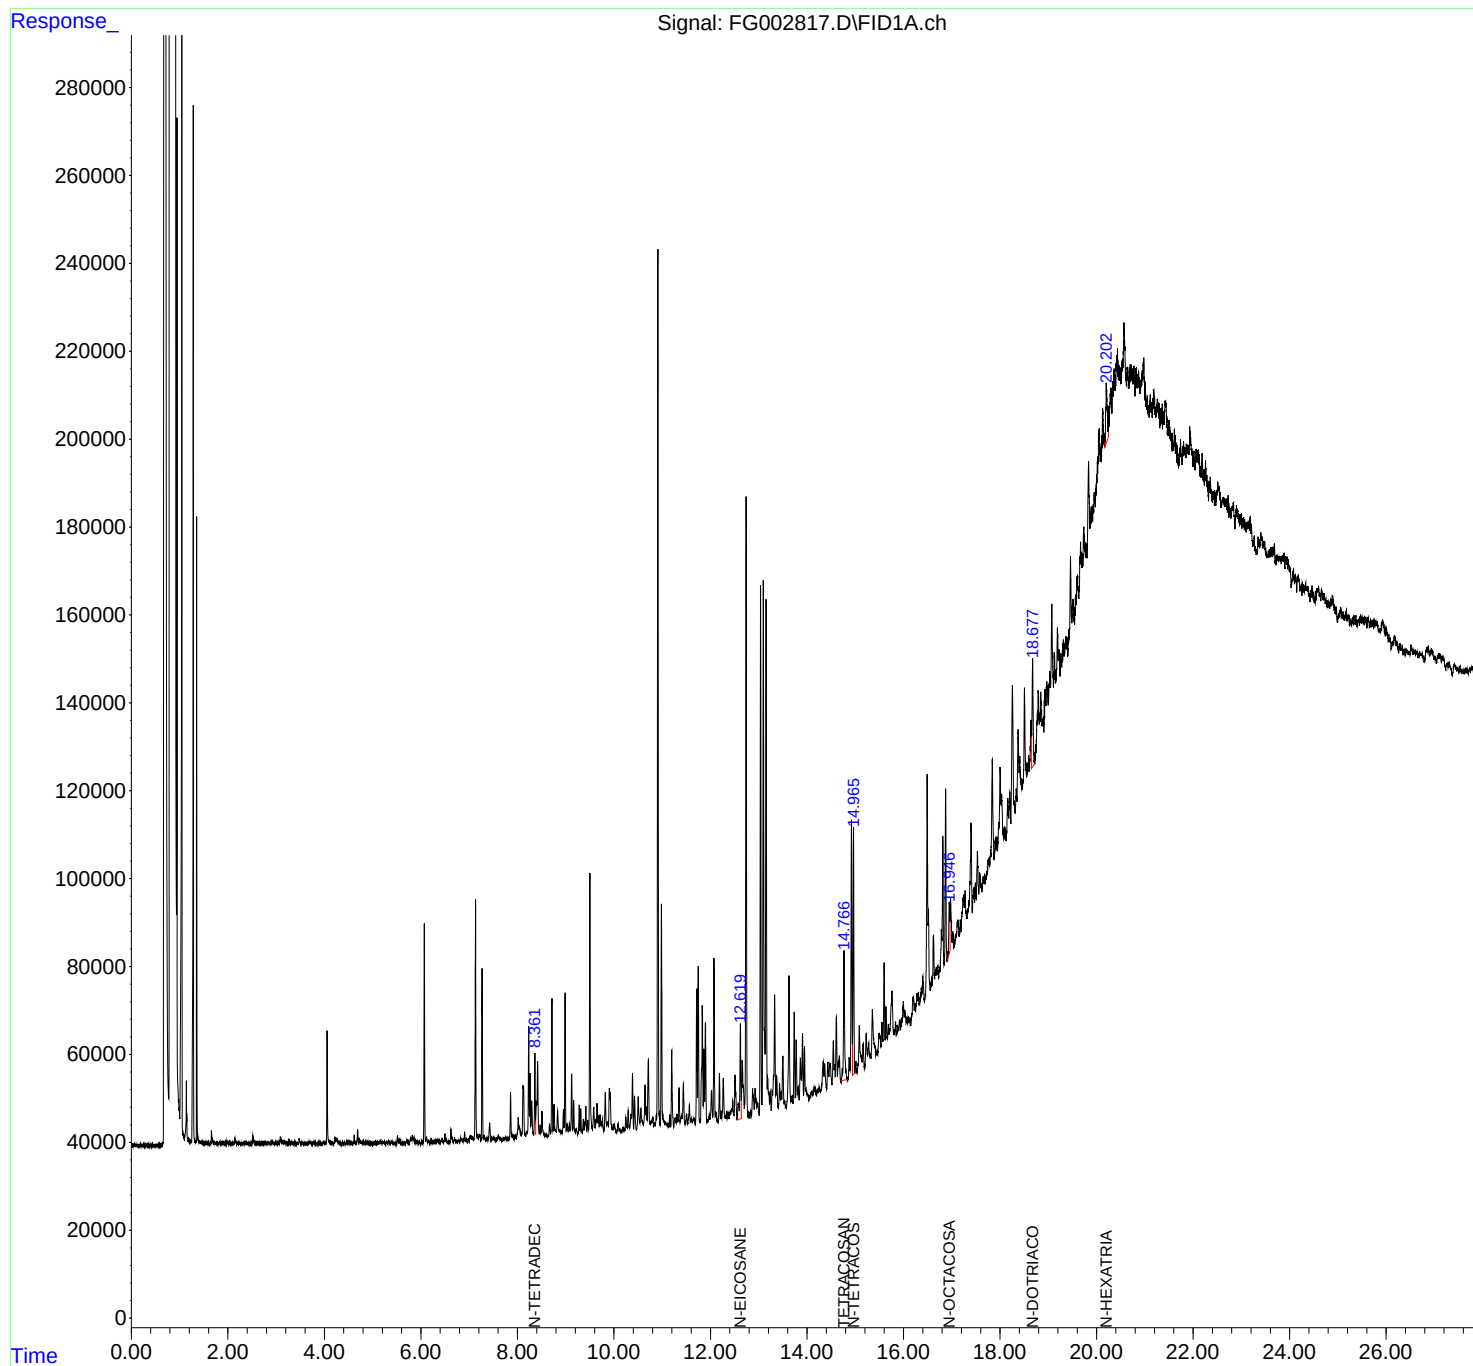


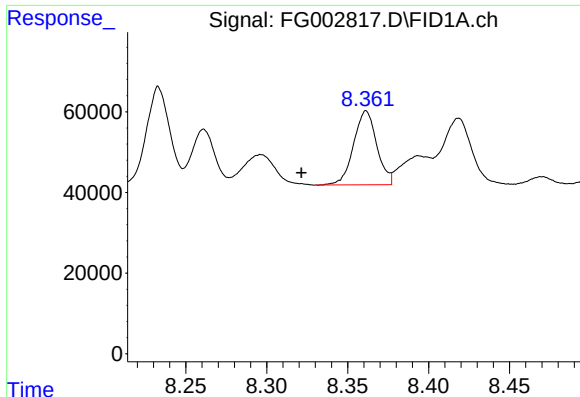

#6 N-TETRADECANE


R.T.: 8.361 min
Delta R.T.: 0.040 min
Response: 182919
Conc: 1.60 ug/ml

Instrument :
FID_G
ClientSampleId :

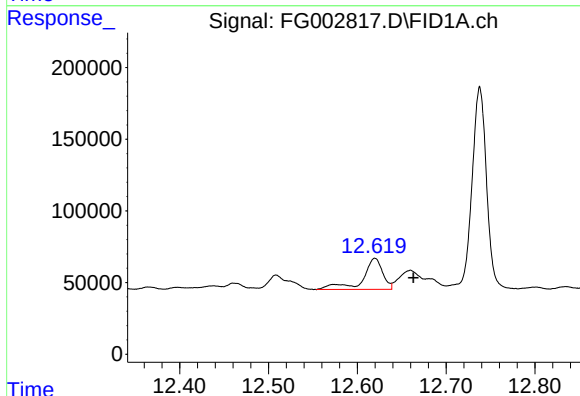


#9 N-EICOSANE

R.T.: 12.620 min
Delta R.T.: -0.043 min
Response: 338265
Conc: 3.00 ug/ml

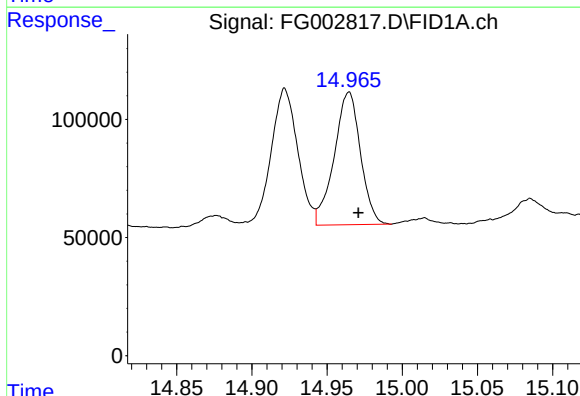


#10 N-TETRACOSANE

R.T.: 14.964 min
Delta R.T.: -0.007 min
Response: 682680
Conc: 6.50 ug/ml

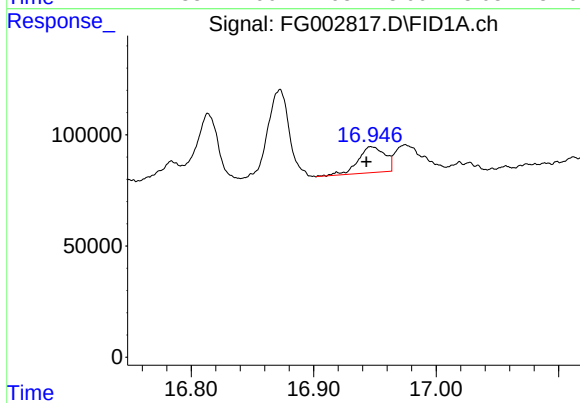

#11 N-OCTACOSANE


R.T.: 16.948 min
Delta R.T.: 0.004 min
Response: 177592
Conc: 1.80 ug/ml

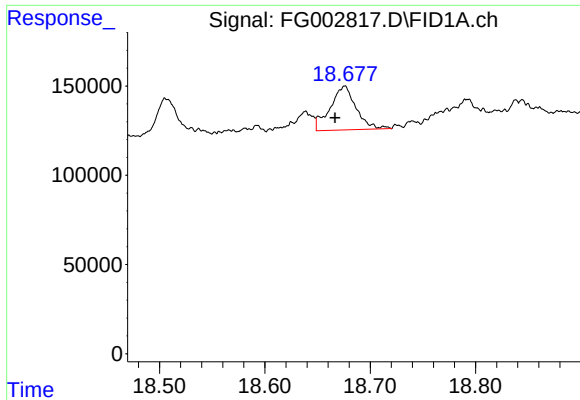

#12 N-DOTRIACONTANE


R.T.: 18.675 min
Delta R.T.: 0.009 min
Response: 418083
Conc: 4.87 ug/ml

Instrument :
FID_G
ClientSampleId :

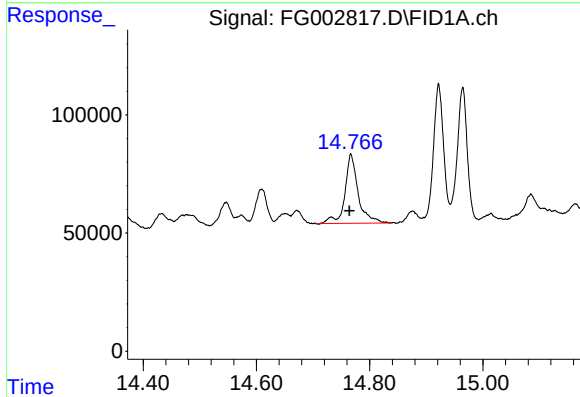

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.767 min
Delta R.T.: 0.003 min
Response: 476145
Conc: 3.87 ug/ml

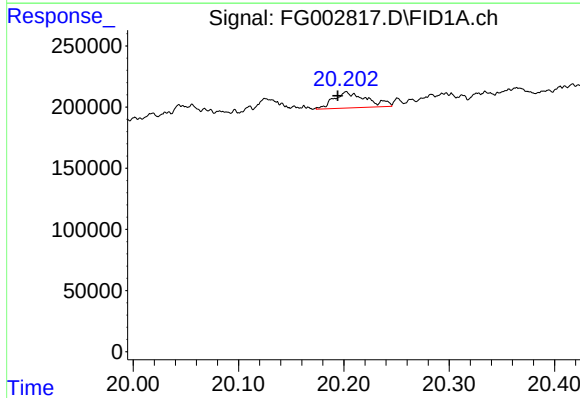

#14 N-HEXATRIACONTANE

R.T.: 20.203 min
Delta R.T.: 0.008 min
Response: 281900
Conc: 4.25 ug/ml