

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110818\
 Data File : FG002821.D
 Signal(s) : FID1A.ch
 Acq On : 08 Nov 2018 14:04
 Operator : AJ\SJ
 Sample : J5827-26 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 08 14:35:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
 Quant Title :
 QLast Update : Wed Nov 07 10:34:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.765	468210	3.810 ug/ml
Target Compounds			
6) N-TETRADECANE	8.359	176602	1.545 ug/ml
9) N-EICOSANE	12.615	319355	2.829 ug/ml
10) N-TETRACOSANE	14.959	654365	6.227 ug/ml
11) N-OCTACOSANE	16.945	156163	1.583 ug/ml
12) N-DOTRIACONTANE	18.673	258661	3.011 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110818\
Data File : FG002821.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2018 14:04
Operator : AJ\SJ
Sample : J5827-26 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 14:35:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
Quant Title :
QLast Update : Wed Nov 07 10:34:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

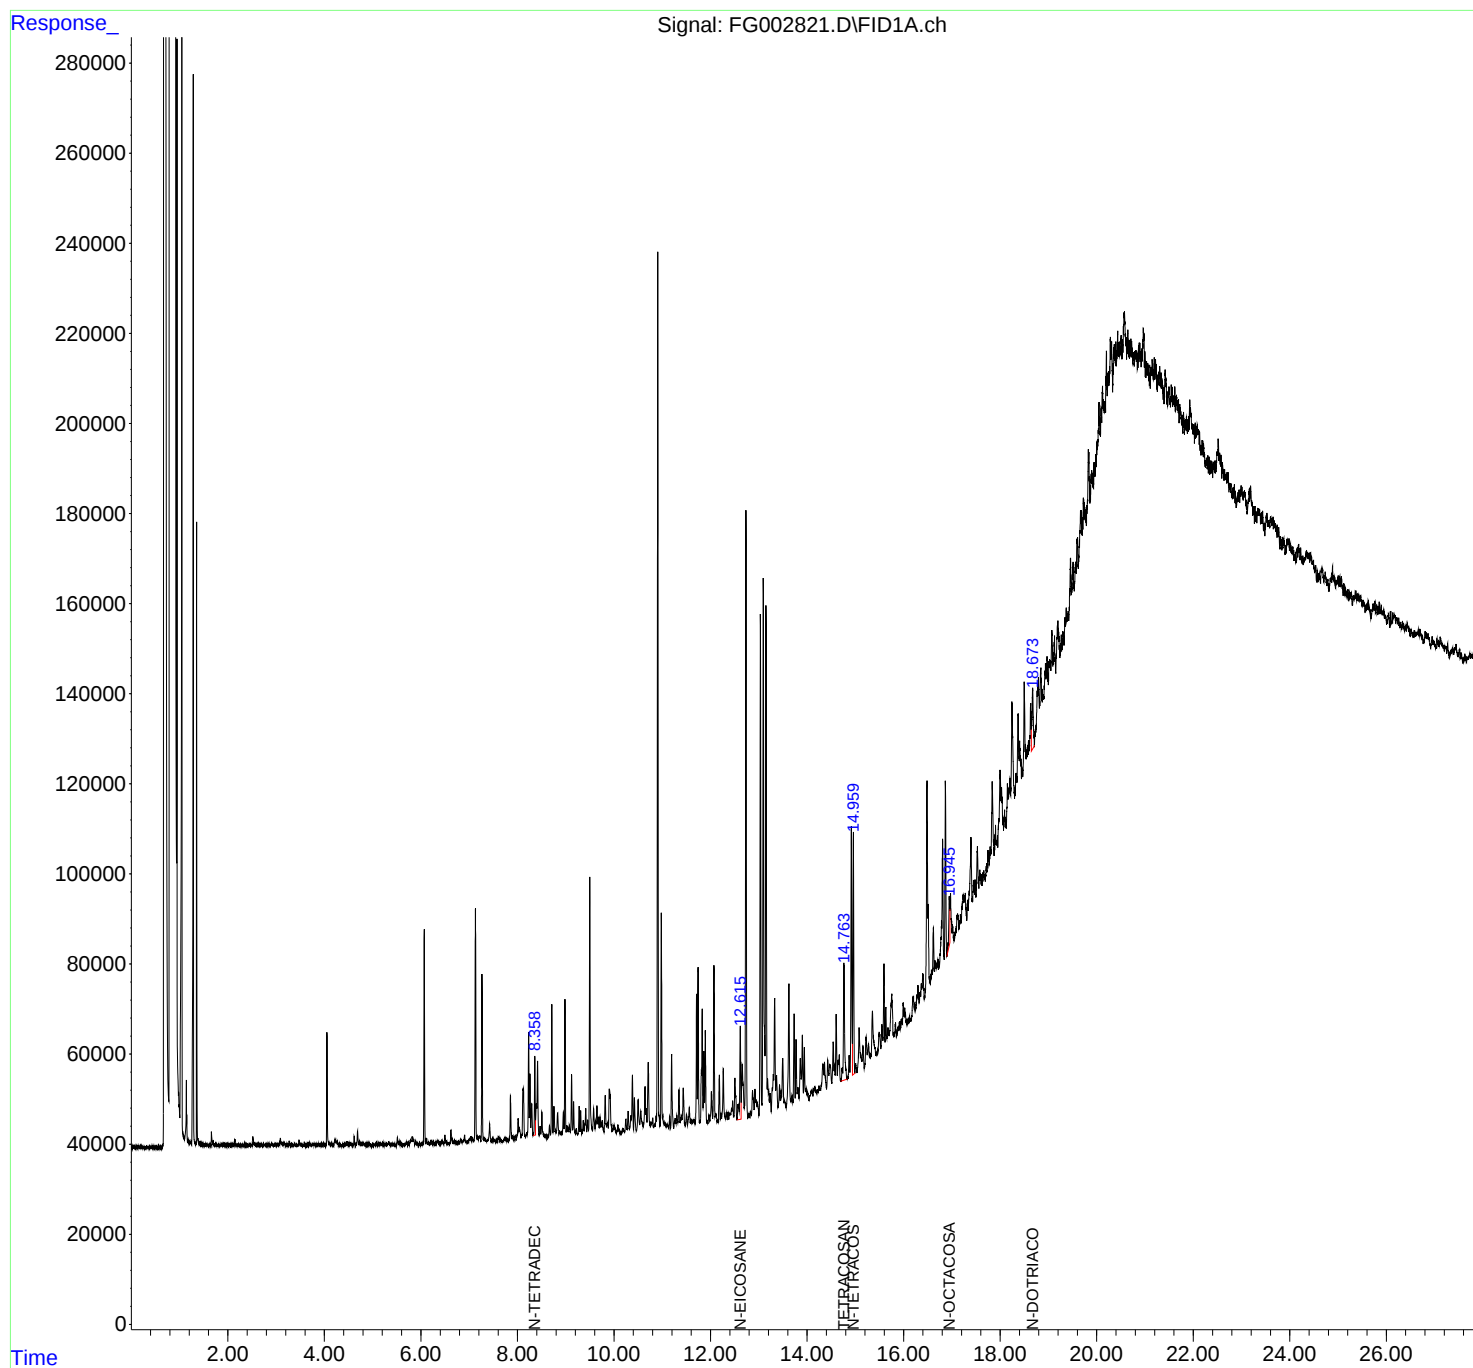


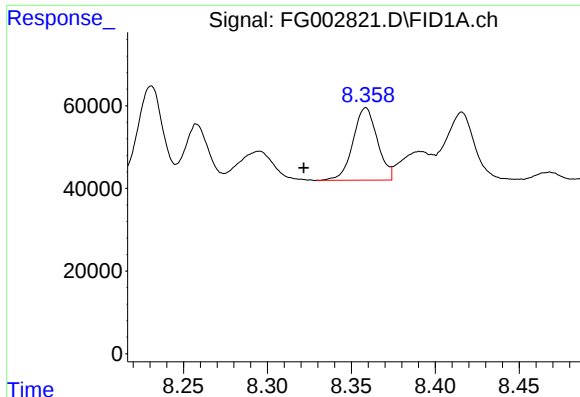

#6 N-TETRADECANE


R.T.: 8.359 min
Delta R.T.: 0.037 min
Response: 176602
Conc: 1.55 ug/ml

Instrument :
FID_G
ClientSampleId :

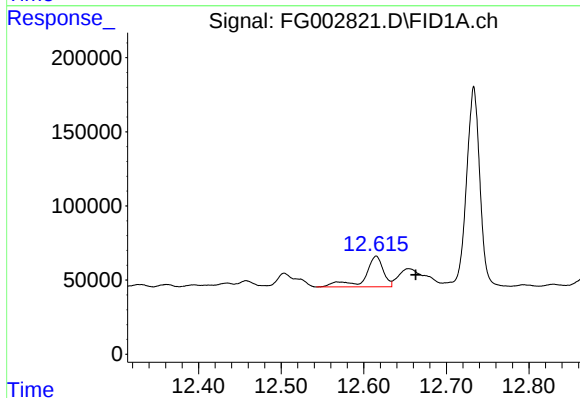


#9 N-EICOSANE

R.T.: 12.615 min
Delta R.T.: -0.048 min
Response: 319355
Conc: 2.83 ug/ml

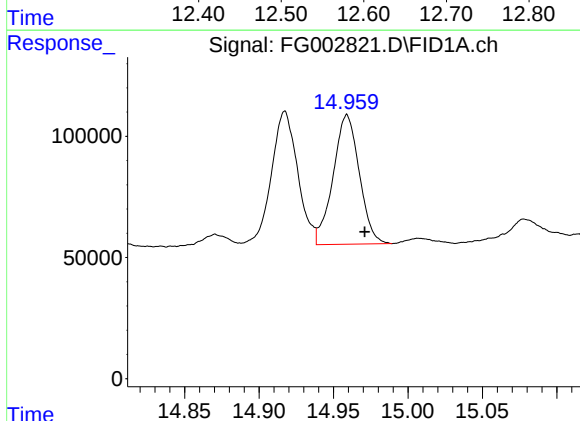


#10 N-TETRACOSANE

R.T.: 14.959 min
Delta R.T.: -0.012 min
Response: 654365
Conc: 6.23 ug/ml

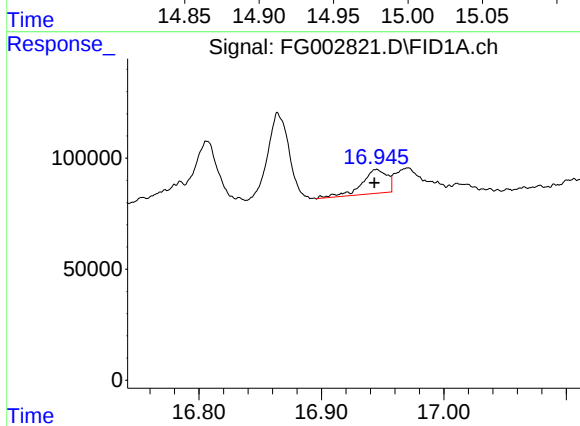

#11 N-OCTACOSANE


R.T.: 16.945 min
Delta R.T.: 0.002 min
Response: 156163
Conc: 1.58 ug/ml

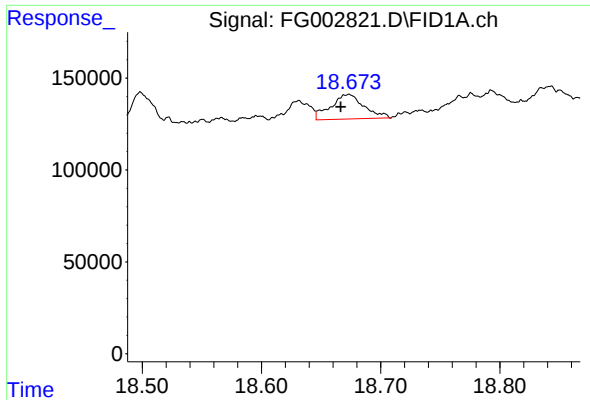

#12 N-DOTRIACONTANE

R.T.: 18.673 min
Delta R.T.: 0.006 min
Response: 258661
Conc: 3.01 ug/ml

Instrument :
FID_G
ClientSampleId :

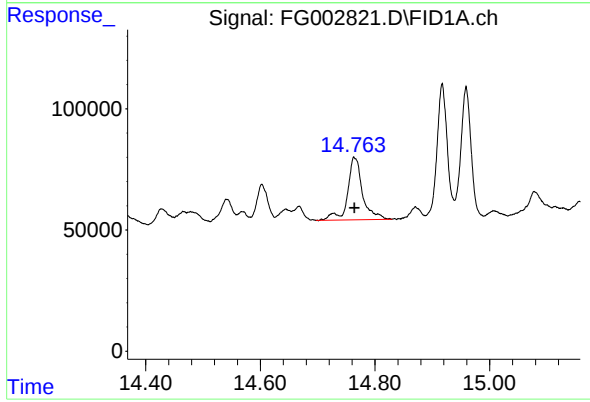

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.765 min
Delta R.T.: 0.000 min
Response: 468210
Conc: 3.81 ug/ml