

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110819\
Data File : FG006254.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2019 16:33
Operator : DD\AJ
Sample : K5742-05 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-22-(14-15)

Integration File: autoint1.e
Quant Time: Nov 08 22:44:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG103019.M
Quant Title :
QLast Update : Thu Oct 31 03:29:10 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
1) N-OCTANE	2.307	2630425	26.774 ug/ml
2) N-DECANE	4.366	1302410	12.946 ug/ml
3) N-DODECANE	6.353	591688	5.871 ug/ml
4) N-TETRADECANE	8.101	468864	4.696 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110819\
Data File : FG006254.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2019 16:33
Operator : DD\AJ
Sample : K5742-05 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SB-22-(14-15)

Integration File: autoint1.e
Quant Time: Nov 08 22:44:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG103019.M
Quant Title :
QLast Update : Thu Oct 31 03:29:10 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

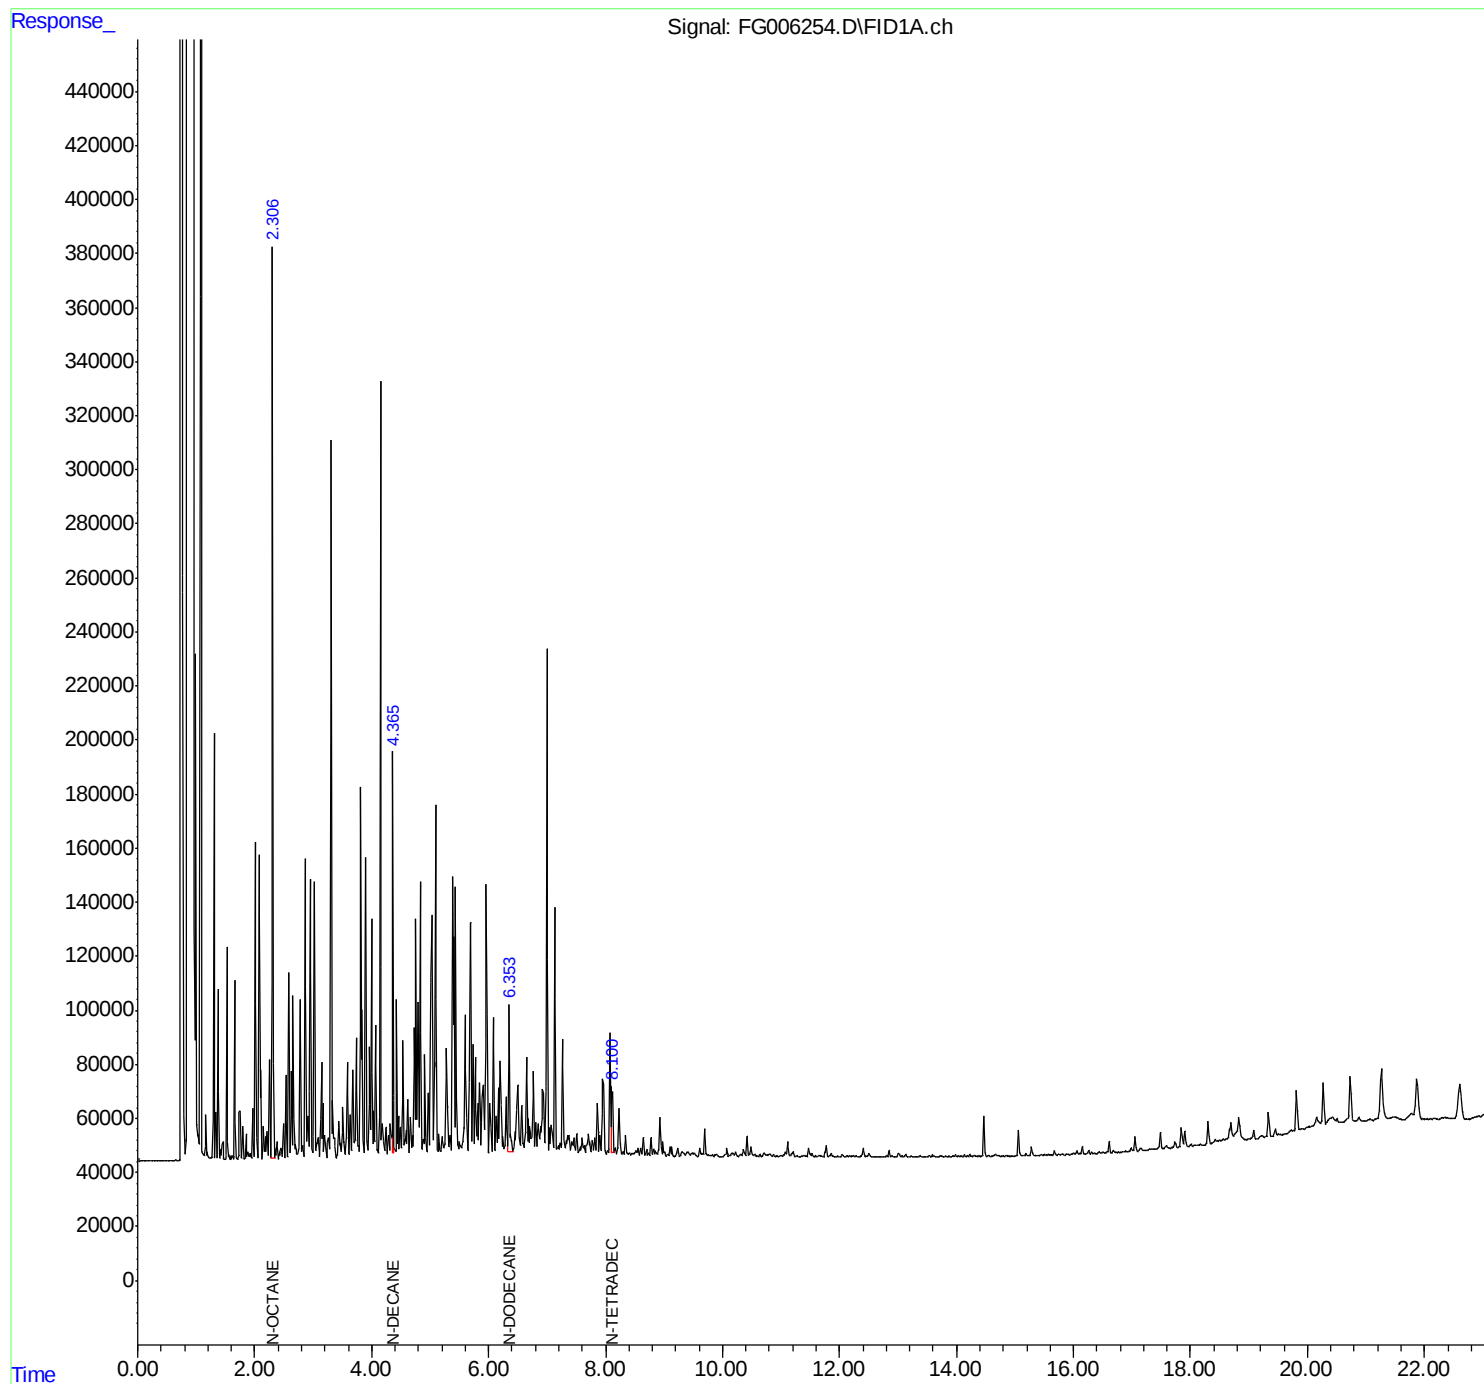


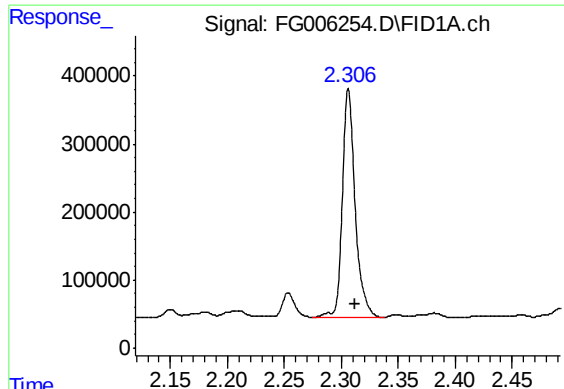

#1 N-OCTANE


R.T.: 2.307 min
Delta R.T.: -0.005 min
Response: 2630425
Conc: 26.77 ug/ml

Instrument :
FID_G
ClientSampleId :
SB-22-(14-15)

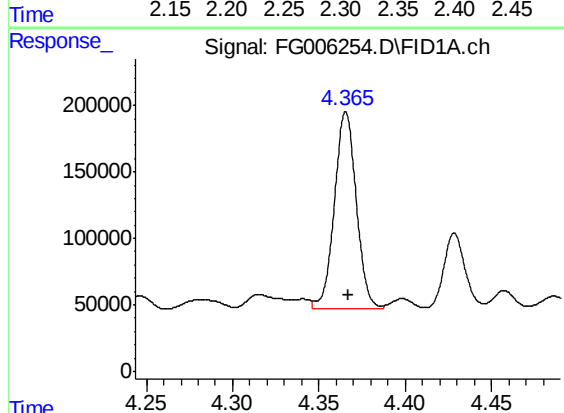


#2 N-DECANE

R.T.: 4.366 min
Delta R.T.: -0.002 min
Response: 1302410
Conc: 12.95 ug/ml

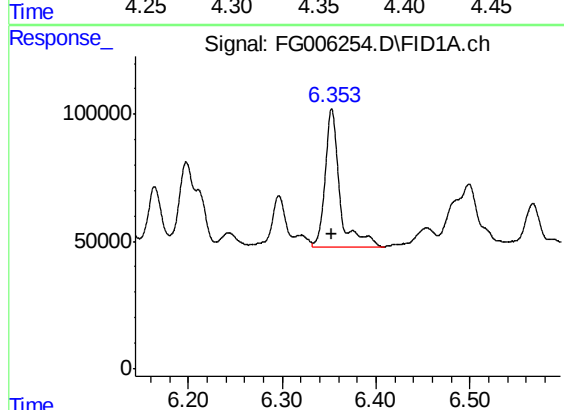


#3 N-DODECANE

R.T.: 6.353 min
Delta R.T.: 0.000 min
Response: 591688
Conc: 5.87 ug/ml

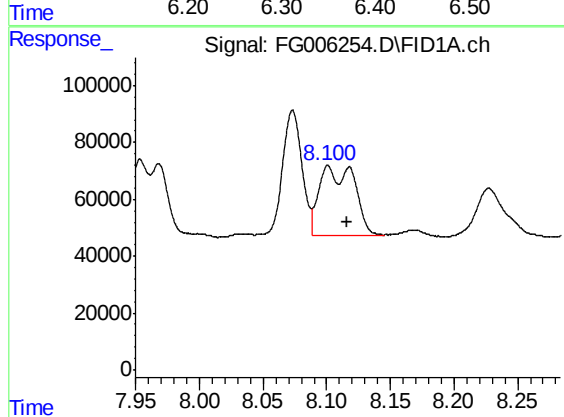

#4 N-TETRADECANE

R.T.: 8.101 min
Delta R.T.: -0.015 min
Response: 468864
Conc: 4.70 ug/ml

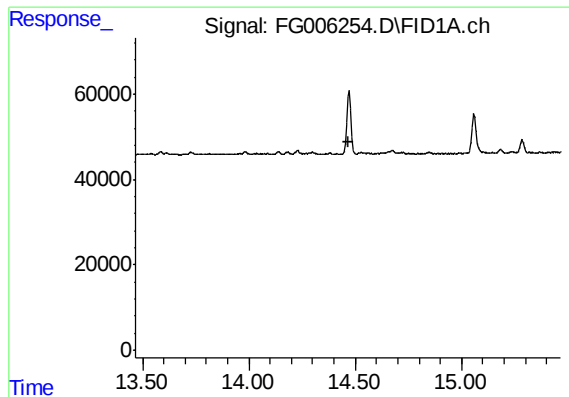

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.466 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :
SB-22-(14-15)