

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110821\
Data File : FG009003.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2021 12:38
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 00:16:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.730	1905210	16.507 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.199	74189	0.787 ug/ml
18) N-TETRACONTANE	21.889	94761	1.073 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110821\
Data File : FG009003.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2021 12:38
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 00:16:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

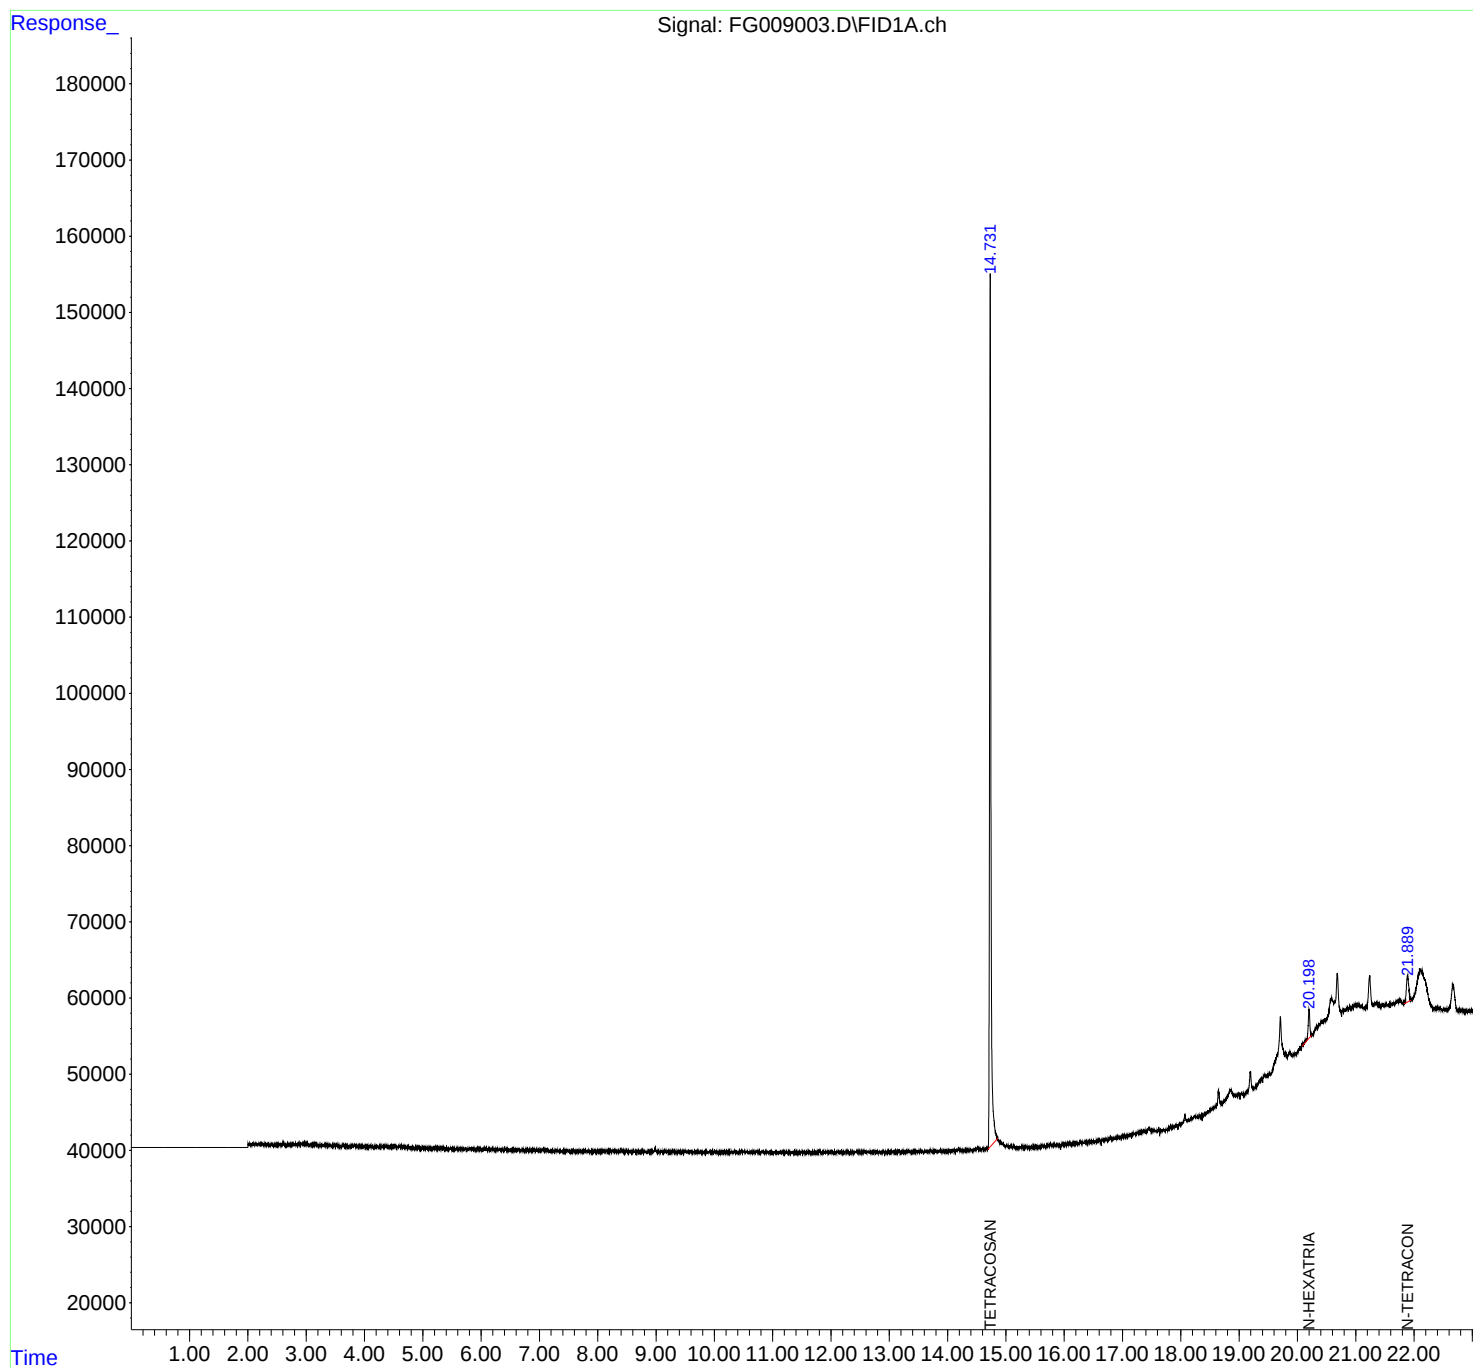

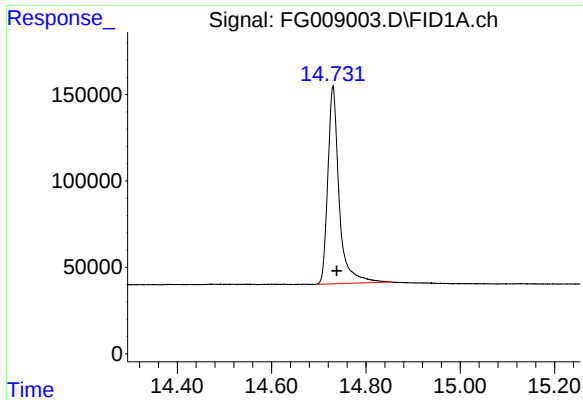


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.730 min
Delta R.T.: -0.008 min
Response: 1905210
Conc: 16.51 ug/ml

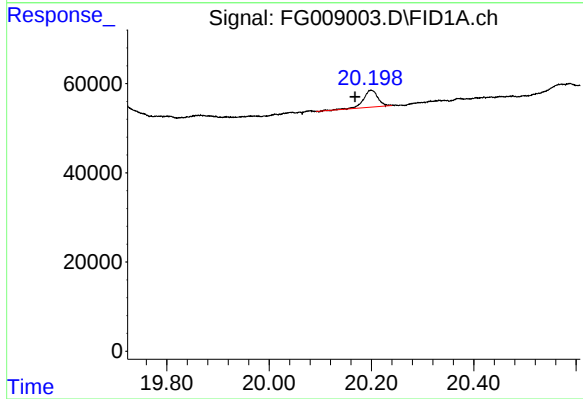

#16 N-HEXATRIACONTANE

R.T.: 20.199 min
Delta R.T.: 0.031 min
Response: 74189
Conc: 0.79 ug/ml

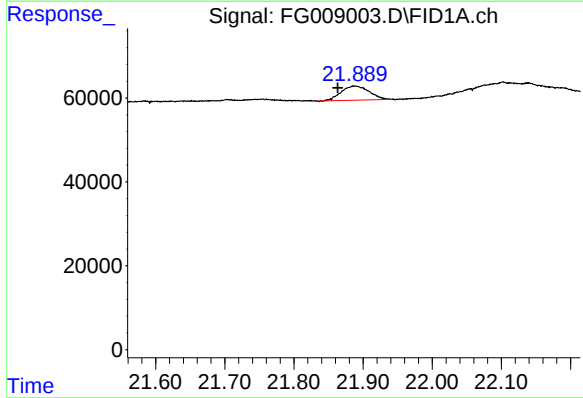

#18 N-TETRACONTANE

R.T.: 21.889 min
Delta R.T.: 0.025 min
Response: 94761
Conc: 1.07 ug/ml