

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110821\
Data File : FG009005.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2021 13:47
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 00:17:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.458	2505343	18.451 ug/ml
12) N-OCTACOSANE	16.910	2383161	19.385 ug/ml
13) N-TRIACONTANE	17.799	98415	0.841 ug/ml
14) N-DOTRIACONTANE	18.634	139499	1.281 ug/ml
15) N-TETRATRIACONTANE	19.419	106206	1.046 ug/ml
16) N-HEXATRIACONTANE	20.162	63336	0.671 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110821\
Data File : FG009005.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2021 13:47
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 00:17:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

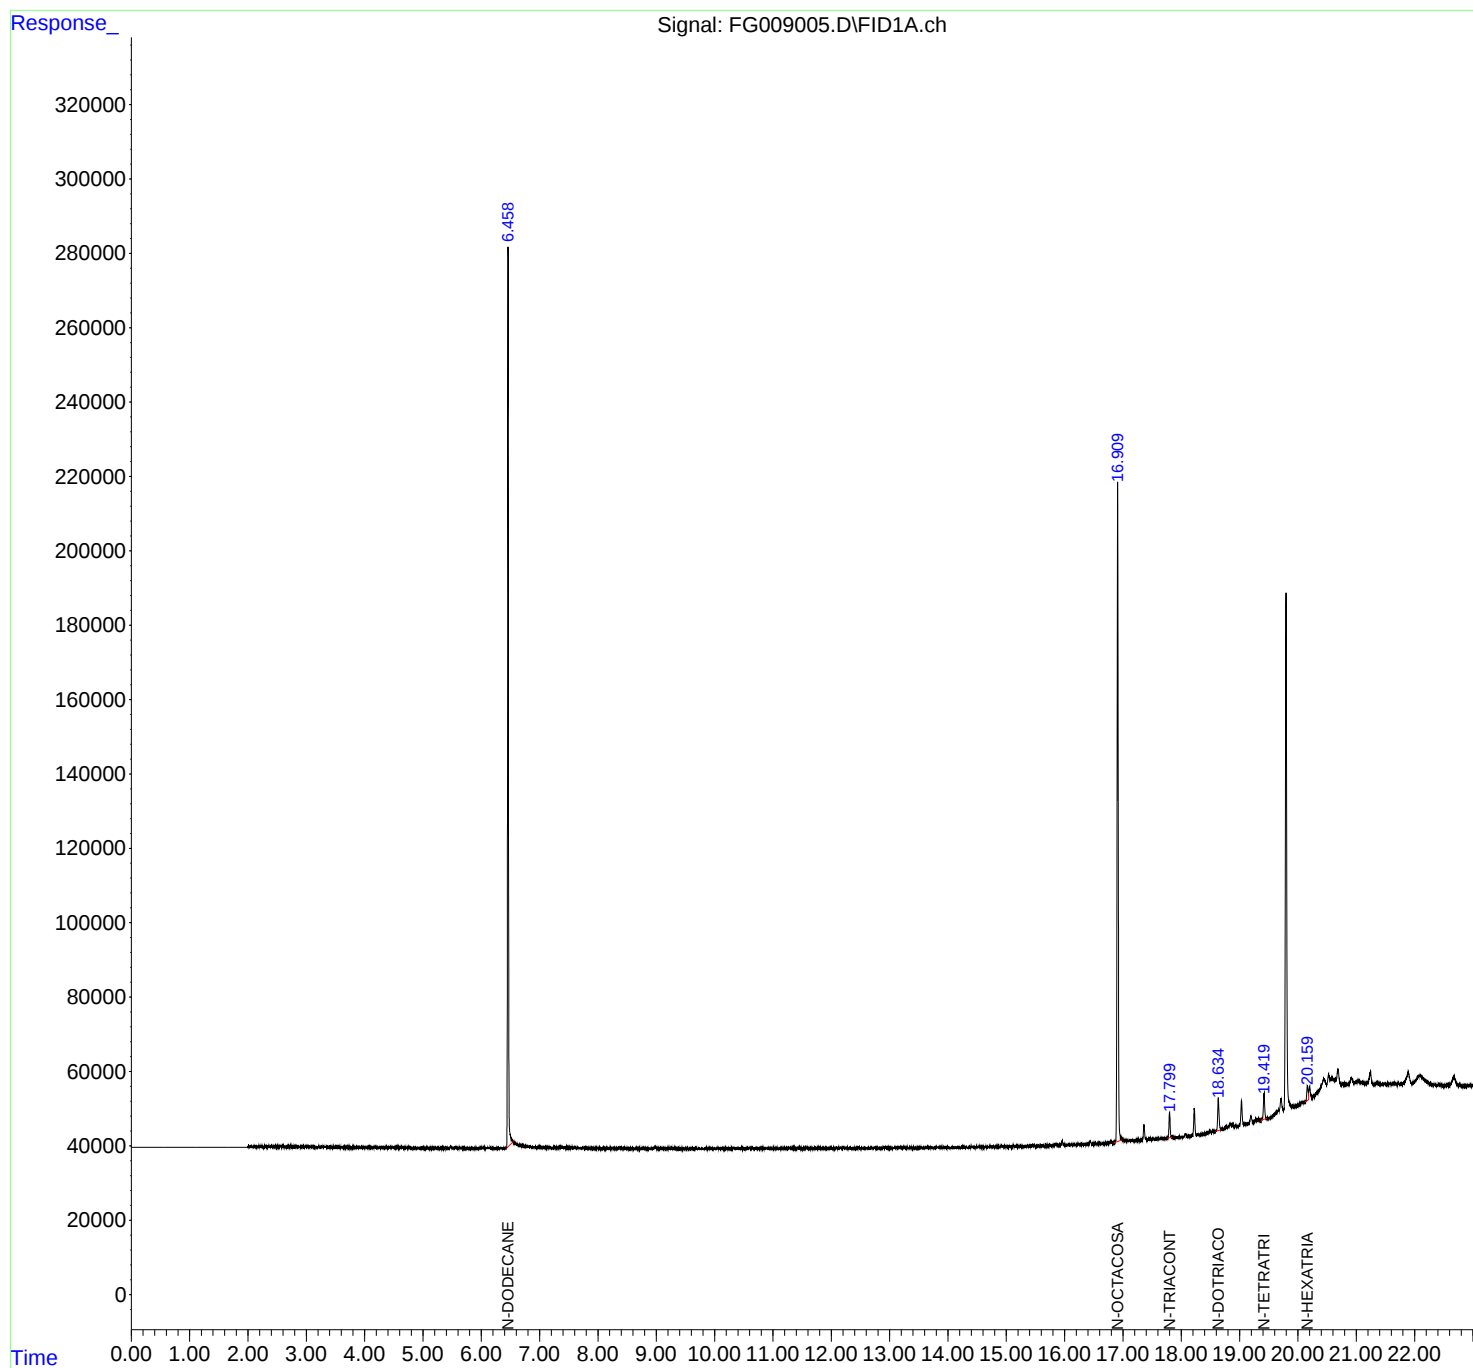

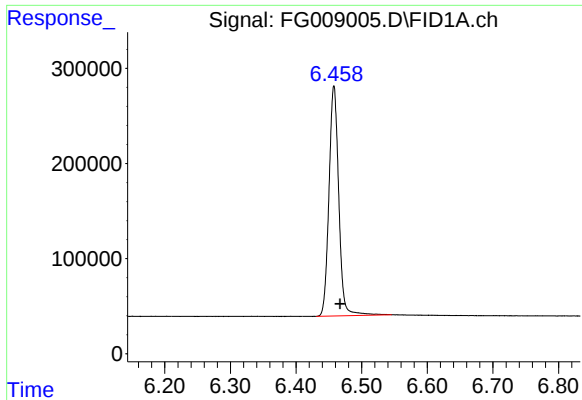


#3 N-DODECANE

R.T.: 6.458 min
Delta R.T.: -0.009 min
Response: 2505343
Conc: 18.45 ug/ml

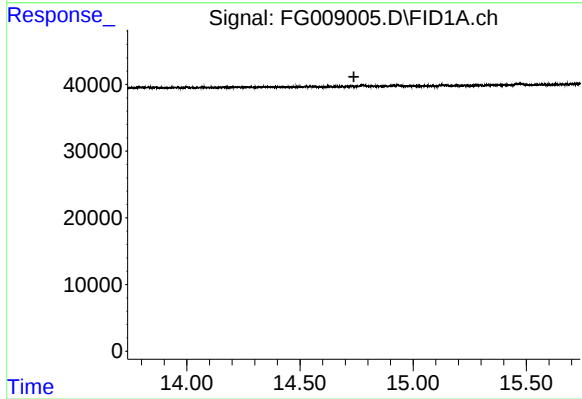


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.738 min
Response: 0
Conc: N.D.

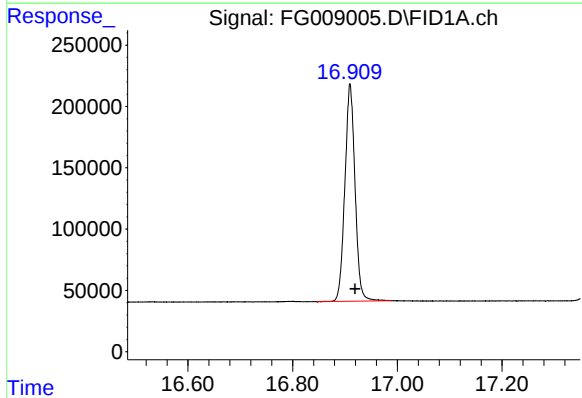


#12 N-OCTACOSANE

R.T.: 16.910 min
Delta R.T.: -0.010 min
Response: 2383161
Conc: 19.39 ug/ml

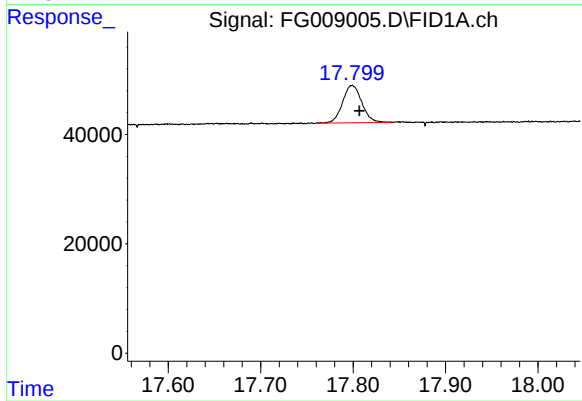


#13 N-TRIACONTANE

R.T.: 17.799 min
Delta R.T.: -0.008 min
Response: 98415
Conc: 0.84 ug/ml

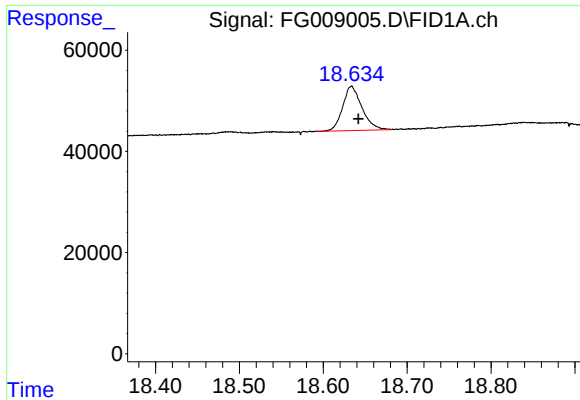


#14 N-DOTRIACONTANE

R.T.: 18.634 min
Delta R.T.: -0.008 min
Response: 139499
Conc: 1.28 ug/ml

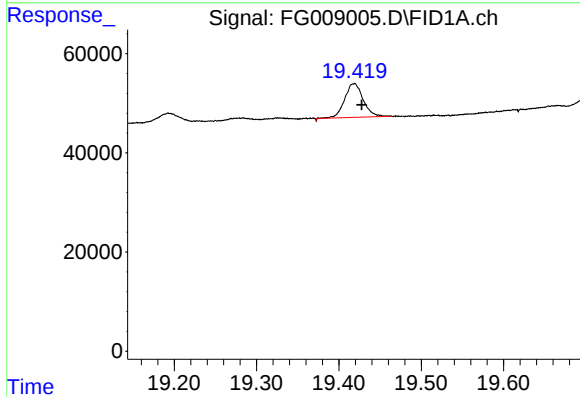

#15 N-TETRATRIACONTANE

R.T.: 19.419 min
Delta R.T.: -0.009 min
Response: 106206
Conc: 1.05 ug/ml

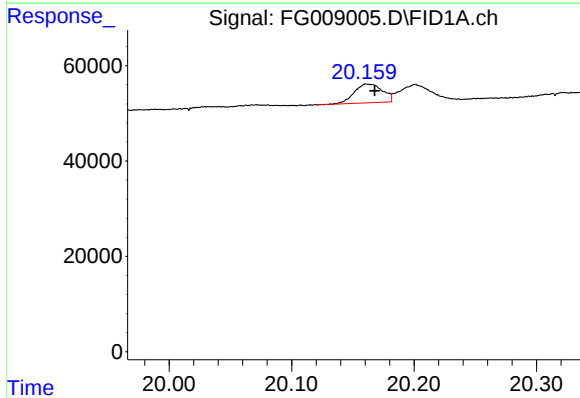

#16 N-HEXATRIACONTANE

R.T.: 20.162 min
Delta R.T.: -0.006 min
Response: 63336
Conc: 0.67 ug/ml