

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110823\
Data File : FG013162.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2023 11:10
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 23:10:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG101623.M
Quant Title :
QLast Update : Mon Oct 16 12:31:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.084	2117311	20.212 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.985	49495	0.473 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110823\
Data File : FG013162.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2023 11:10
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 08 23:10:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG101623.M
Quant Title :
QLast Update : Mon Oct 16 12:31:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

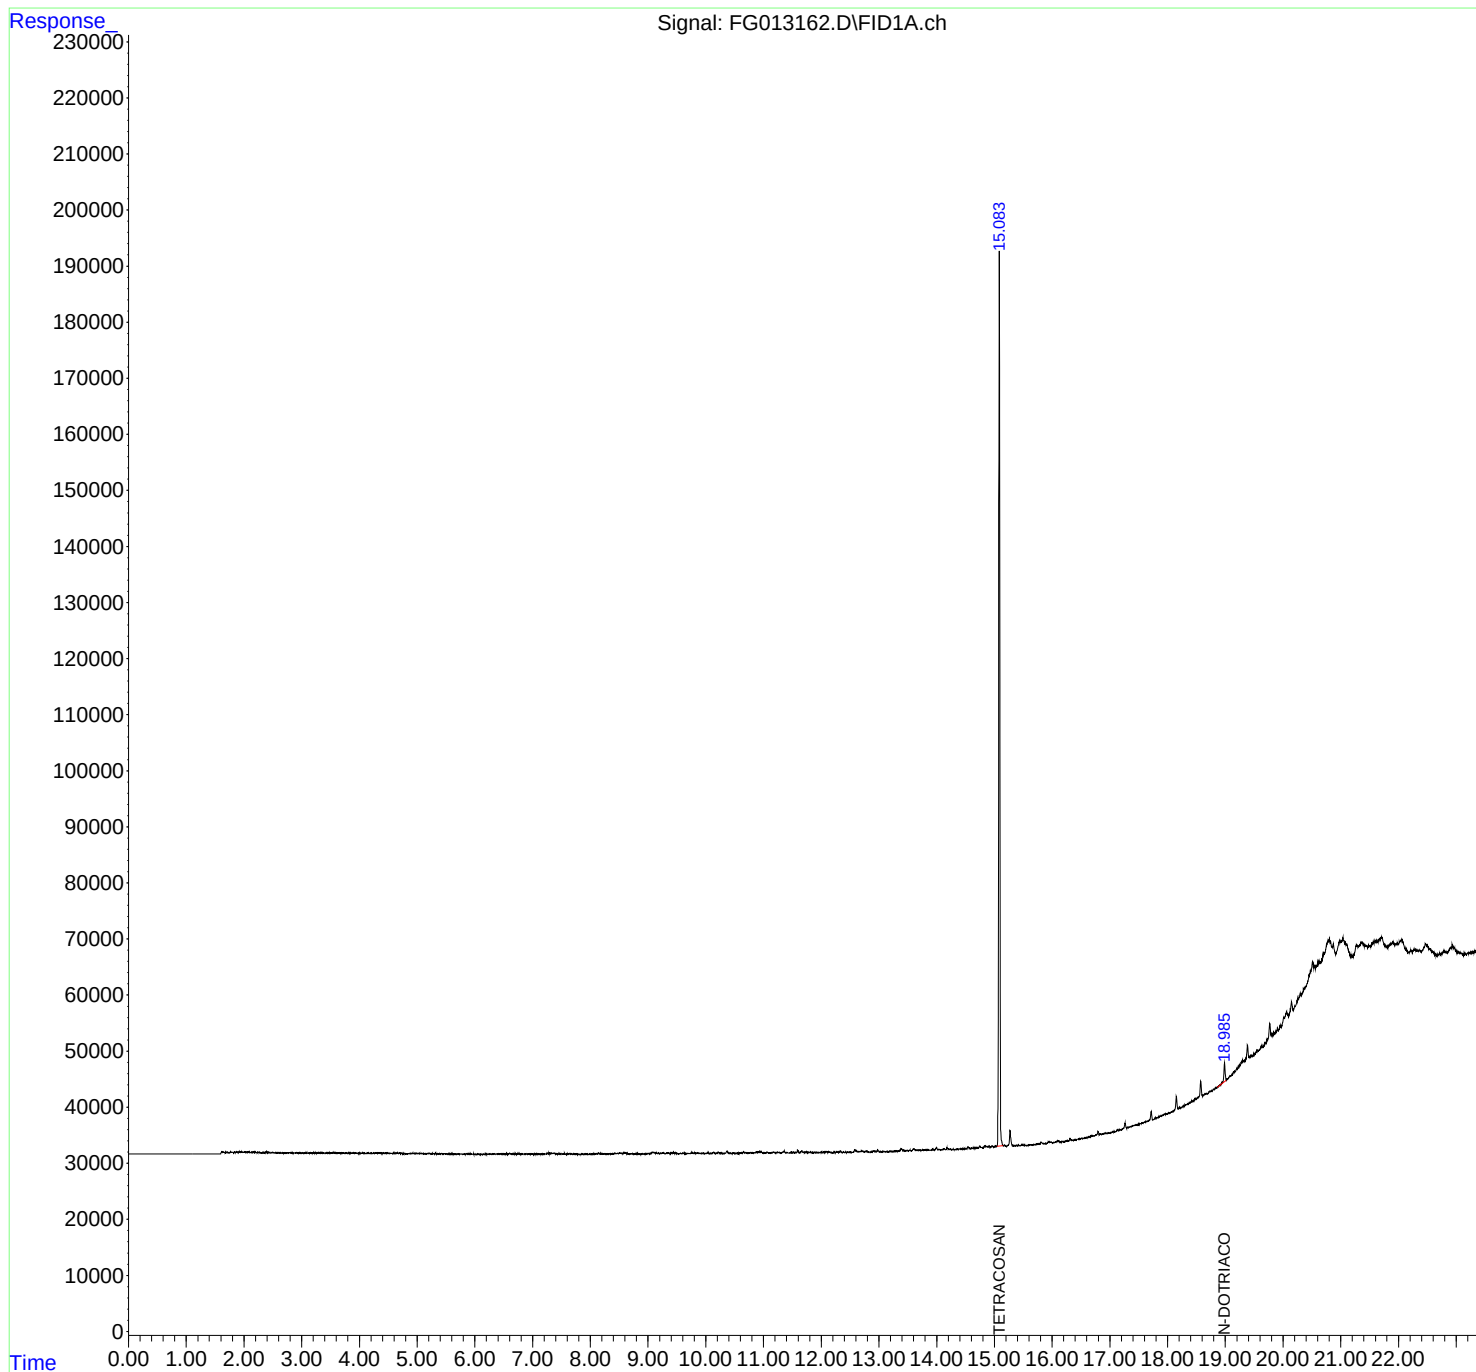


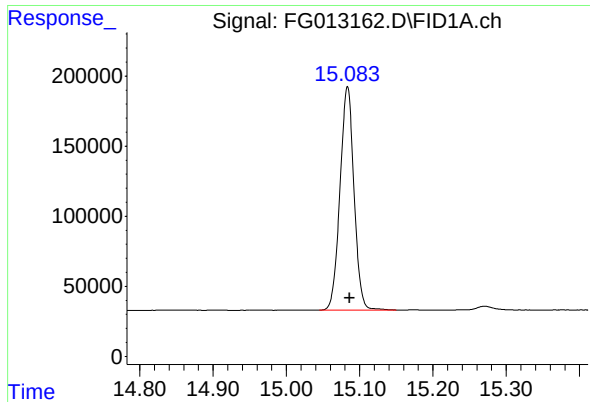

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.084 min
Delta R.T.: -0.003 min
Response: 2117311
Conc: 20.21 ug/ml

Instrument :
FID_G
ClientSampleId :

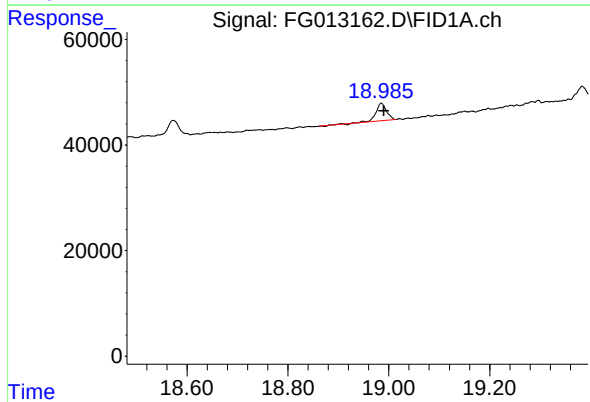

#14 N-DOTRIACONTANE

R.T.: 18.985 min
Delta R.T.: -0.005 min
Response: 49495
Conc: 0.47 ug/ml