

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110823\
Data File : FG013167.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2023 14:08
Operator : YP\AJ
Sample : 05292-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CORONA

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

Integration File: autoint1.e
Quant Time: Nov 08 23:11:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG101623.M
Quant Title :
QLast Update : Mon Oct 16 12:31:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.084	2083585	19.890 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110823\
Data File : FG013167.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2023 14:08
Operator : YP\AJ
Sample : 05292-01
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
CORONA


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023

Integration File: autoint1.e
Quant Time: Nov 08 23:11:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG101623.M
Quant Title :
QLast Update : Mon Oct 16 12:31:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

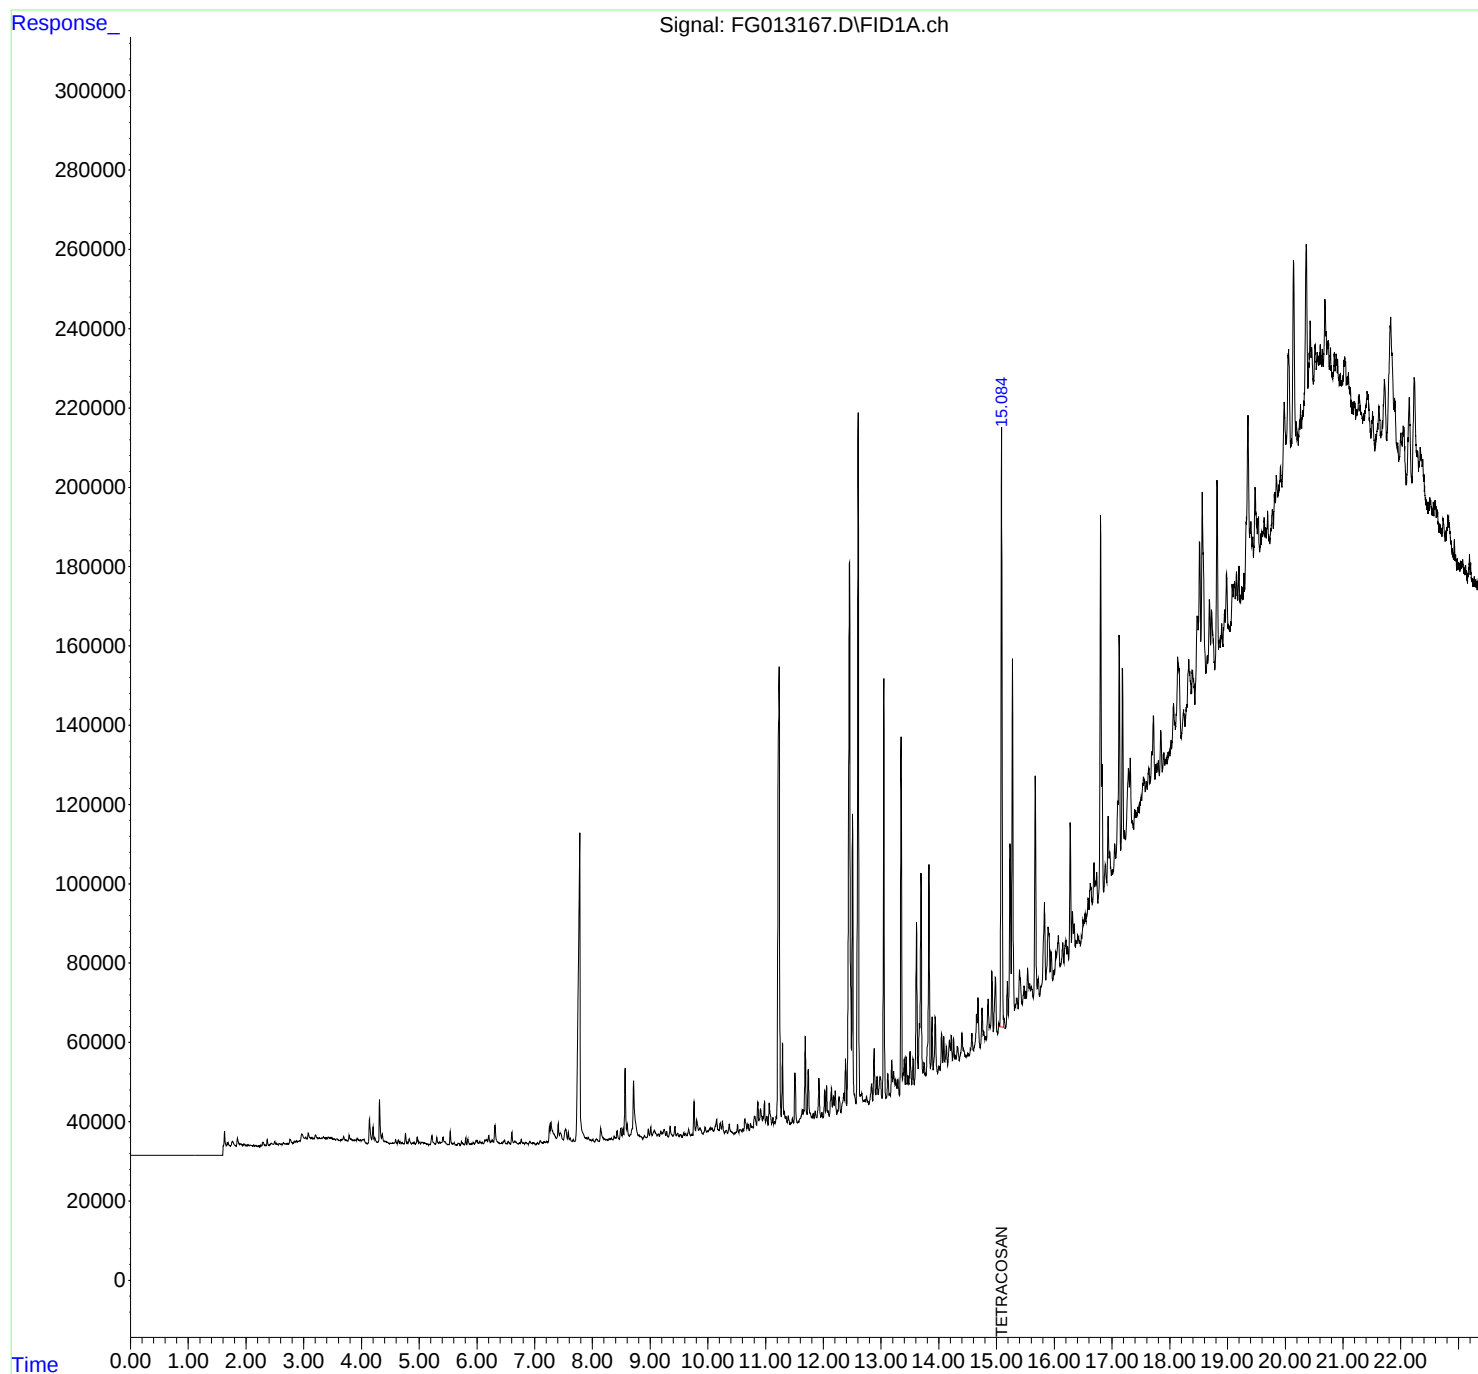

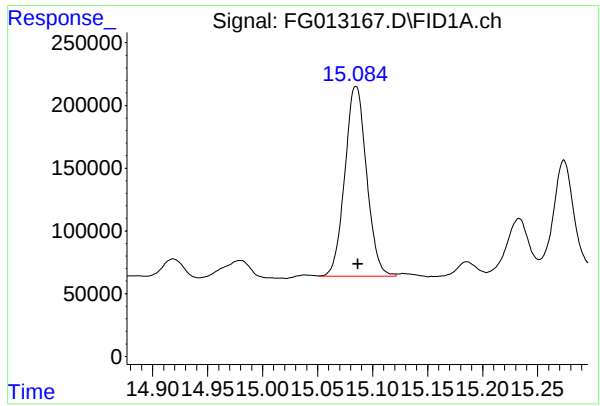

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.084 min
Delta R.T.: -0.002 min
Response: 2083585
Conc: 19.89 ug/ml

Instrument :
FID_G
ClientSampleId :
CORONA

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/09/2023
Supervised By :Ankita Jodhani 11/09/2023