

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110823\
 Data File : FG013171.D
 Signal(s) : FID1A.ch
 Acq On : 08 Nov 2023 16:05
 Operator : YP\AJ
 Sample : PB156990BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 PB156990BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/09/2023
 Supervised By :Ankita Jodhani 11/09/2023

Integration File: autoint1.e
 Quant Time: Nov 08 23:11:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG101623.M
 Quant Title :
 QLast Update : Mon Oct 16 12:31:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.085	1765738	16.856 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110823\
Data File : FG013171.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2023 16:05
Operator : YP\AJ
Sample : PB156990BL
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
PB156990BL


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/09/2023
Supervised By : Ankita Jodhani 11/09/2023

Integration File: autoint1.e
Quant Time: Nov 08 23:11:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG101623.M
Quant Title :
QLast Update : Mon Oct 16 12:31:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

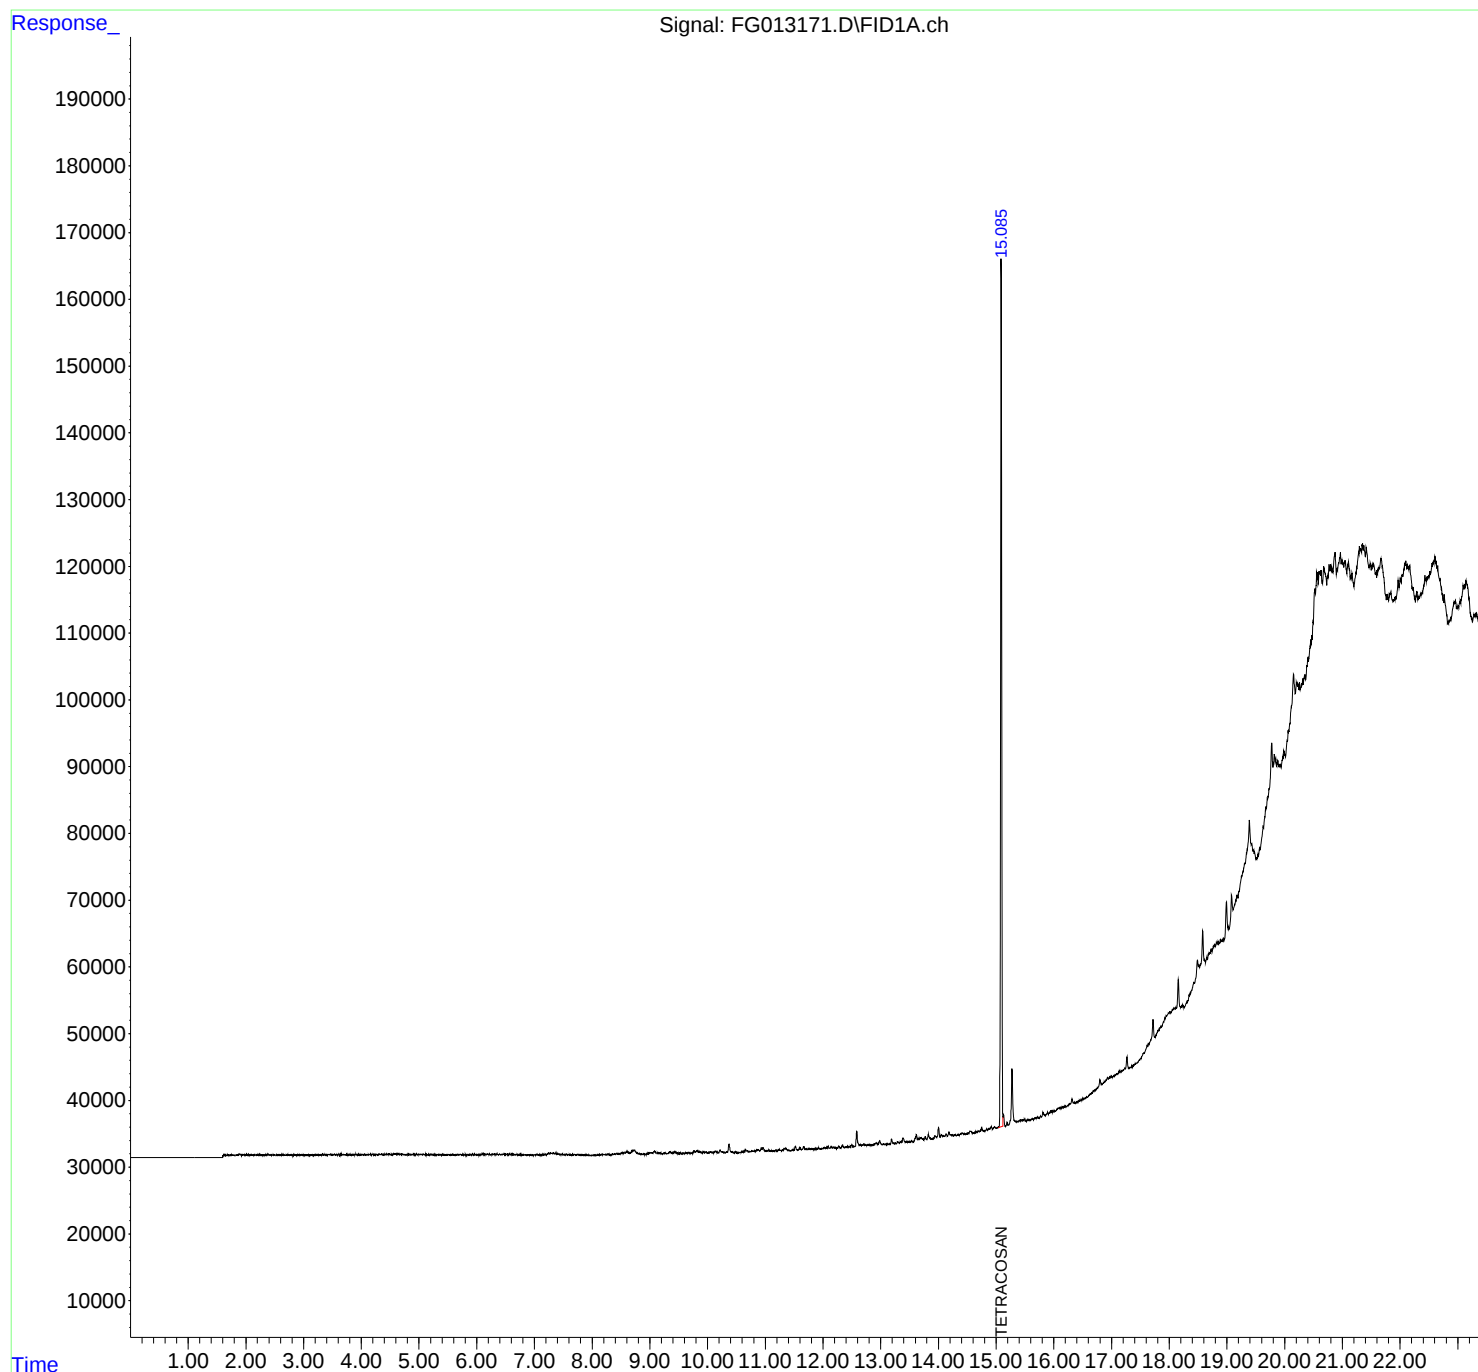

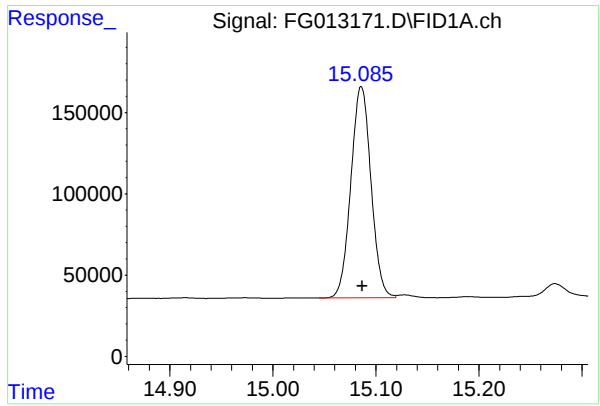

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.085 min
Delta R.T.: -0.002 min
Response: 1765738
Conc: 16.86 ug/ml

Instrument :

FID_G

ClientSampleId :

PB156990BL

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/09/2023

Supervised By :Ankita Jodhani 11/09/2023