

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110824AL\
 Data File : FG014715.D
 Signal(s) : FID1A.ch
 Acq On : 08 Nov 2024 17:30
 Operator : YP\AJ
 Sample : P4721-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 09 03:41:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 102124.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 22 06:49:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.390	3132365	25.510 ug/ml
Spiked Amount 50.000		Recovery =	51.02%
Target Compounds			
4) T n-Dodecane (C12)	6.742	79222	0.596 ug/ml
6) T n-Tetradecane (C14)	8.574	53083	0.400 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110824AL\
Data File : FG014715.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2024 17:30
Operator : YP\AJ
Sample : P4721-13
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 09 03:41:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 102124.M
Quant Title : GC Extractables
QLast Update : Tue Oct 22 06:49:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

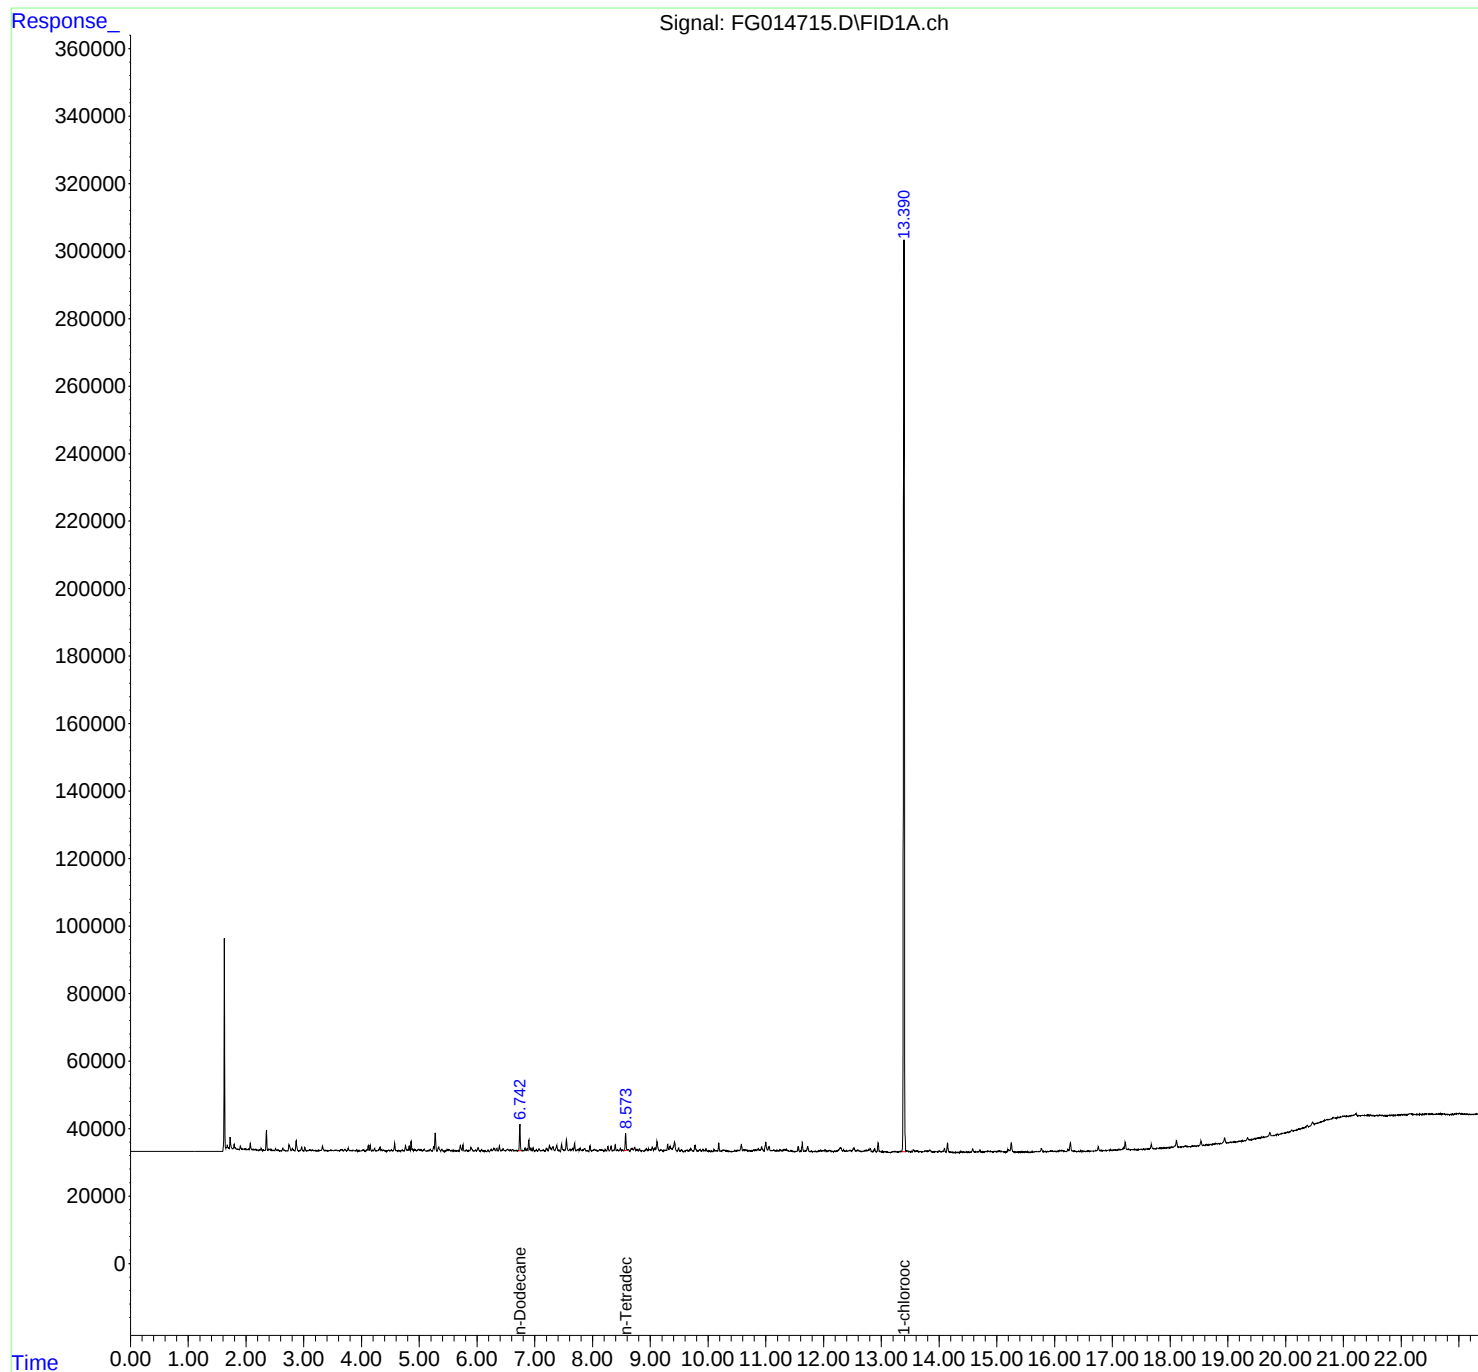


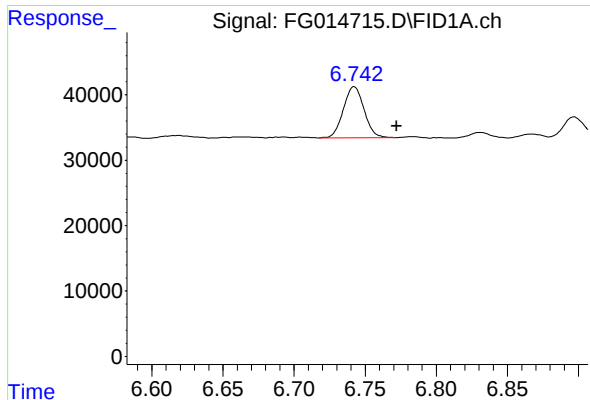

#4 n-Dodecane (C12)


R.T.: 6.742 min
Delta R.T.: -0.030 min
Response: 79222
Conc: 0.60 ug/ml

Instrument :
FID_G
ClientSampleId :

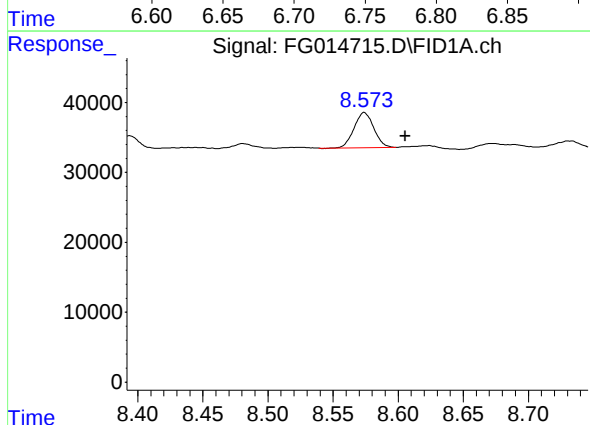


#6 n-Tetradecane (C14)

R.T.: 8.574 min
Delta R.T.: -0.031 min
Response: 53083
Conc: 0.40 ug/ml

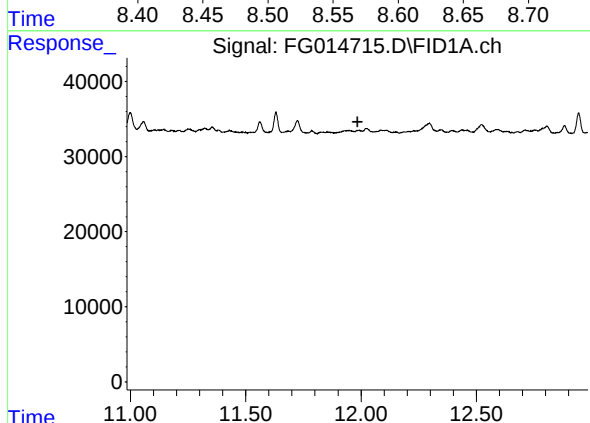

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.984 min
Response: 0
Conc: N.D.

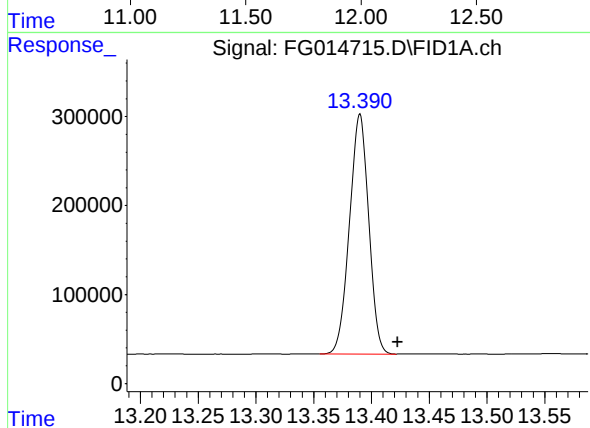

#12 1-chlorooctadecane (SURR)

R.T.: 13.390 min
Delta R.T.: -0.033 min
Response: 3132365
Conc: 25.51 ug/ml