

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110824AL\
 Data File : FG014717.D
 Signal(s) : FID1A.ch
 Acq On : 08 Nov 2024 18:27
 Operator : YP\AJ
 Sample : P4721-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 09 03:41:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 102124.M
 Quant Title : GC Extractables
 QLast Update : Tue Oct 22 06:49:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.391	3447930	28.080 ug/ml
Spiked Amount 50.000		Recovery =	56.16%
Target Compounds			
4) T n-Dodecane (C12)	6.742	68022	0.512 ug/ml
6) T n-Tetradecane (C14)	8.575	55653	0.419 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110824AL\
Data File : FG014717.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2024 18:27
Operator : YP\AJ
Sample : P4721-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 09 03:41:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 102124.M
Quant Title : GC Extractables
QLast Update : Tue Oct 22 06:49:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

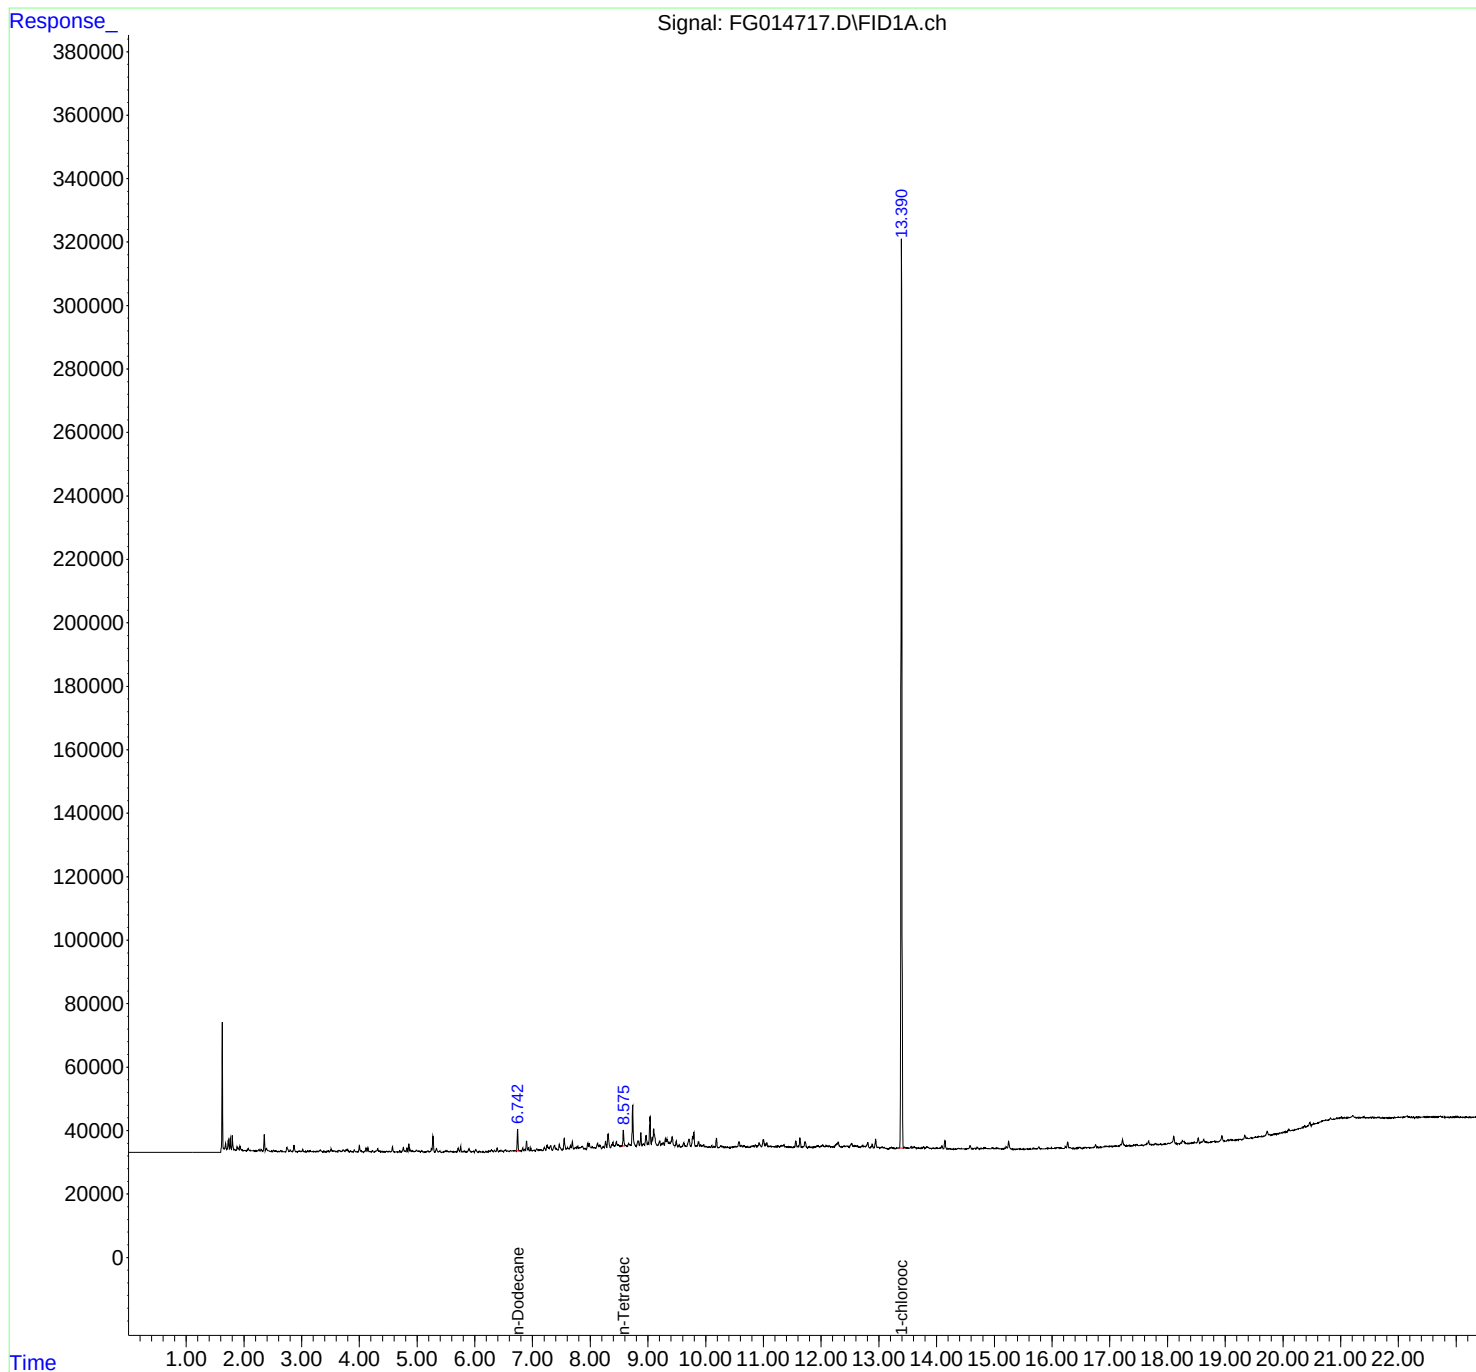


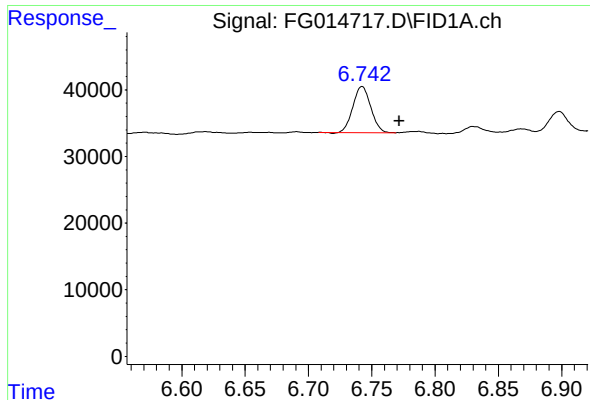

#4 n-Dodecane (C12)


R.T.: 6.742 min
Delta R.T.: -0.030 min
Response: 68022
Conc: 0.51 ug/ml

Instrument :
FID_G
ClientSampleId :

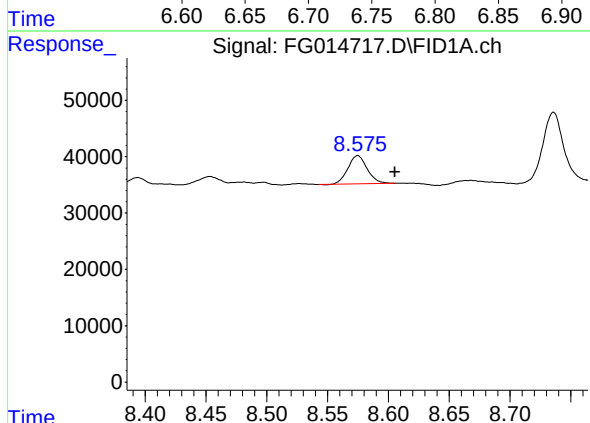


#6 n-Tetradecane (C14)

R.T.: 8.575 min
Delta R.T.: -0.030 min
Response: 55653
Conc: 0.42 ug/ml

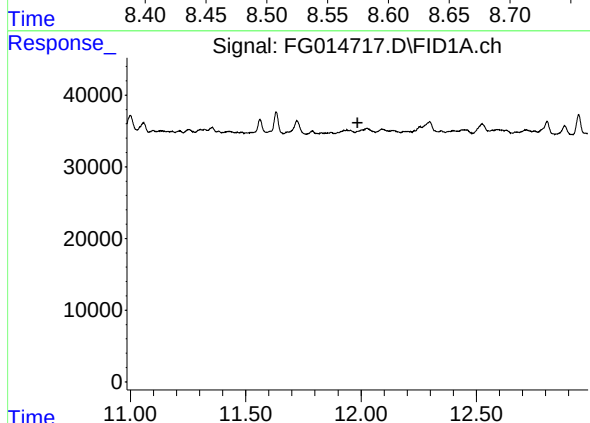

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.984 min
Response: 0
Conc: N.D.

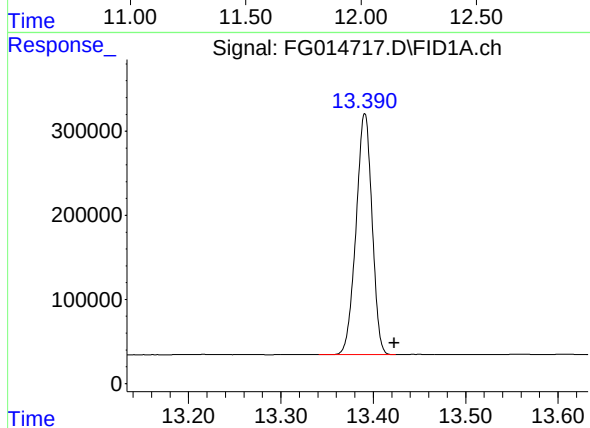

#12 1-chlorooctadecane (SURR)

R.T.: 13.391 min
Delta R.T.: -0.032 min
Response: 3447930
Conc: 28.08 ug/ml