

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110918\
 Data File : FG002831.D
 Signal(s) : FID1A.ch
 Acq On : 08 Nov 2018 19:21
 Operator : AJ\SJ
 Sample : J5768-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 09 08:37:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.762	190208	1.731 ug/ml
Target Compounds			
7) N-EICOSANE	12.612	105842	0.816 ug/ml
10) N-TETRACOSANE	14.955	245695	1.967 ug/ml
12) N-OCTACOSANE	16.941	151788	1.248 ug/ml
13) N-TRIACONTANE	17.831	130527	1.088 ug/ml
14) N-DOTRIACONTANE	18.669	173164	1.502 ug/ml
15) N-TETRATRIACONTANE	19.457	115539	1.039 ug/ml
16) N-HEXATRIACONTANE	20.192	814815	7.738 ug/ml
17) N-OCTATRIACONTANE	20.956	25265	0.265 ug/ml
18) N-TETRACONTANE	21.884	195106	1.975 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110918\
Data File : FG002831.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2018 19:21
Operator : AJ\SJ
Sample : J5768-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 08:37:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

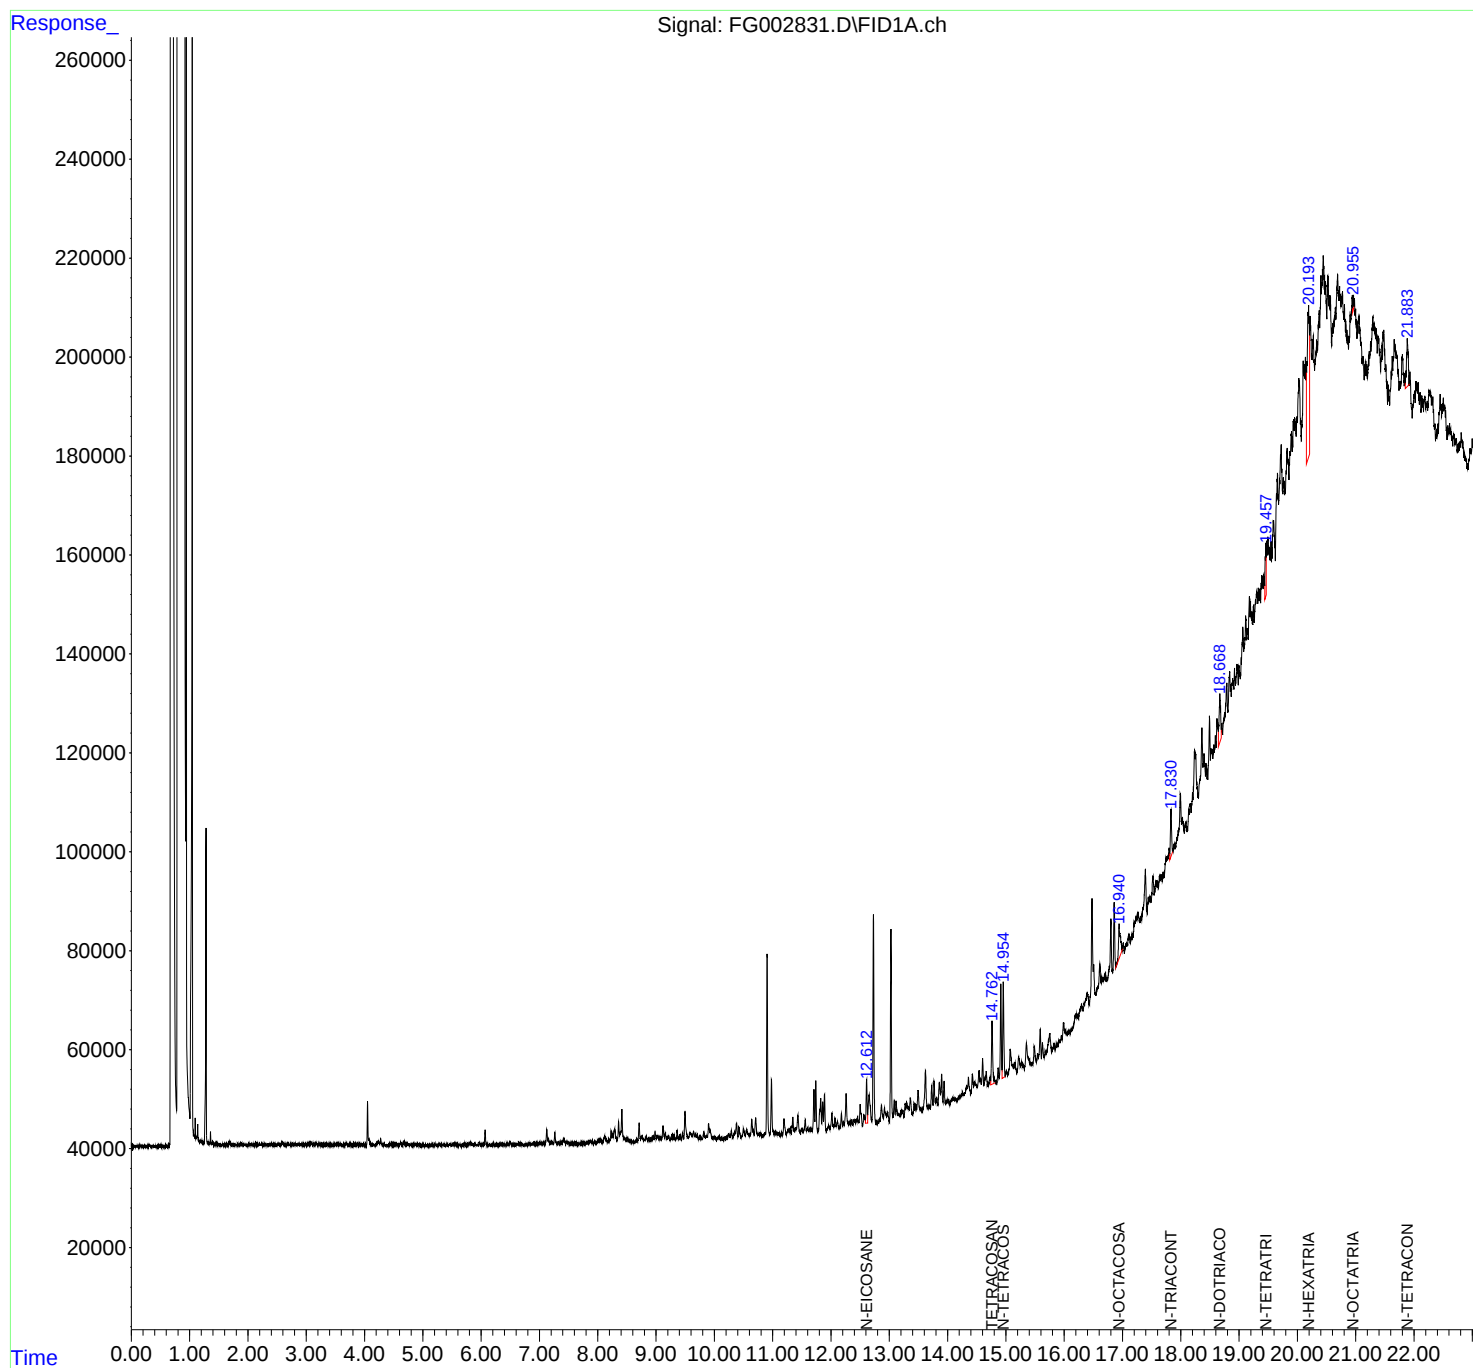

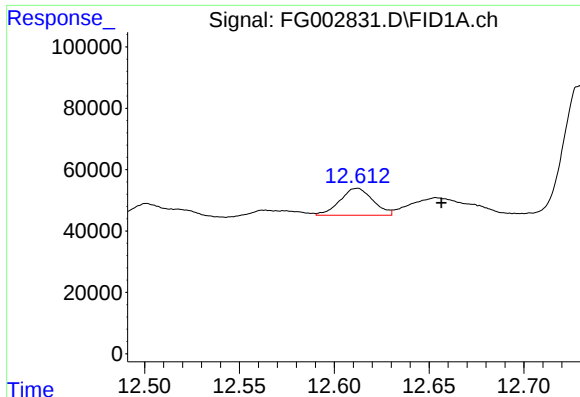


#7 N-EICOSANE

R.T.: 12.612 min
Delta R.T.: -0.044 min
Response: 105842
Conc: 0.82 ug/ml

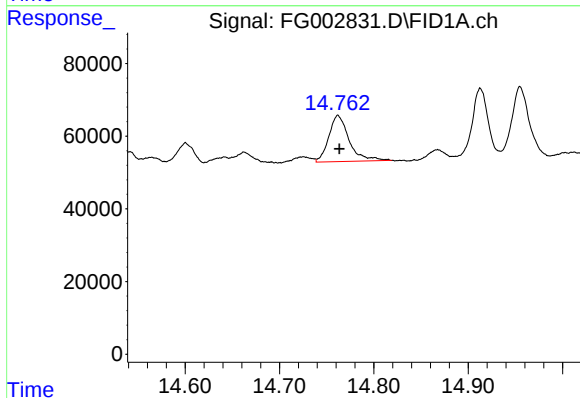


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.762 min
Delta R.T.: -0.002 min
Response: 190208
Conc: 1.73 ug/ml

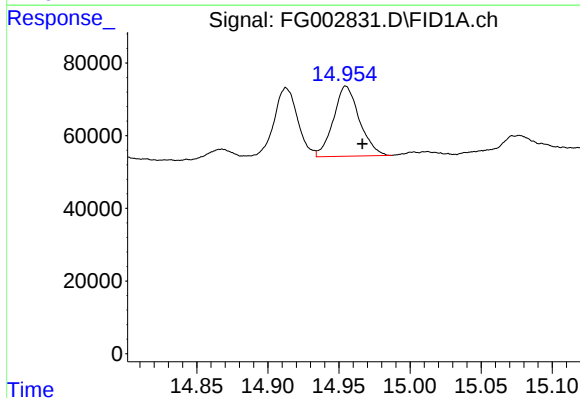


#10 N-TETRACOSANE

R.T.: 14.955 min
Delta R.T.: -0.012 min
Response: 245695
Conc: 1.97 ug/ml

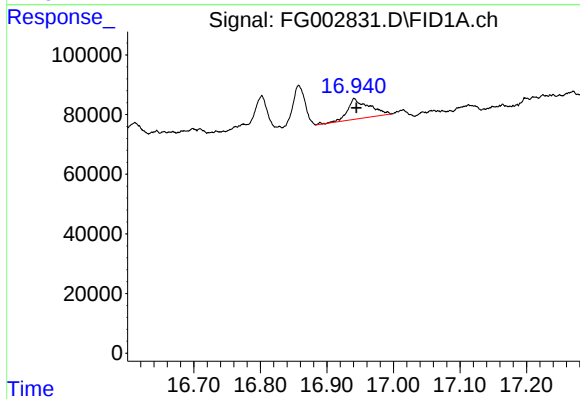


#12 N-OCTACOSANE

R.T.: 16.941 min
Delta R.T.: -0.003 min
Response: 151788
Conc: 1.25 ug/ml

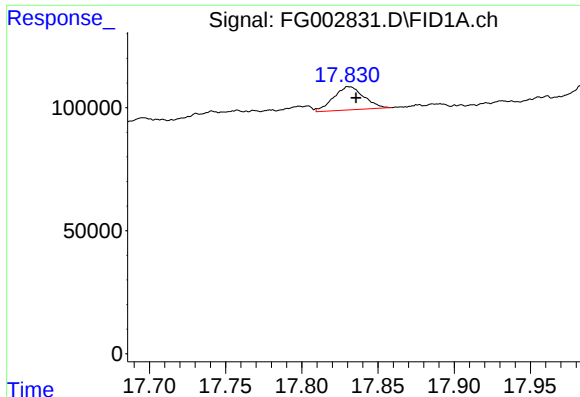


#13 N-TRIACONTANE

R.T.: 17.831 min
Delta R.T.: -0.004 min
Response: 130527
Conc: 1.09 ug/ml

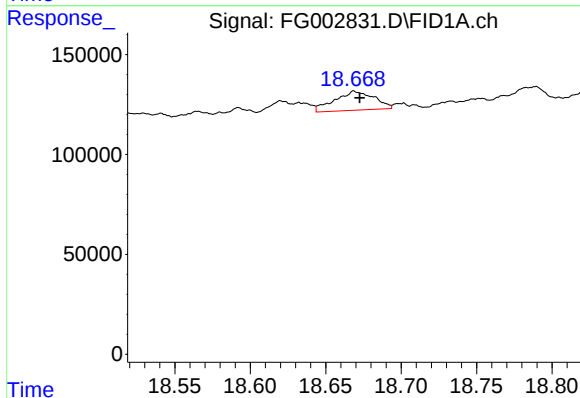


#14 N-DOTRIACONTANE

R.T.: 18.669 min
Delta R.T.: -0.004 min
Response: 173164
Conc: 1.50 ug/ml

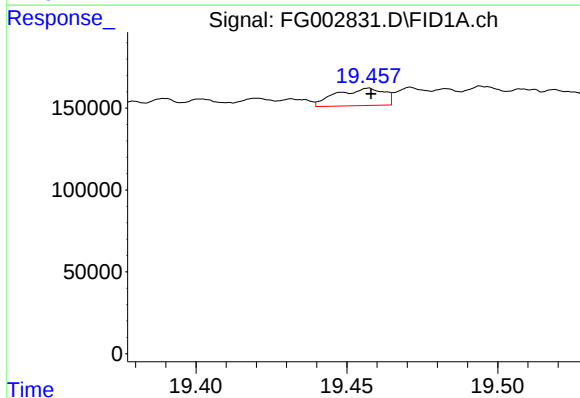


#15 N-TETRATRIACONTANE

R.T.: 19.457 min
Delta R.T.: 0.000 min
Response: 115539
Conc: 1.04 ug/ml

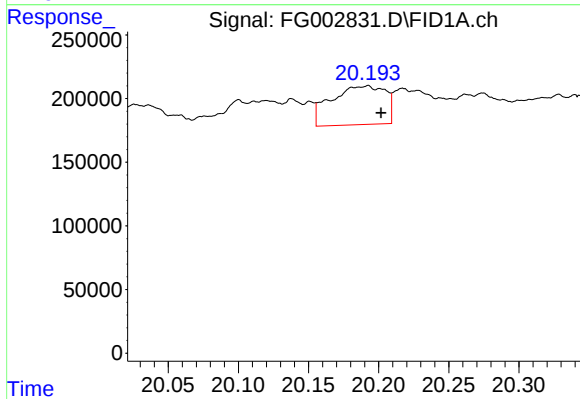


#16 N-HEXATRIACONTANE

R.T.: 20.192 min
Delta R.T.: -0.010 min
Response: 814815
Conc: 7.74 ug/ml

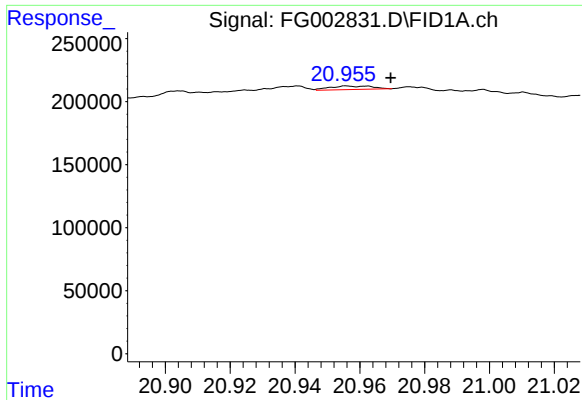

#17 N-OCTATRIACONTANE

R.T.: 20.956 min
Delta R.T.: -0.013 min
Response: 25265
Conc: 0.27 ug/ml

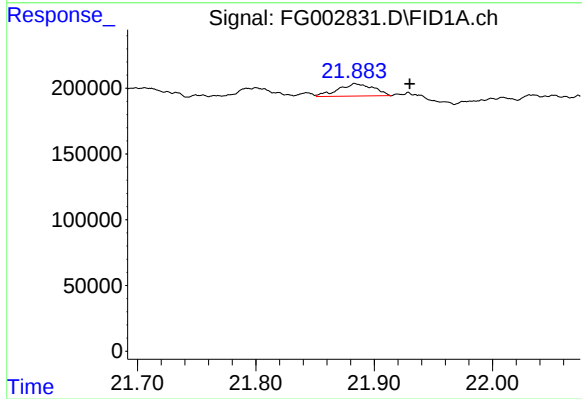

#18 N-TETRACONTANE

R.T.: 21.884 min
Delta R.T.: -0.046 min
Response: 195106
Conc: 1.98 ug/ml