

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110918\
 Data File : FG002834.D
 Signal(s) : FID1A.ch
 Acq On : 08 Nov 2018 20:51
 Operator : AJ\SJ
 Sample : J5858-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 09 08:37:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.762	2124337	19.330 ug/ml
Target Compounds			
4) N-TETRADECANE	8.358f	854764	6.464 ug/ml
5) N-HEXADECANE	9.931	236619	1.777 ug/ml
8) N-DOCOSANE	13.859	129809	1.020 ug/ml
10) N-TETRACOSANE	14.966	202811	1.623 ug/ml
11) N-HEXACOSANE	15.989	290916	2.360 ug/ml
12) N-OCTACOSANE	16.941	435065	3.577 ug/ml
13) N-TRIACONTANE	17.829	391657	3.264 ug/ml
14) N-DOTRIACONTANE	18.664	172689	1.498 ug/ml
15) N-TETRATRIACONTANE	19.451	66731	0.600 ug/ml
16) N-HEXATRIACONTANE	20.195	218037	2.071 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110918\
Data File : FG002834.D
Signal(s) : FID1A.ch
Acq On : 08 Nov 2018 20:51
Operator : AJ\SJ
Sample : J5858-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 08:37:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

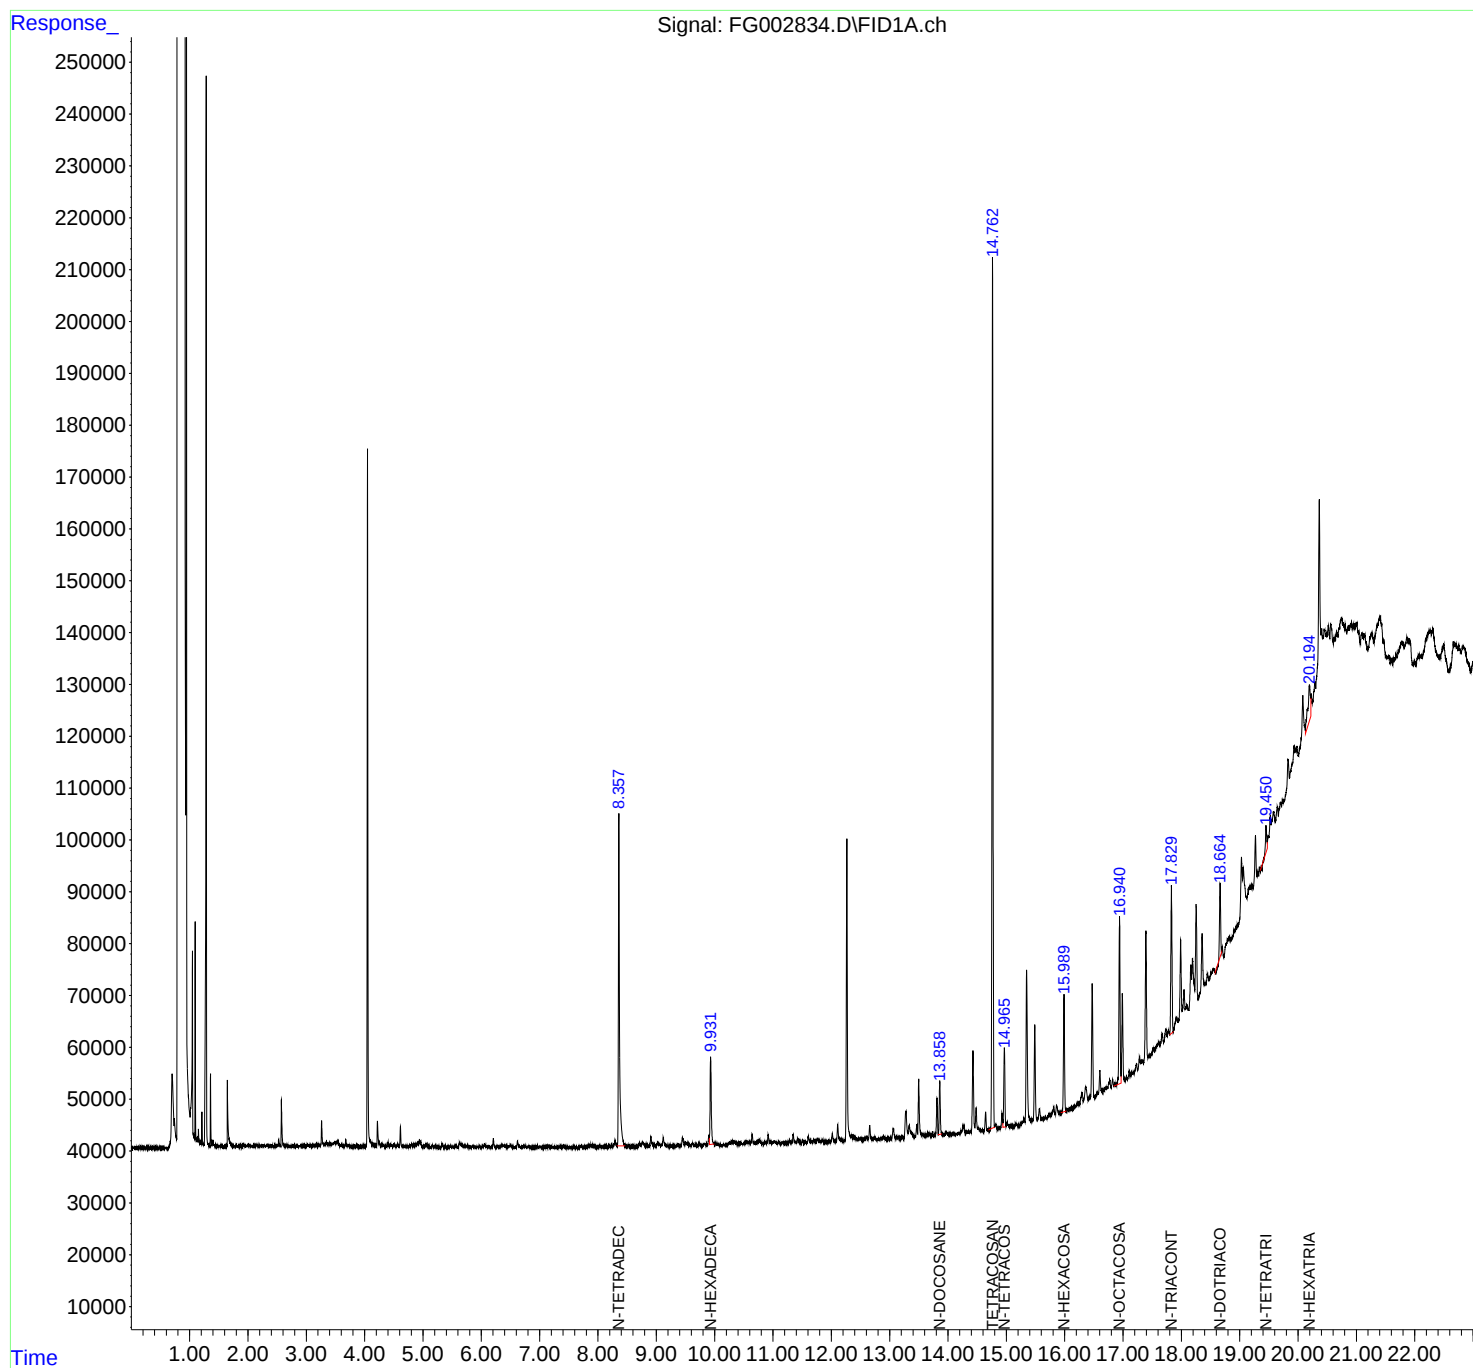

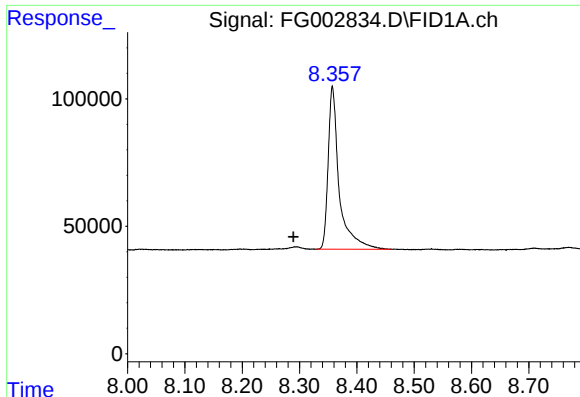


#4 N-TETRADECANE

R.T.: 8.358 min
Delta R.T.: 0.068 min
Response: 854764
Conc: 6.46 ug/ml

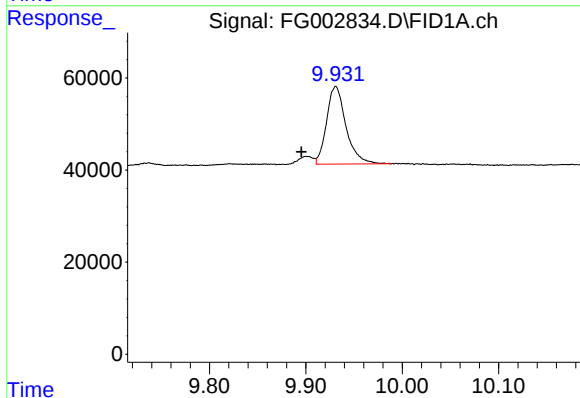


#5 N-HEXADECANE

R.T.: 9.931 min
Delta R.T.: 0.036 min
Response: 236619
Conc: 1.78 ug/ml

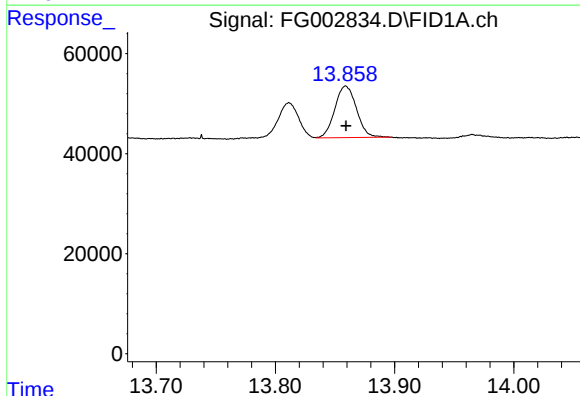


#8 N-DOCOSANE

R.T.: 13.859 min
Delta R.T.: 0.000 min
Response: 129809
Conc: 1.02 ug/ml

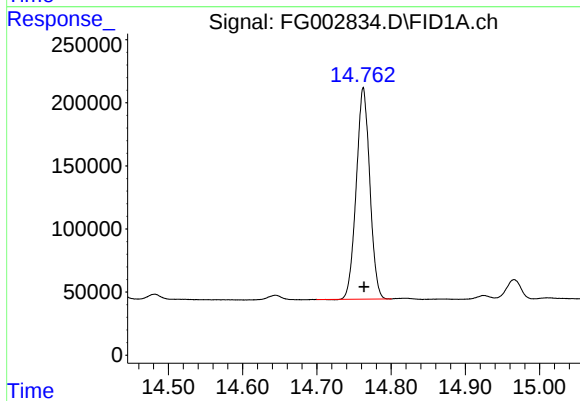


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.762 min
Delta R.T.: -0.001 min
Response: 2124337
Conc: 19.33 ug/ml

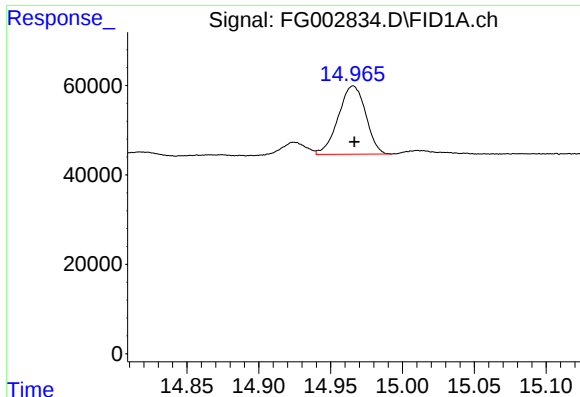


#10 N-TETRACOSANE

R.T.: 14.966 min
Delta R.T.: 0.000 min
Response: 202811
Conc: 1.62 ug/ml

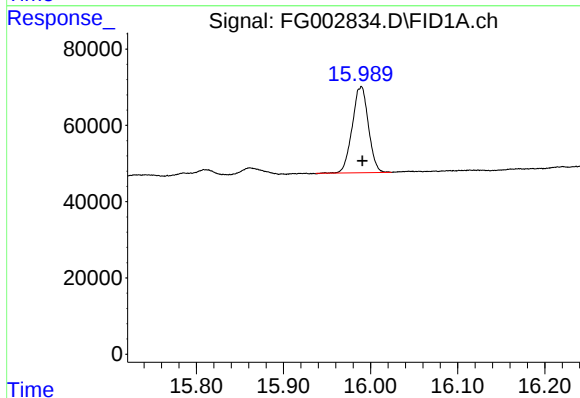


#11 N-HEXACOSANE

R.T.: 15.989 min
Delta R.T.: -0.001 min
Response: 290916
Conc: 2.36 ug/ml

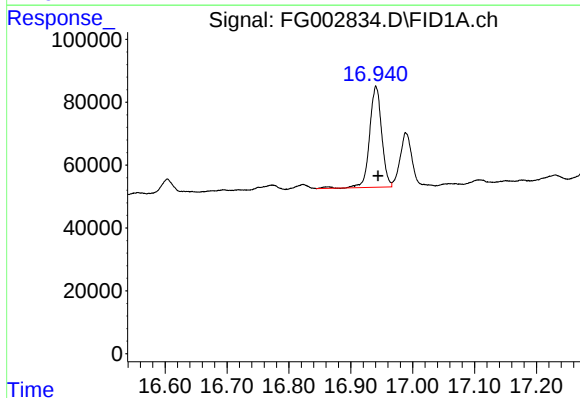


#12 N-OCTACOSANE

R.T.: 16.941 min
Delta R.T.: -0.003 min
Response: 435065
Conc: 3.58 ug/ml

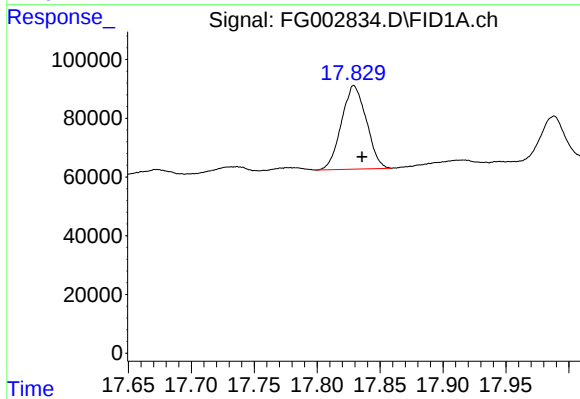


#13 N-TRIACONTANE

R.T.: 17.829 min
Delta R.T.: -0.006 min
Response: 391657
Conc: 3.26 ug/ml

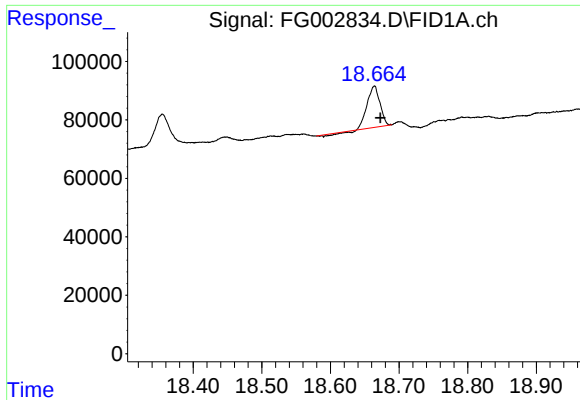


#14 N-DOTRIACONTANE

R.T.: 18.664 min
Delta R.T.: -0.009 min
Response: 172689
Conc: 1.50 ug/ml

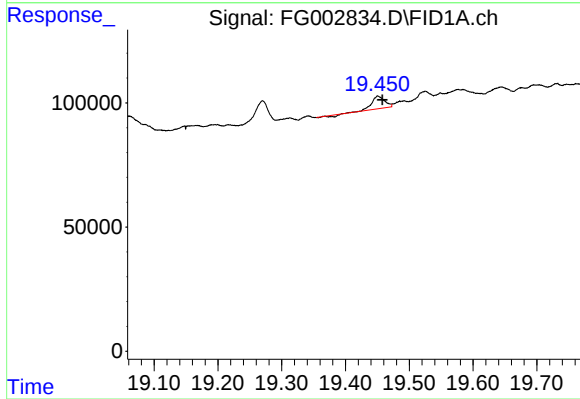

#15 N-TETRATRIACONTANE

R.T.: 19.451 min
Delta R.T.: -0.007 min
Response: 66731
Conc: 0.60 ug/ml

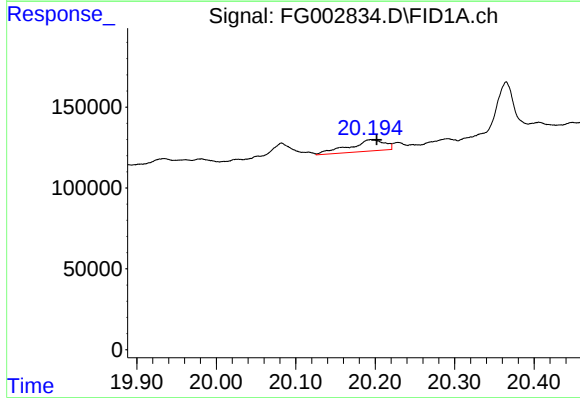

#16 N-HEXATRIACONTANE

R.T.: 20.195 min
Delta R.T.: -0.007 min
Response: 218037
Conc: 2.07 ug/ml