

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110921\
Data File : FG009019.D
Signal(s) : FID1A.ch
Acq On : 09 Nov 2021 17:21
Operator : AJ\MA
Sample : M4495-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:19:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.727	2156965	18.688 ug/ml
Target Compounds				
15)	N-TETRATRIACONTANE	19.426	66280	0.652 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110921\
Data File : FG009019.D
Signal(s) : FID1A.ch
Acq On : 09 Nov 2021 17:21
Operator : AJ\MA
Sample : M4495-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:19:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

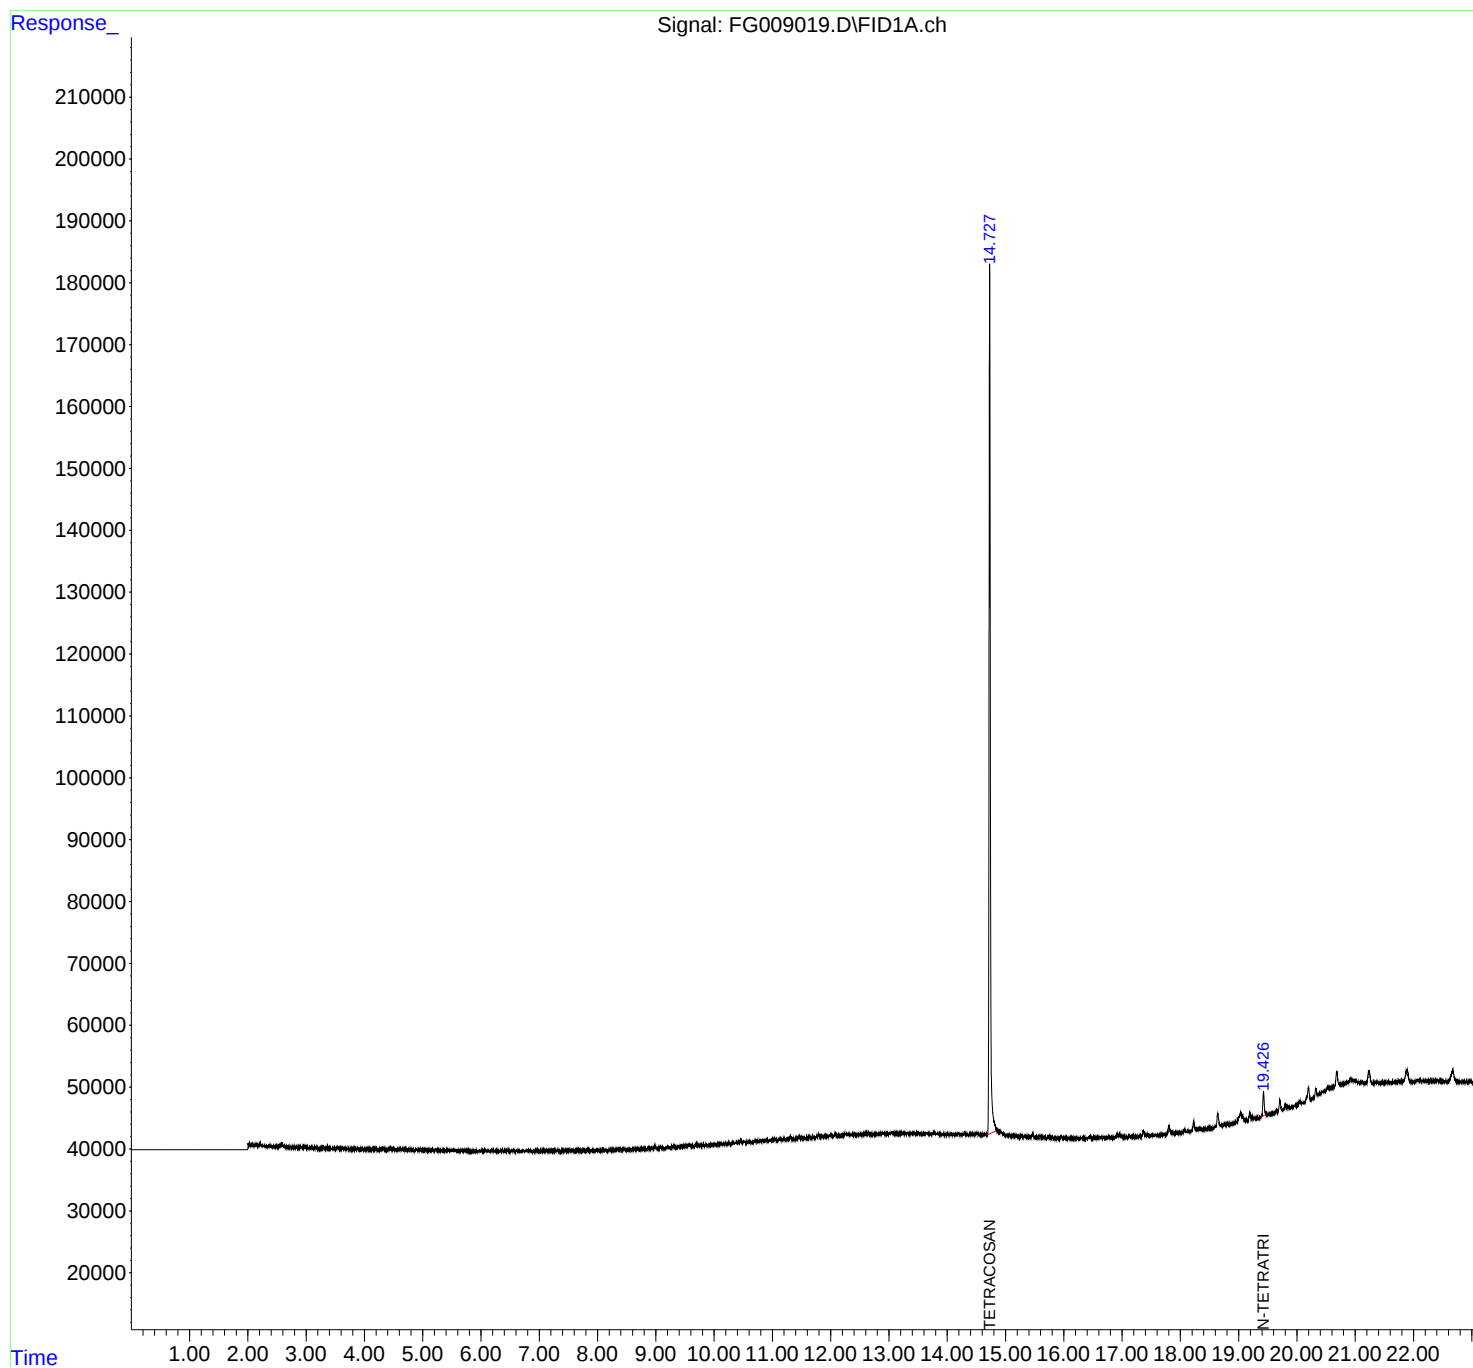


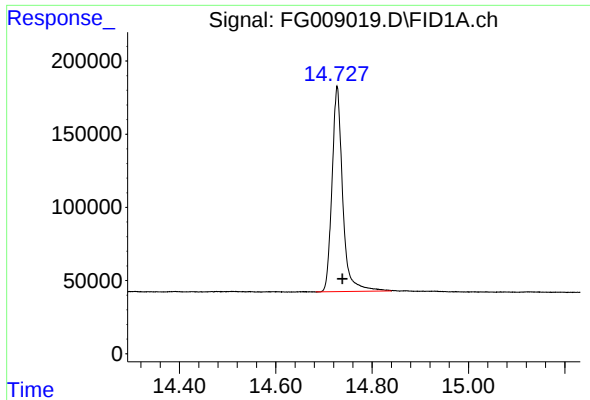

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.727 min
Delta R.T.: -0.011 min
Response: 2156965
Conc: 18.69 ug/ml

Instrument :
FID_G
ClientSampleId :

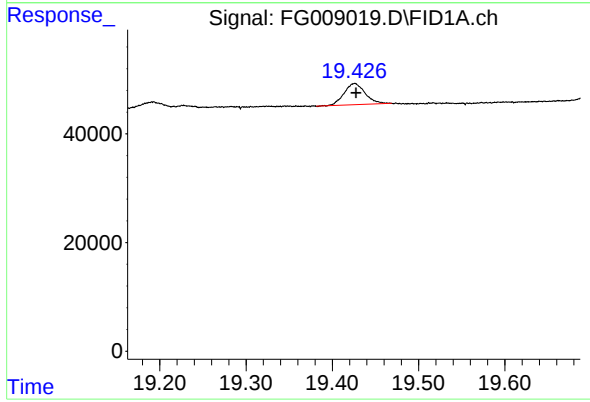

#15 N-TETRATRIACONTANE

R.T.: 19.426 min
Delta R.T.: -0.001 min
Response: 66280
Conc: 0.65 ug/ml