

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110921\
Data File : FG009027.D
Signal(s) : FID1A.ch
Acq On : 09 Nov 2021 21:28
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:21:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.726	2254100	19.530 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.803	62125	0.531 ug/ml
14) N-DOTRIACONTANE	18.638	58965	0.542 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG110921\
Data File : FG009027.D
Signal(s) : FID1A.ch
Acq On : 09 Nov 2021 21:28
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 00:21:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG110121.M
Quant Title :
QLast Update : Tue Nov 02 01:56:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

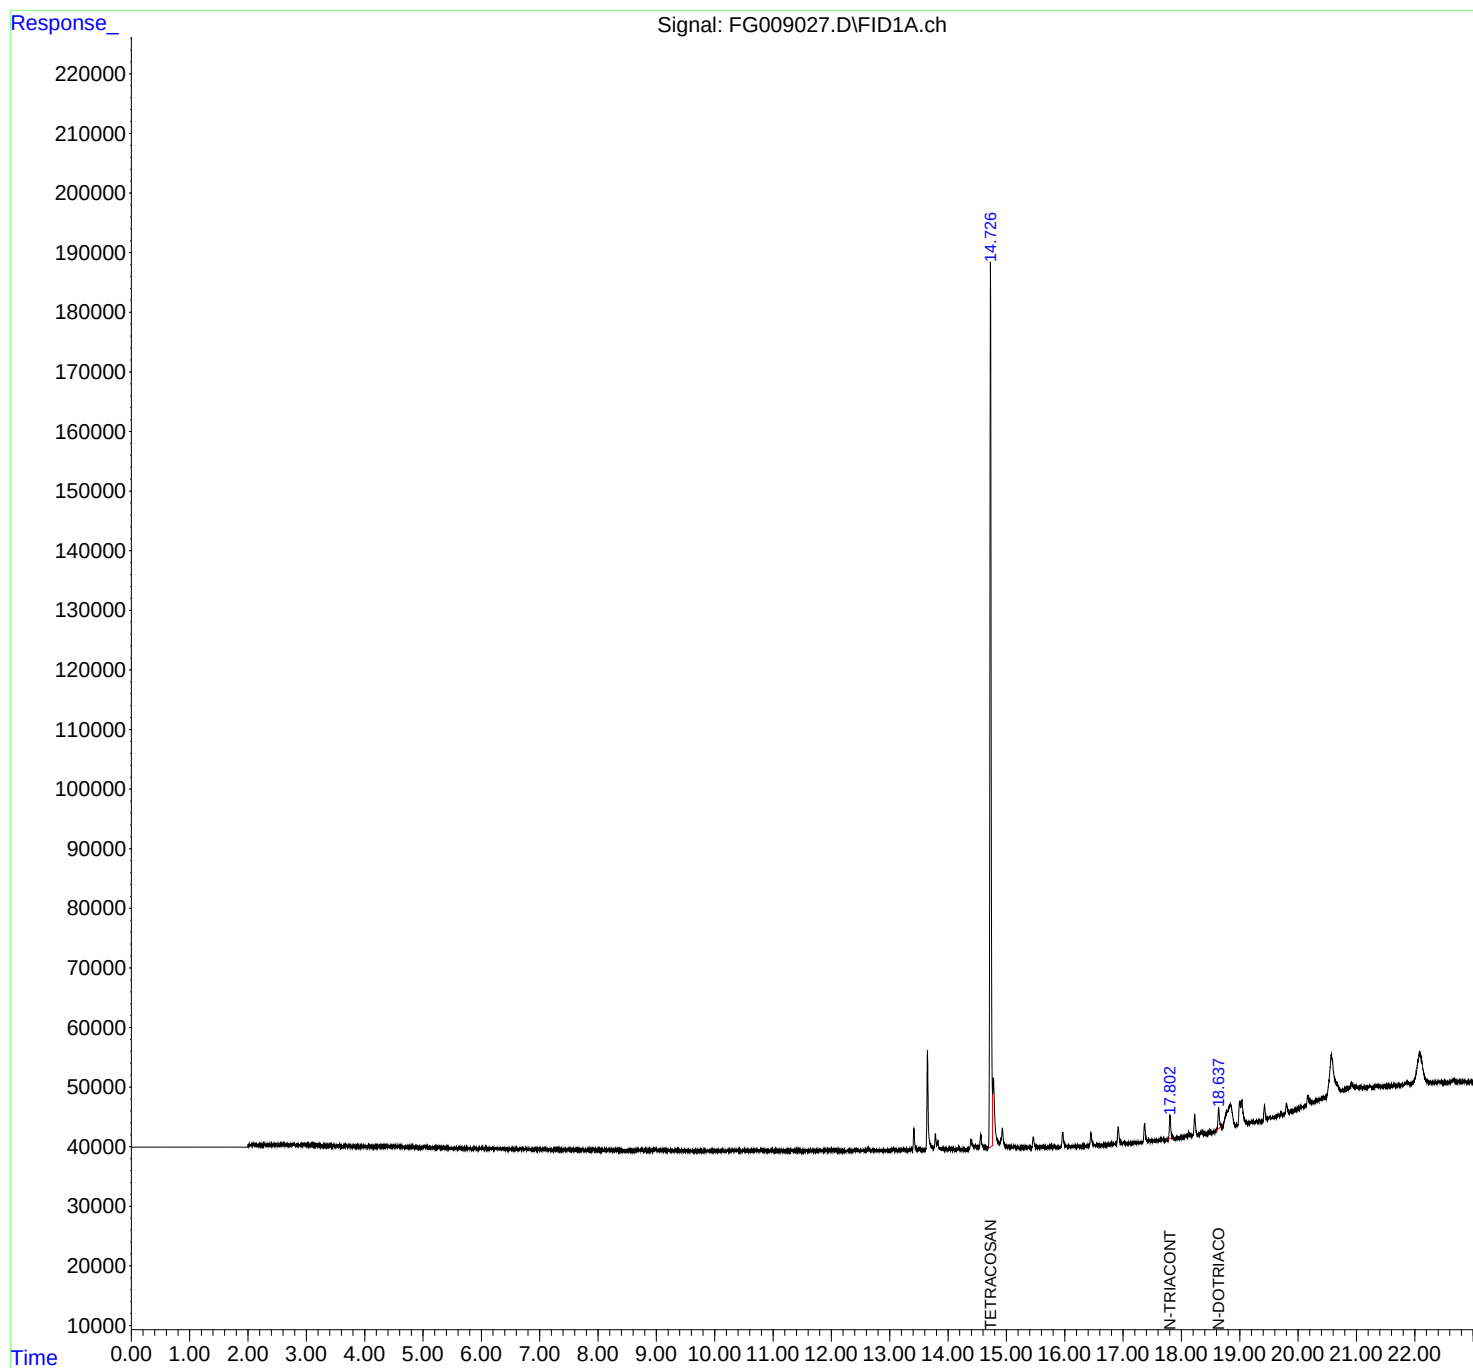


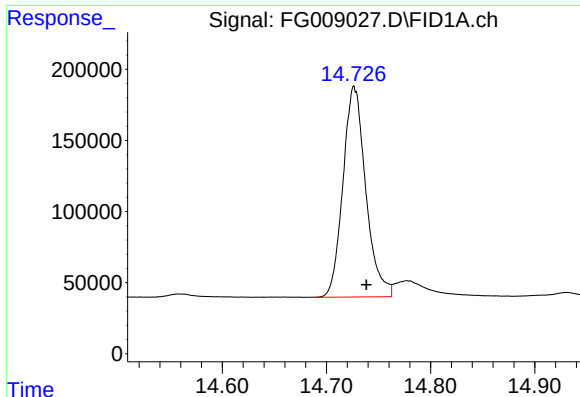

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.726 min
Delta R.T.: -0.012 min
Response: 2254100
Conc: 19.53 ug/ml

Instrument :
FID_G
ClientSampleId :

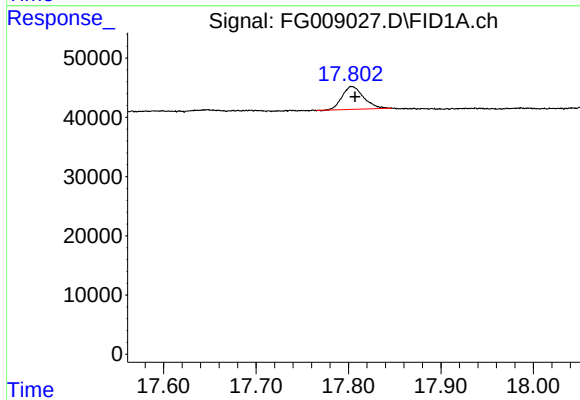

#13 N-TRIACONTANE

R.T.: 17.803 min
Delta R.T.: -0.004 min
Response: 62125
Conc: 0.53 ug/ml

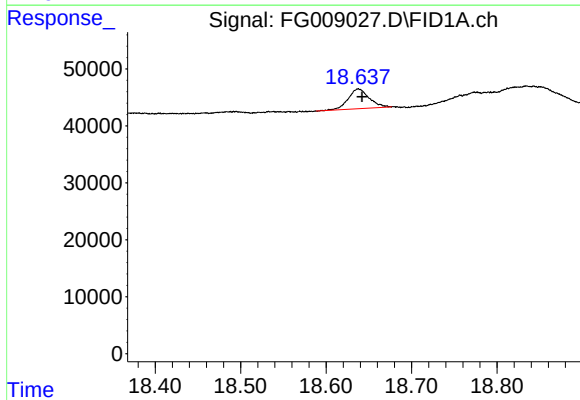

#14 N-DOTRIACONTANE

R.T.: 18.638 min
Delta R.T.: -0.004 min
Response: 58965
Conc: 0.54 ug/ml