

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111018\
 Data File : FG002854.D
 Signal(s) : FID1A.ch
 Acq On : 09 Nov 2018 13:48
 Operator : AJ\SJ
 Sample : J5269-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 09 20:40:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.761	1432693	13.036 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.356f	617732	4.672 ug/ml
8)	N-DOCOSANE	13.859	86358	0.678 ug/ml
10)	N-TETRACOSANE	14.960	99646	0.798 ug/ml
12)	N-OCTACOSANE	16.942	255549	2.101 ug/ml
13)	N-TRIACONTANE	17.831	313176	2.610 ug/ml
14)	N-DOTRIACONTANE	18.665	226962	1.969 ug/ml
15)	N-TETRATRIACONTANE	19.454	100921	0.908 ug/ml
16)	N-HEXATRIACONTANE	20.204	138911	1.319 ug/ml
17)	N-OCTATRIACONTANE	20.955	6581	0.069 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111018\
Data File : FG002854.D
Signal(s) : FID1A.ch
Acq On : 09 Nov 2018 13:48
Operator : AJ\SJ
Sample : J5269-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 20:40:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

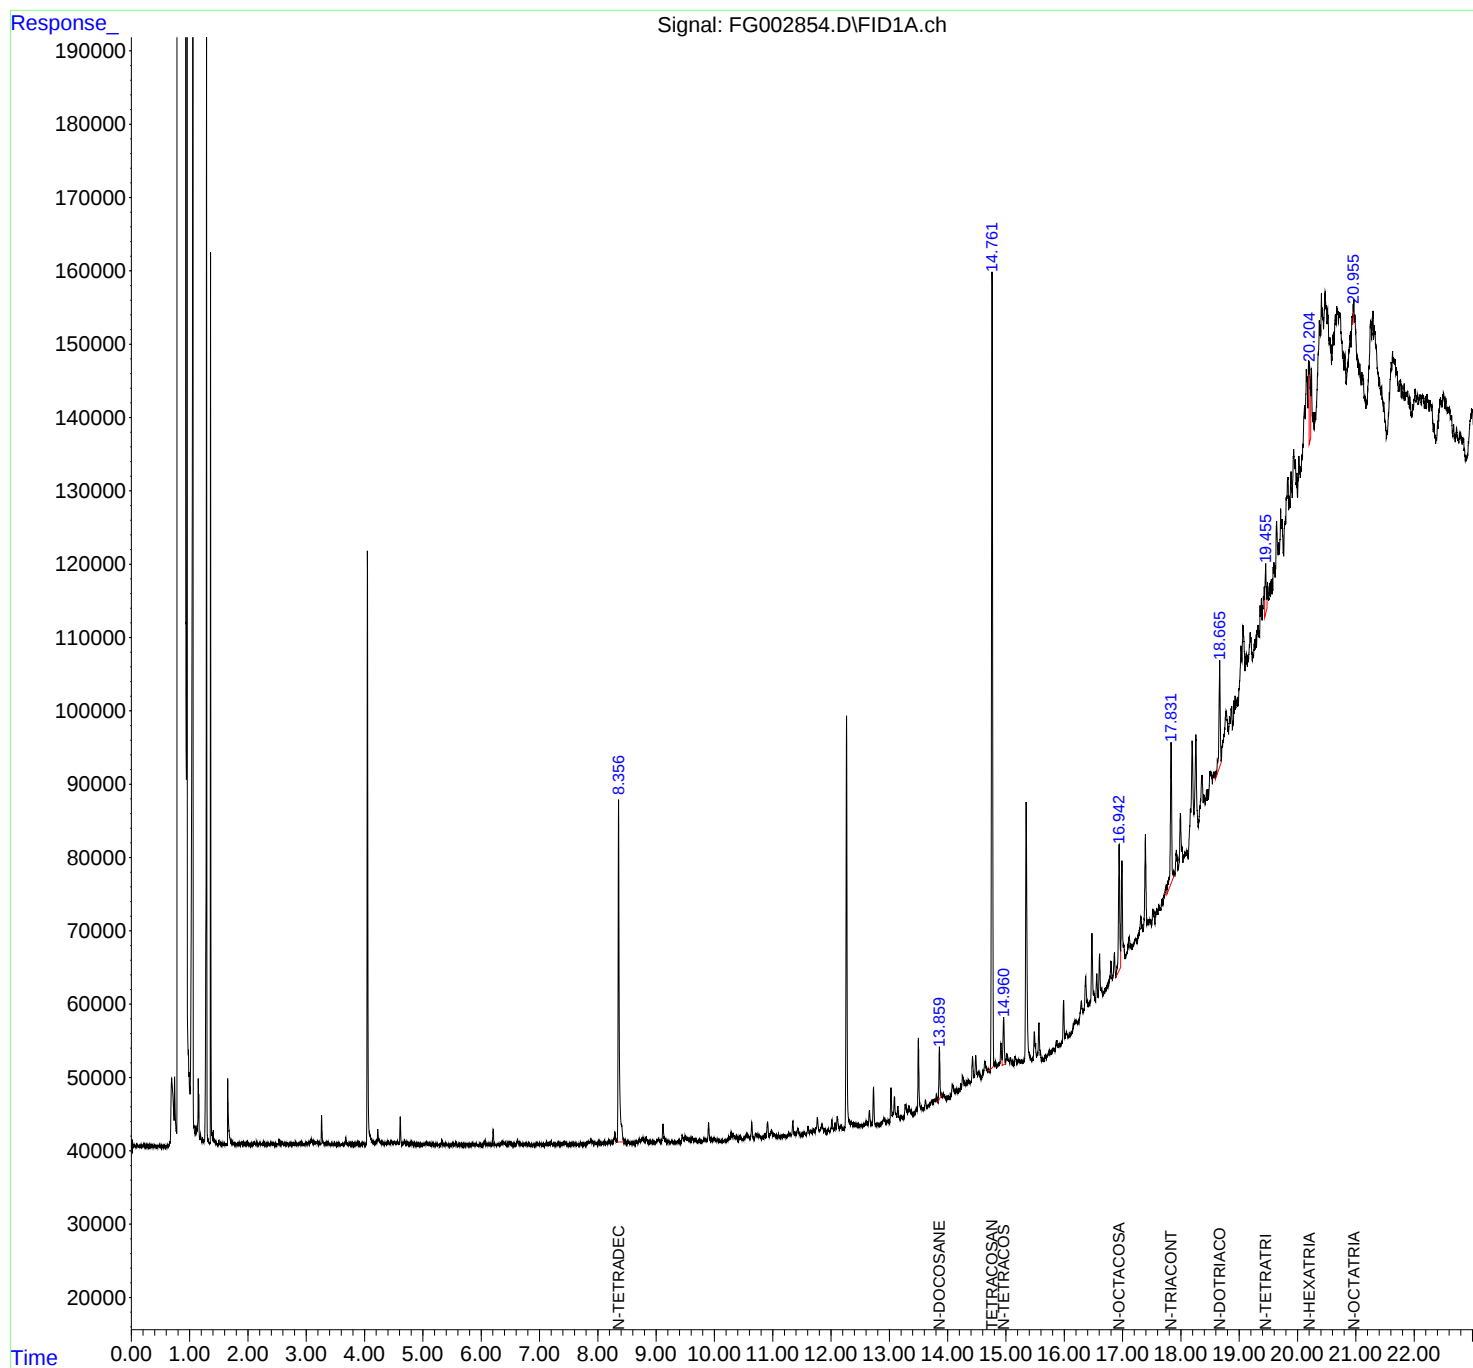

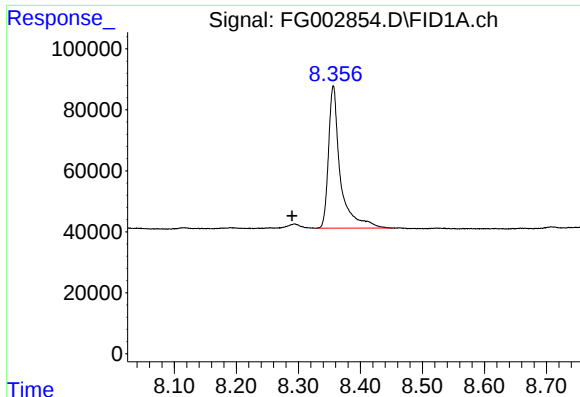


#4 N-TETRADECANE

R.T.: 8.356 min
Delta R.T.: 0.067 min
Response: 617732
Conc: 4.67 ug/ml

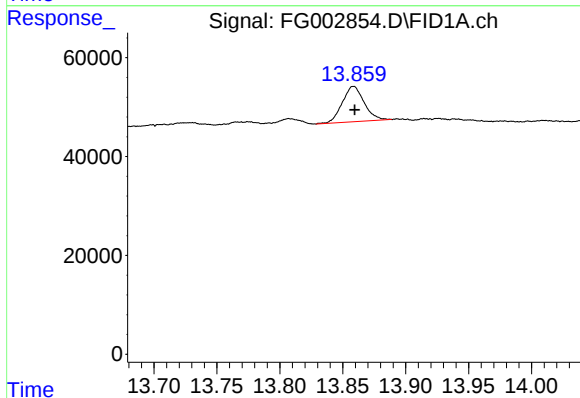


#8 N-DOCOSANE

R.T.: 13.859 min
Delta R.T.: 0.000 min
Response: 86358
Conc: 0.68 ug/ml

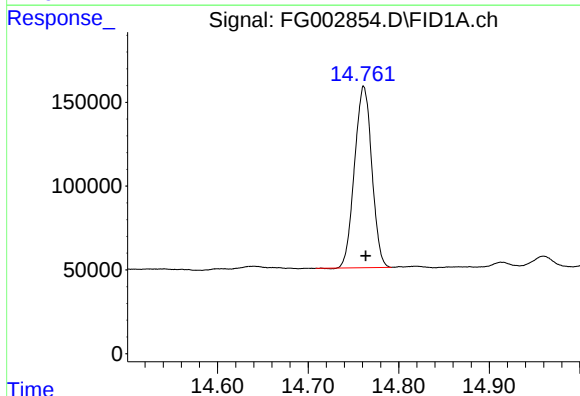


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.761 min
Delta R.T.: -0.002 min
Response: 1432693
Conc: 13.04 ug/ml

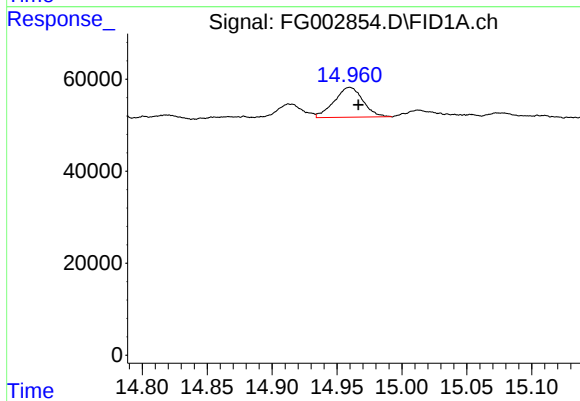


#10 N-TETRACOSANE

R.T.: 14.960 min
Delta R.T.: -0.007 min
Response: 99646
Conc: 0.80 ug/ml

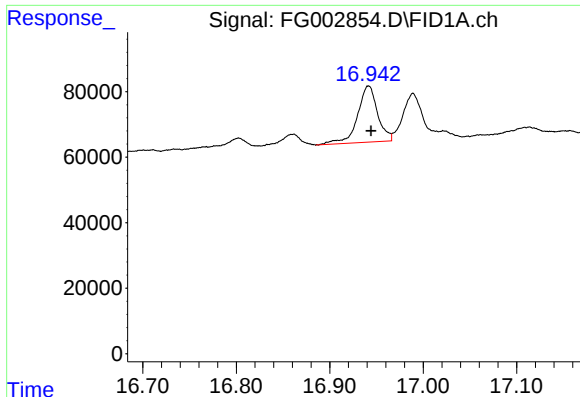


#12 N-OCTACOSANE

R.T.: 16.942 min
Delta R.T.: -0.002 min
Response: 255549
Conc: 2.10 ug/ml

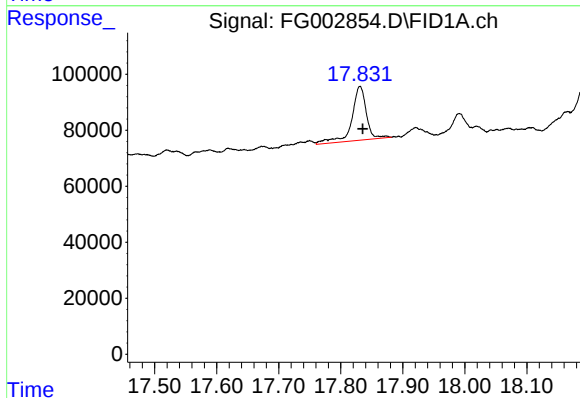


#13 N-TRIACONTANE

R.T.: 17.831 min
Delta R.T.: -0.005 min
Response: 313176
Conc: 2.61 ug/ml

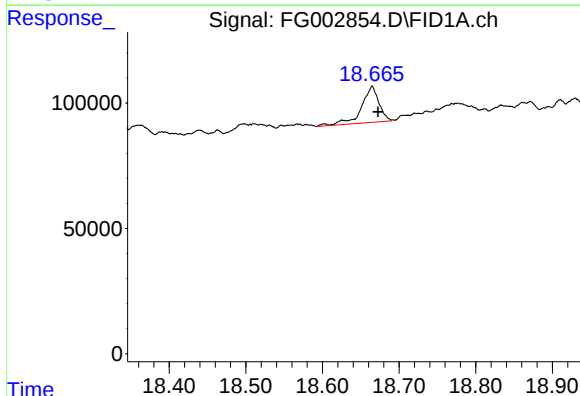


#14 N-DOTRIACONTANE

R.T.: 18.665 min
Delta R.T.: -0.008 min
Response: 226962
Conc: 1.97 ug/ml

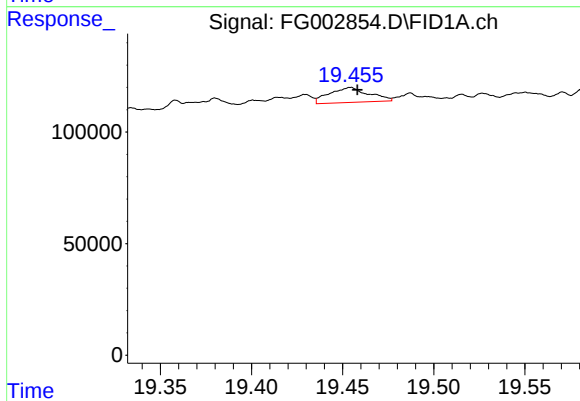


#15 N-TETRATRIACONTANE

R.T.: 19.454 min
Delta R.T.: -0.004 min
Response: 100921
Conc: 0.91 ug/ml

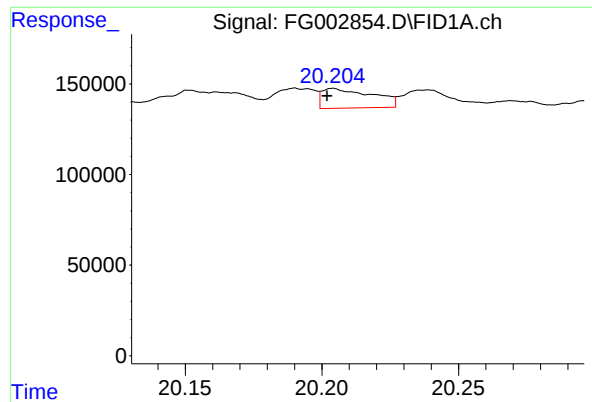

#16 N-HEXATRIACONTANE

R.T.: 20.204 min
Delta R.T.: 0.002 min
Response: 138911
Conc: 1.32 ug/ml

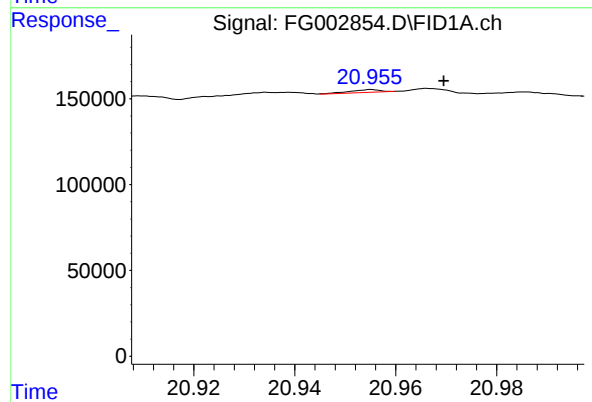

#17 N-OCTATRIACONTANE

R.T.: 20.955 min
Delta R.T.: -0.014 min
Response: 6581
Conc: 0.07 ug/ml