

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111018\
 Data File : FG002857.D
 Signal(s) : FID1A.ch
 Acq On : 09 Nov 2018 15:18
 Operator : AJ\SJ
 Sample : J5269-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 09 20:41:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.762	1617888	14.721 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.255	105756	0.800 ug/ml
5)	N-HEXADECANE	9.918	186065	1.397 ug/ml
8)	N-DOCOSANE	13.860	79816	0.627 ug/ml
10)	N-TETRACOSANE	14.955	356385	2.853 ug/ml
11)	N-HEXACOSANE	15.988	214828	1.743 ug/ml
12)	N-OCTACOSANE	16.941	591523	4.863 ug/ml
13)	N-TRIACONTANE	17.830	464472	3.871 ug/ml
14)	N-DOTRIACONTANE	18.666	258920	2.246 ug/ml
15)	N-TETRATRIACONTANE	19.452	73298	0.659 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111018\
Data File : FG002857.D
Signal(s) : FID1A.ch
Acq On : 09 Nov 2018 15:18
Operator : AJ\SJ
Sample : J5269-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 20:41:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

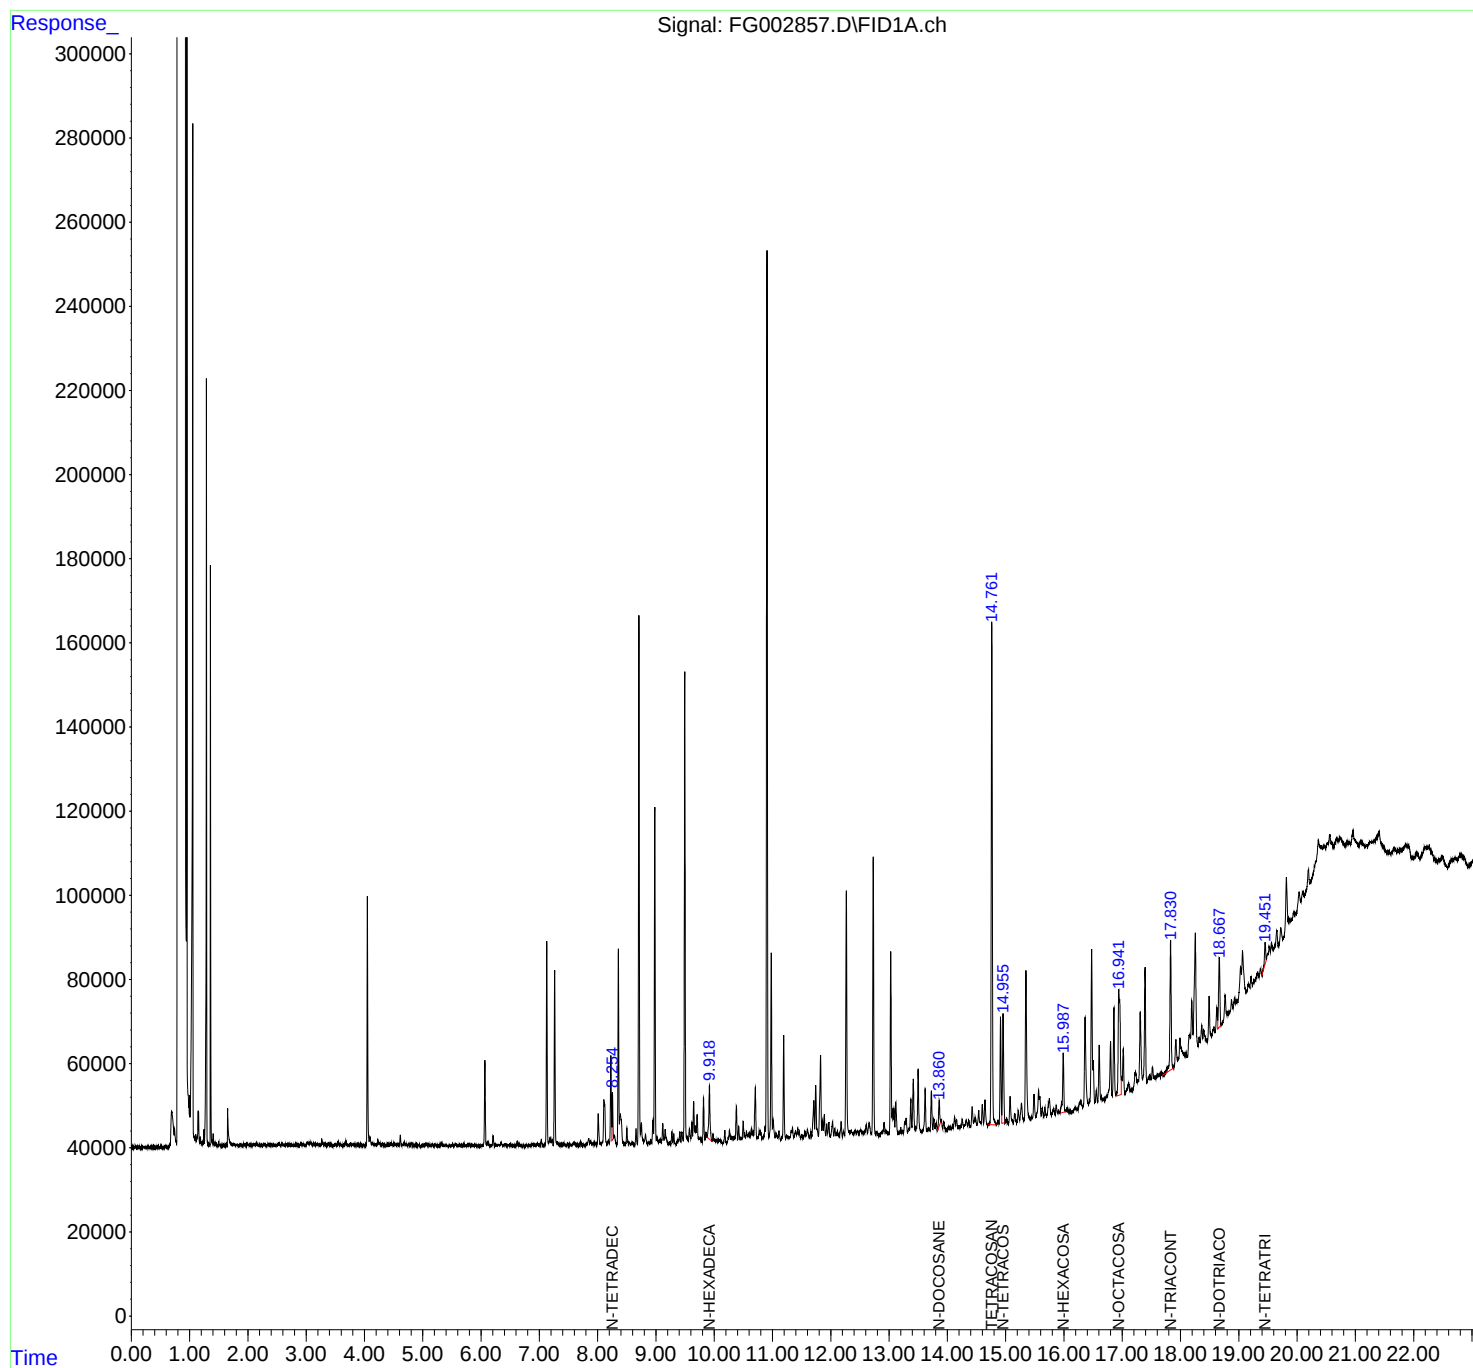

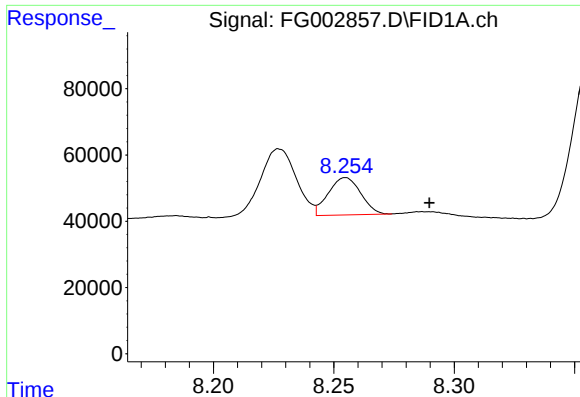


#4 N-TETRADECANE

R.T.: 8.255 min
Delta R.T.: -0.035 min
Response: 105756
Conc: 0.80 ug/ml

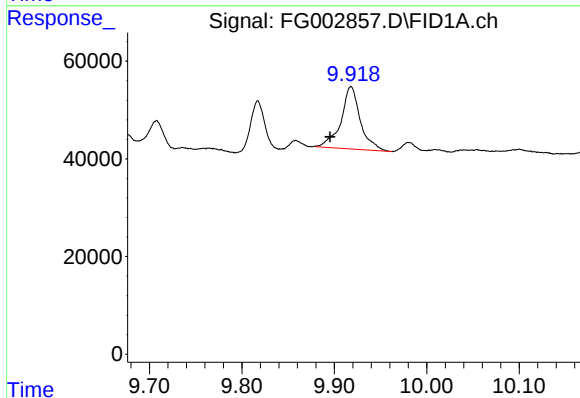


#5 N-HEXADECANE

R.T.: 9.918 min
Delta R.T.: 0.023 min
Response: 186065
Conc: 1.40 ug/ml

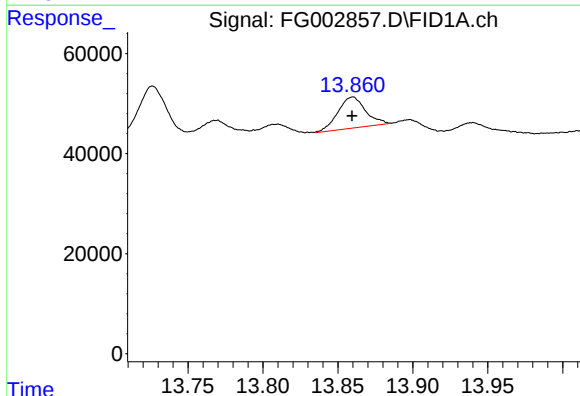


#8 N-DOCOSANE

R.T.: 13.860 min
Delta R.T.: 0.000 min
Response: 79816
Conc: 0.63 ug/ml

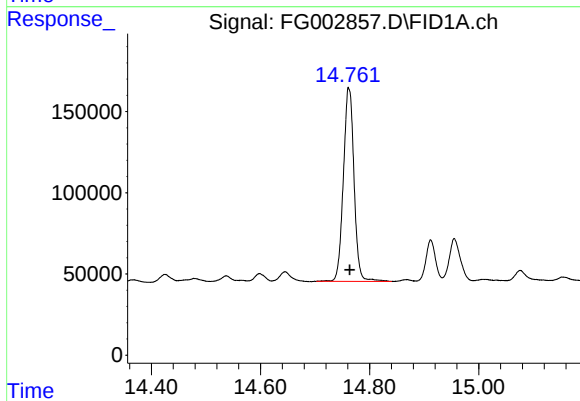


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.762 min
Delta R.T.: -0.002 min
Response: 1617888
Conc: 14.72 ug/ml

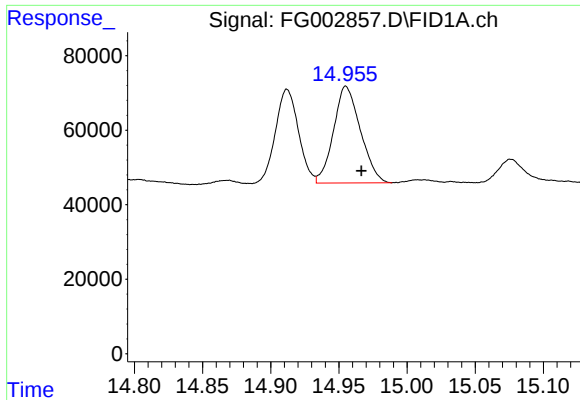


#10 N-TETRACOSANE

R.T.: 14.955 min
Delta R.T.: -0.011 min
Response: 356385
Conc: 2.85 ug/ml

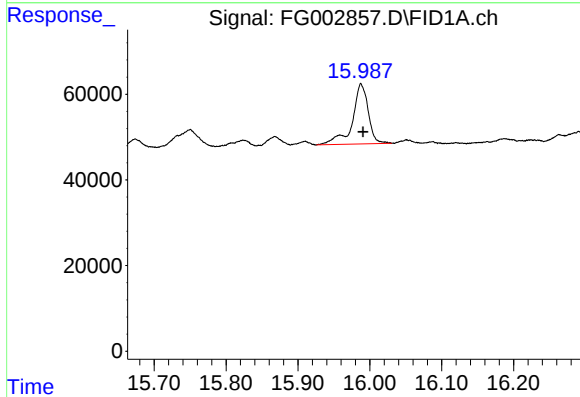


#11 N-HEXACOSANE

R.T.: 15.988 min
Delta R.T.: -0.003 min
Response: 214828
Conc: 1.74 ug/ml

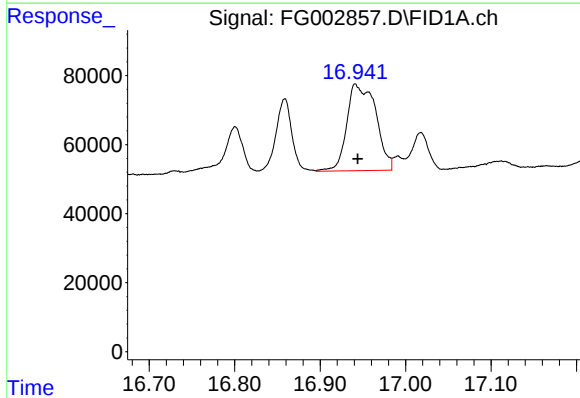


#12 N-OCTACOSANE

R.T.: 16.941 min
Delta R.T.: -0.003 min
Response: 591523
Conc: 4.86 ug/ml

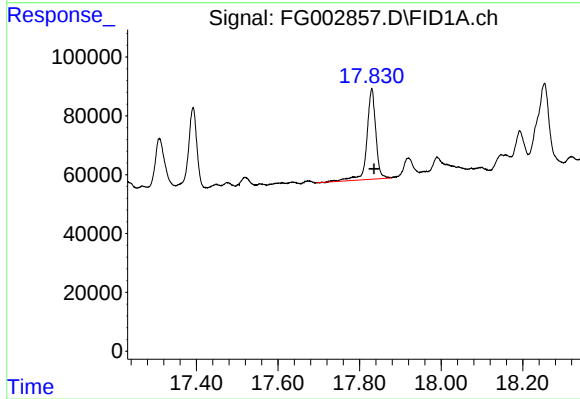


#13 N-TRIACONTANE

R.T.: 17.830 min
Delta R.T.: -0.005 min
Response: 464472
Conc: 3.87 ug/ml

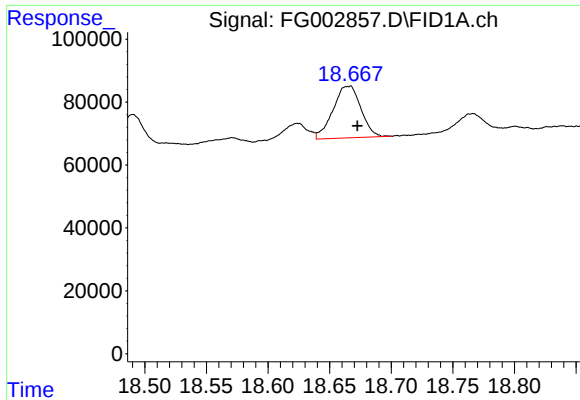

#14 N-DOTRIACONTANE

R.T.: 18.666 min
Delta R.T.: -0.007 min
Response: 258920
Conc: 2.25 ug/ml

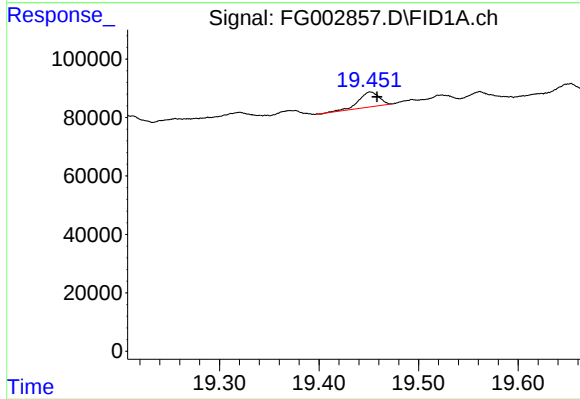

#15 N-TETRATRIACONTANE

R.T.: 19.452 min
Delta R.T.: -0.007 min
Response: 73298
Conc: 0.66 ug/ml