

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111018\
 Data File : FG002863.D
 Signal(s) : FID1A.ch
 Acq On : 09 Nov 2018 18:20
 Operator : AJ\SJ
 Sample : J5884-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 09 20:42:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
 Quant Title :
 QLast Update : Sat Oct 27 02:13:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.761	1997690	18.177 ug/ml
Target Compounds			
4) N-TETRADECANE	8.356f	767405	5.804 ug/ml
7) N-EICOSANE	12.664	229990	1.774 ug/ml
8) N-DOCOSANE	13.858	139742	1.098 ug/ml
10) N-TETRACOSANE	14.963	278092	2.226 ug/ml
11) N-HEXACOSANE	15.988	413978	3.359 ug/ml
12) N-OCTACOSANE	16.941	1118370	9.195 ug/ml
13) N-TRIACONTANE	17.831	896593	7.472 ug/ml
14) N-DOTRIACONTANE	18.662	626941	5.438 ug/ml
15) N-TETRATRIACONTANE	19.448	220771	1.985 ug/ml
16) N-HEXATRIACONTANE	20.194	110336	1.048 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111018\
Data File : FG002863.D
Signal(s) : FID1A.ch
Acq On : 09 Nov 2018 18:20
Operator : AJ\SJ
Sample : J5884-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 20:42:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

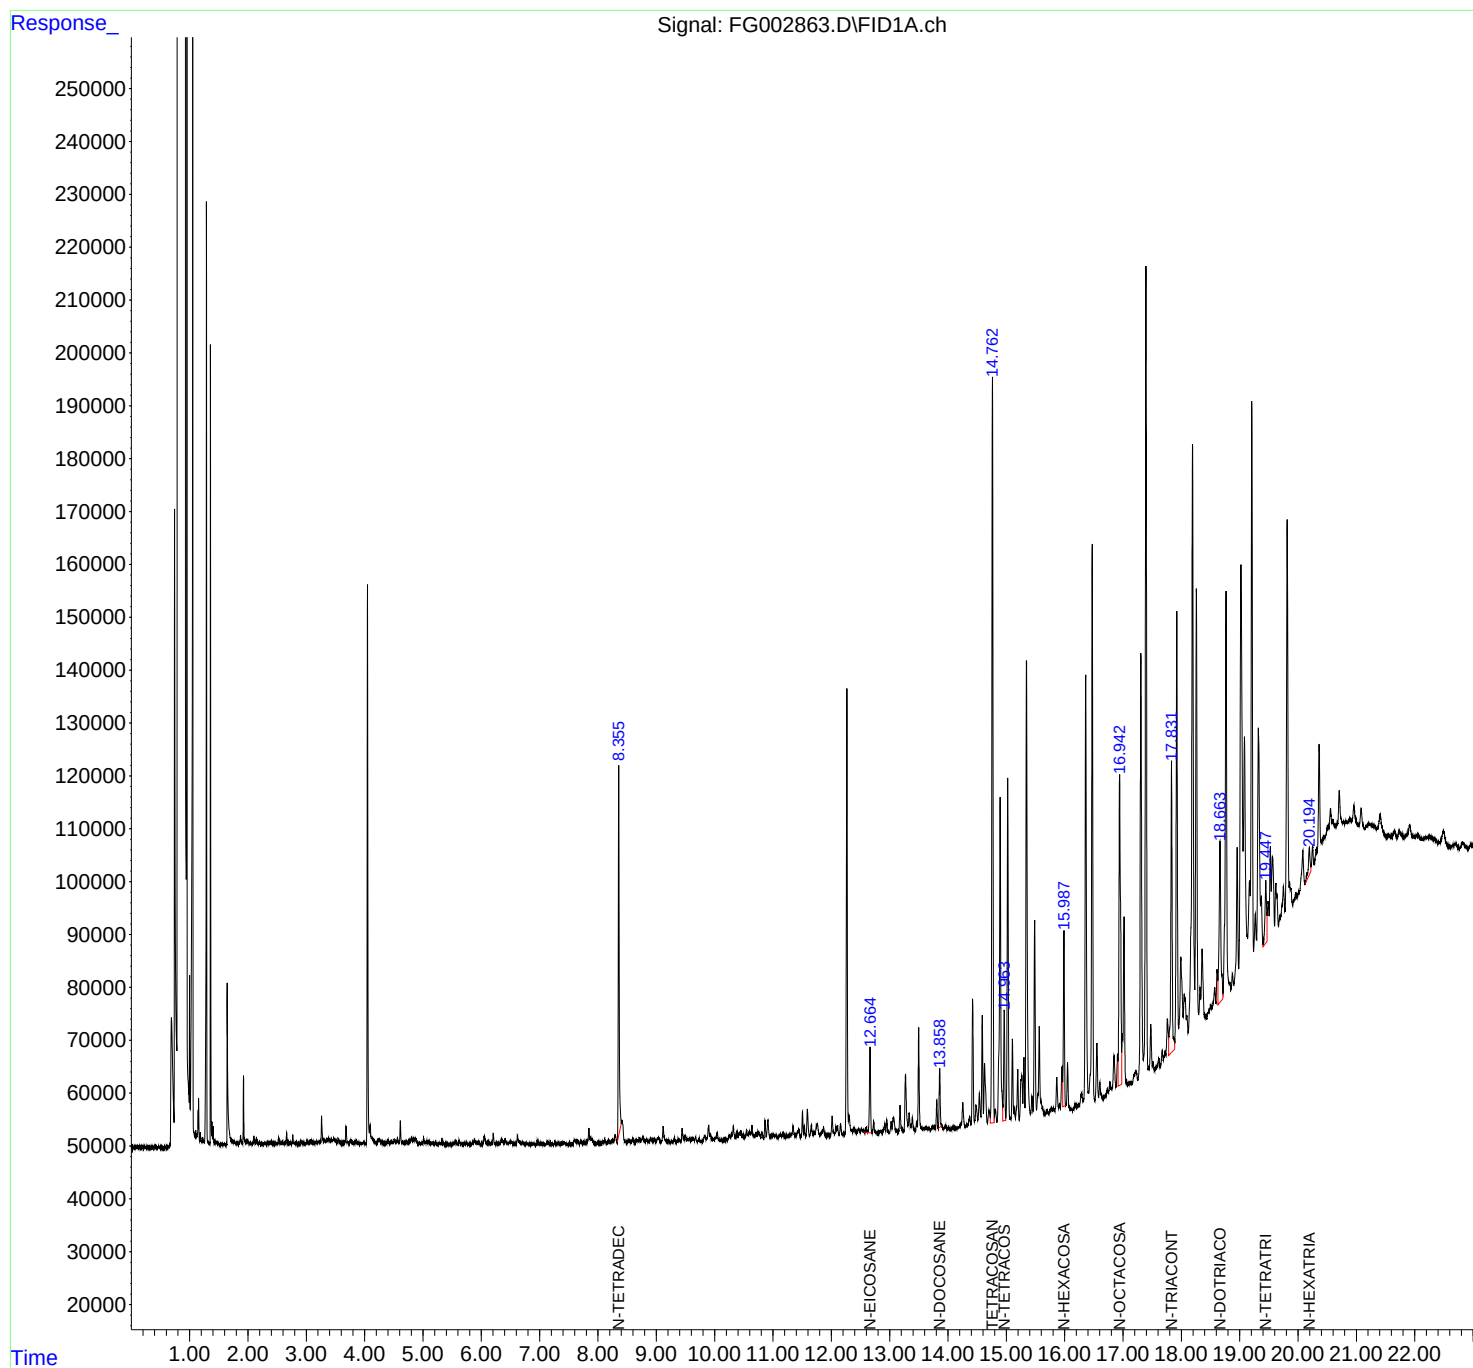

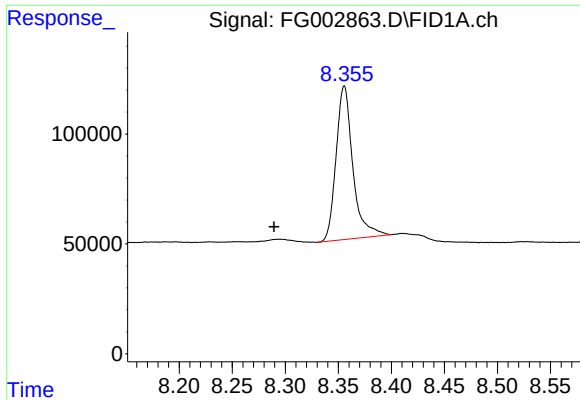


#4 N-TETRADECANE

R.T.: 8.356 min
Delta R.T.: 0.066 min
Response: 767405
Conc: 5.80 ug/ml

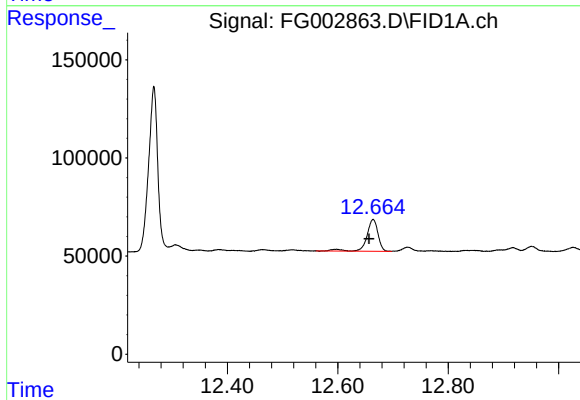


#7 N-EICOSANE

R.T.: 12.664 min
Delta R.T.: 0.008 min
Response: 229990
Conc: 1.77 ug/ml

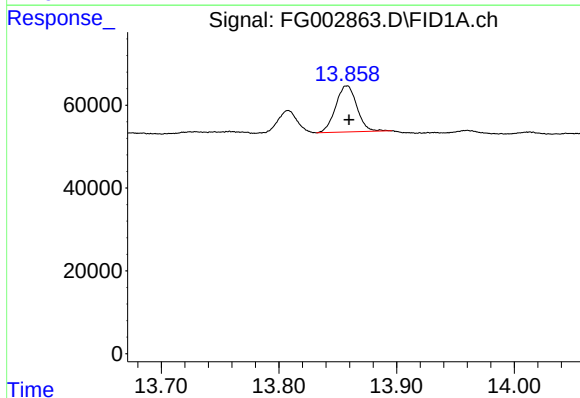


#8 N-DOCOSANE

R.T.: 13.858 min
Delta R.T.: -0.002 min
Response: 139742
Conc: 1.10 ug/ml

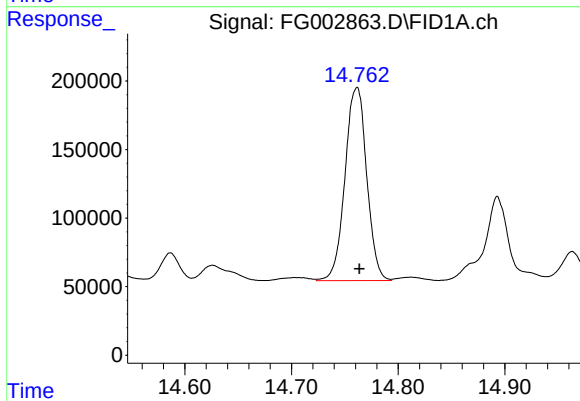


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.761 min
Delta R.T.: -0.002 min
Response: 1997690
Conc: 18.18 ug/ml

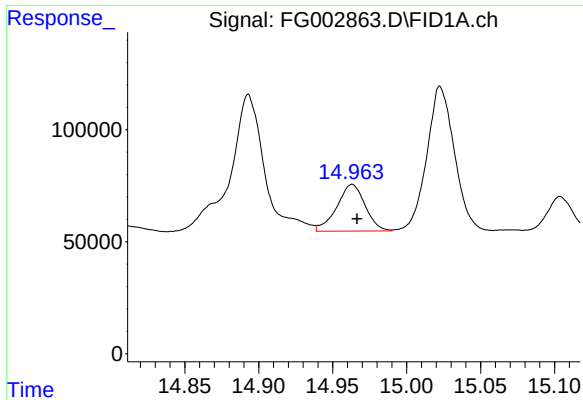


#10 N-TETRACOSANE

R.T.: 14.963 min
Delta R.T.: -0.003 min
Response: 278092
Conc: 2.23 ug/ml

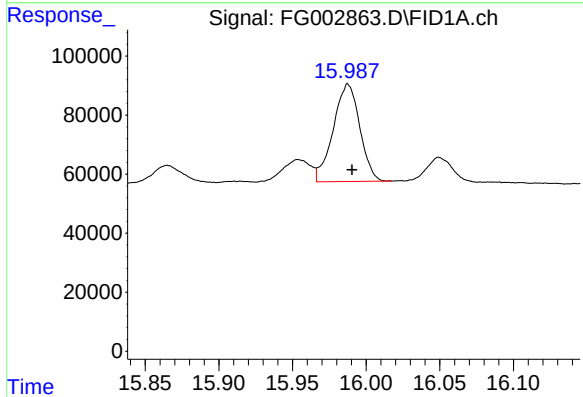


#11 N-HEXACOSANE

R.T.: 15.988 min
Delta R.T.: -0.003 min
Response: 413978
Conc: 3.36 ug/ml

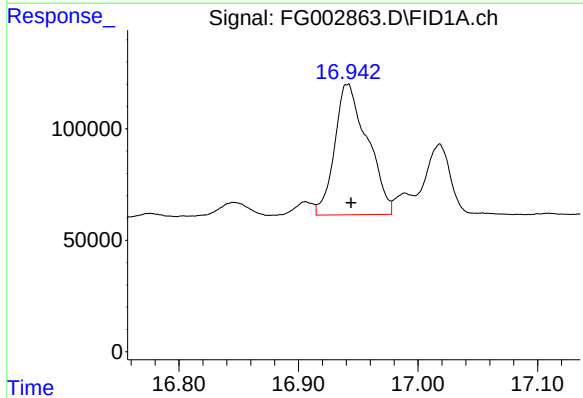


#12 N-OCTACOSANE

R.T.: 16.941 min
Delta R.T.: -0.003 min
Response: 1118370
Conc: 9.20 ug/ml

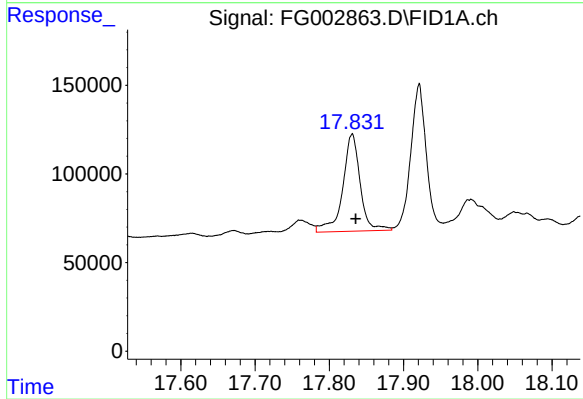


#13 N-TRIACONTANE

R.T.: 17.831 min
Delta R.T.: -0.005 min
Response: 896593
Conc: 7.47 ug/ml

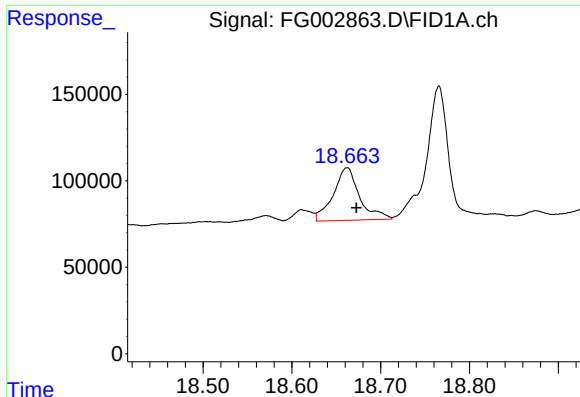


#14 N-DOTRIACONTANE

R.T.: 18.662 min
Delta R.T.: -0.010 min
Response: 626941
Conc: 5.44 ug/ml

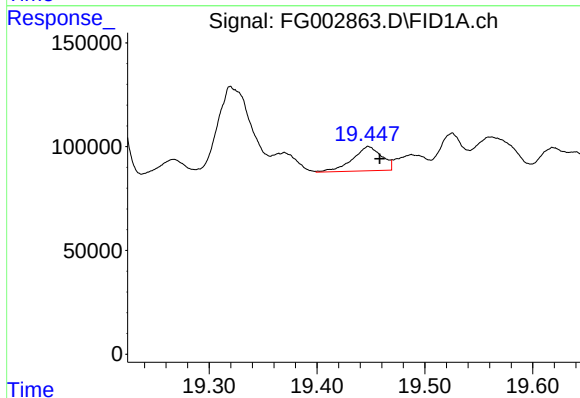

#15 N-TETRATRIACONTANE

R.T.: 19.448 min
Delta R.T.: -0.010 min
Response: 220771
Conc: 1.99 ug/ml

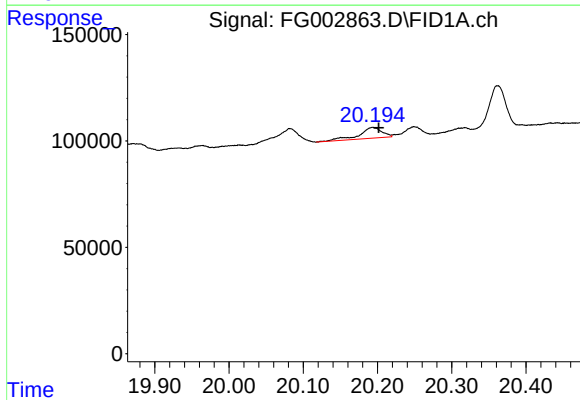

#16 N-HEXATRIACONTANE

R.T.: 20.194 min
Delta R.T.: -0.008 min
Response: 110336
Conc: 1.05 ug/ml