

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111118\
Data File : FG002876.D
Signal(s) : FID1A.ch
Acq On : 10 Nov 2018 01:39
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 10 10:20:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
Quant Title :
QLast Update : Wed Nov 07 10:34:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.755	2054544	16.718 ug/ml
Target Compounds				
12)	N-DOTRIACONTANE	18.658	255990	2.980 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111118\
Data File : FG002876.D
Signal(s) : FID1A.ch
Acq On : 10 Nov 2018 01:39
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 10 10:20:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\C44-FG110618.M
Quant Title :
QLast Update : Wed Nov 07 10:34:24 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

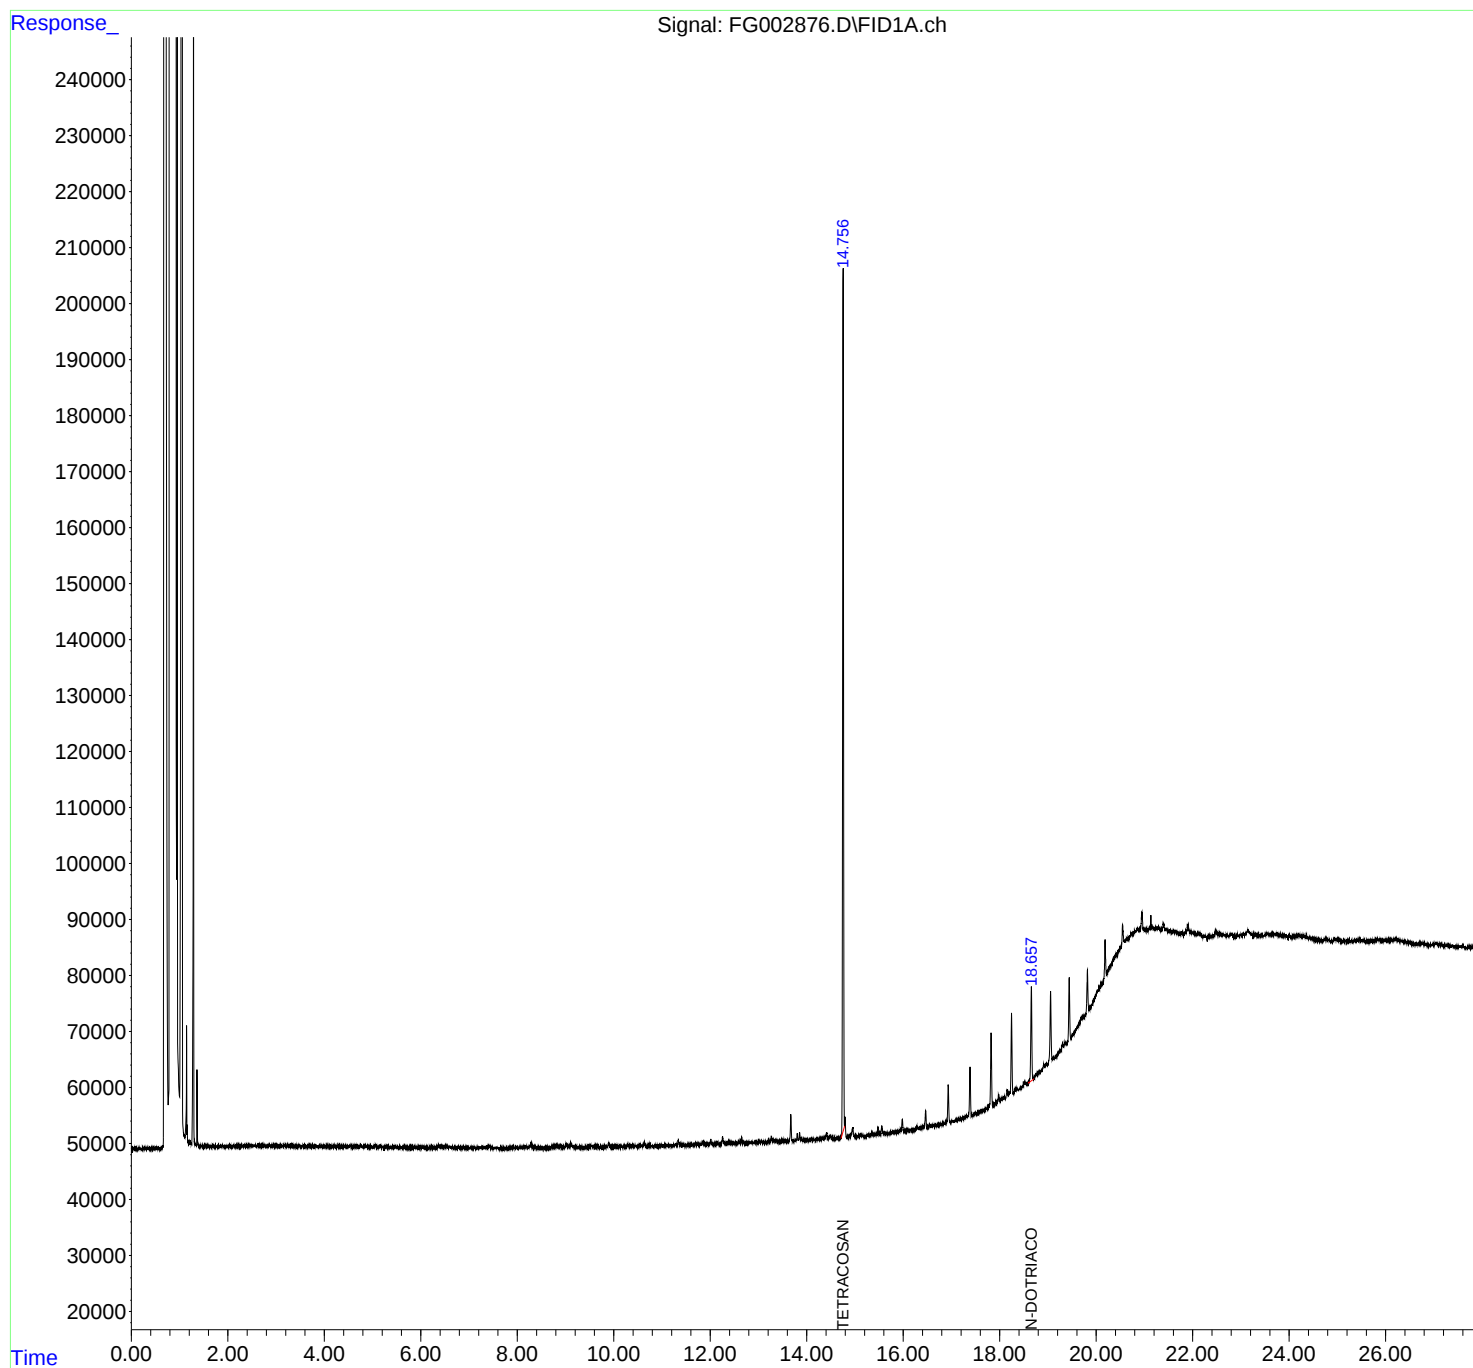

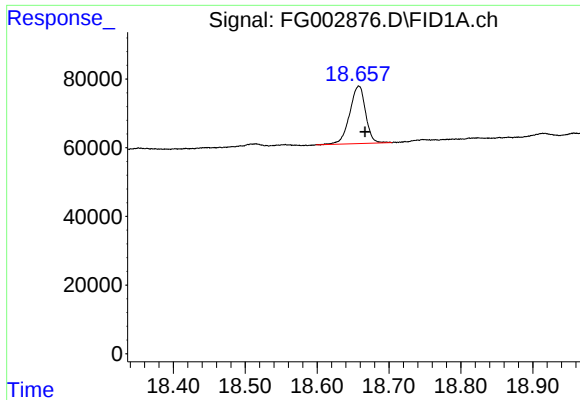

#12 N-DOTRIACONTANE

R.T.: 18.658 min
Delta R.T.: -0.009 min
Response: 255990
Conc: 2.98 ug/ml

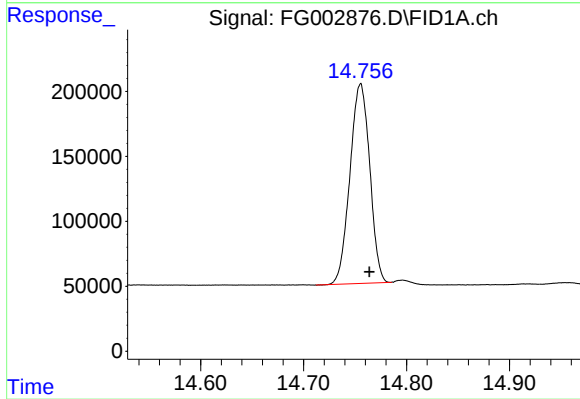

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.755 min
Delta R.T.: -0.009 min
Response: 2054544
Conc: 16.72 ug/ml