

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111218\
Data File : FG002904.D
Signal(s) : FID1A.ch
Acq On : 13 Nov 2018 01:15
Operator : AJ\SJ
Sample : J5887-13 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 13 03:18:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.753	128567	1.170 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.826	241306	2.011 ug/ml
14) N-DOTRIACONTANE	18.659	170811	1.482 ug/ml
15) N-TETRATRIACONTANE	19.443	137688	1.238 ug/ml
16) N-HEXATRIACONTANE	20.191	142056	1.349 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG111218\
Data File : FG002904.D
Signal(s) : FID1A.ch
Acq On : 13 Nov 2018 01:15
Operator : AJ\SJ
Sample : J5887-13 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 13 03:18:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG102618.M
Quant Title :
QLast Update : Sat Oct 27 02:13:37 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

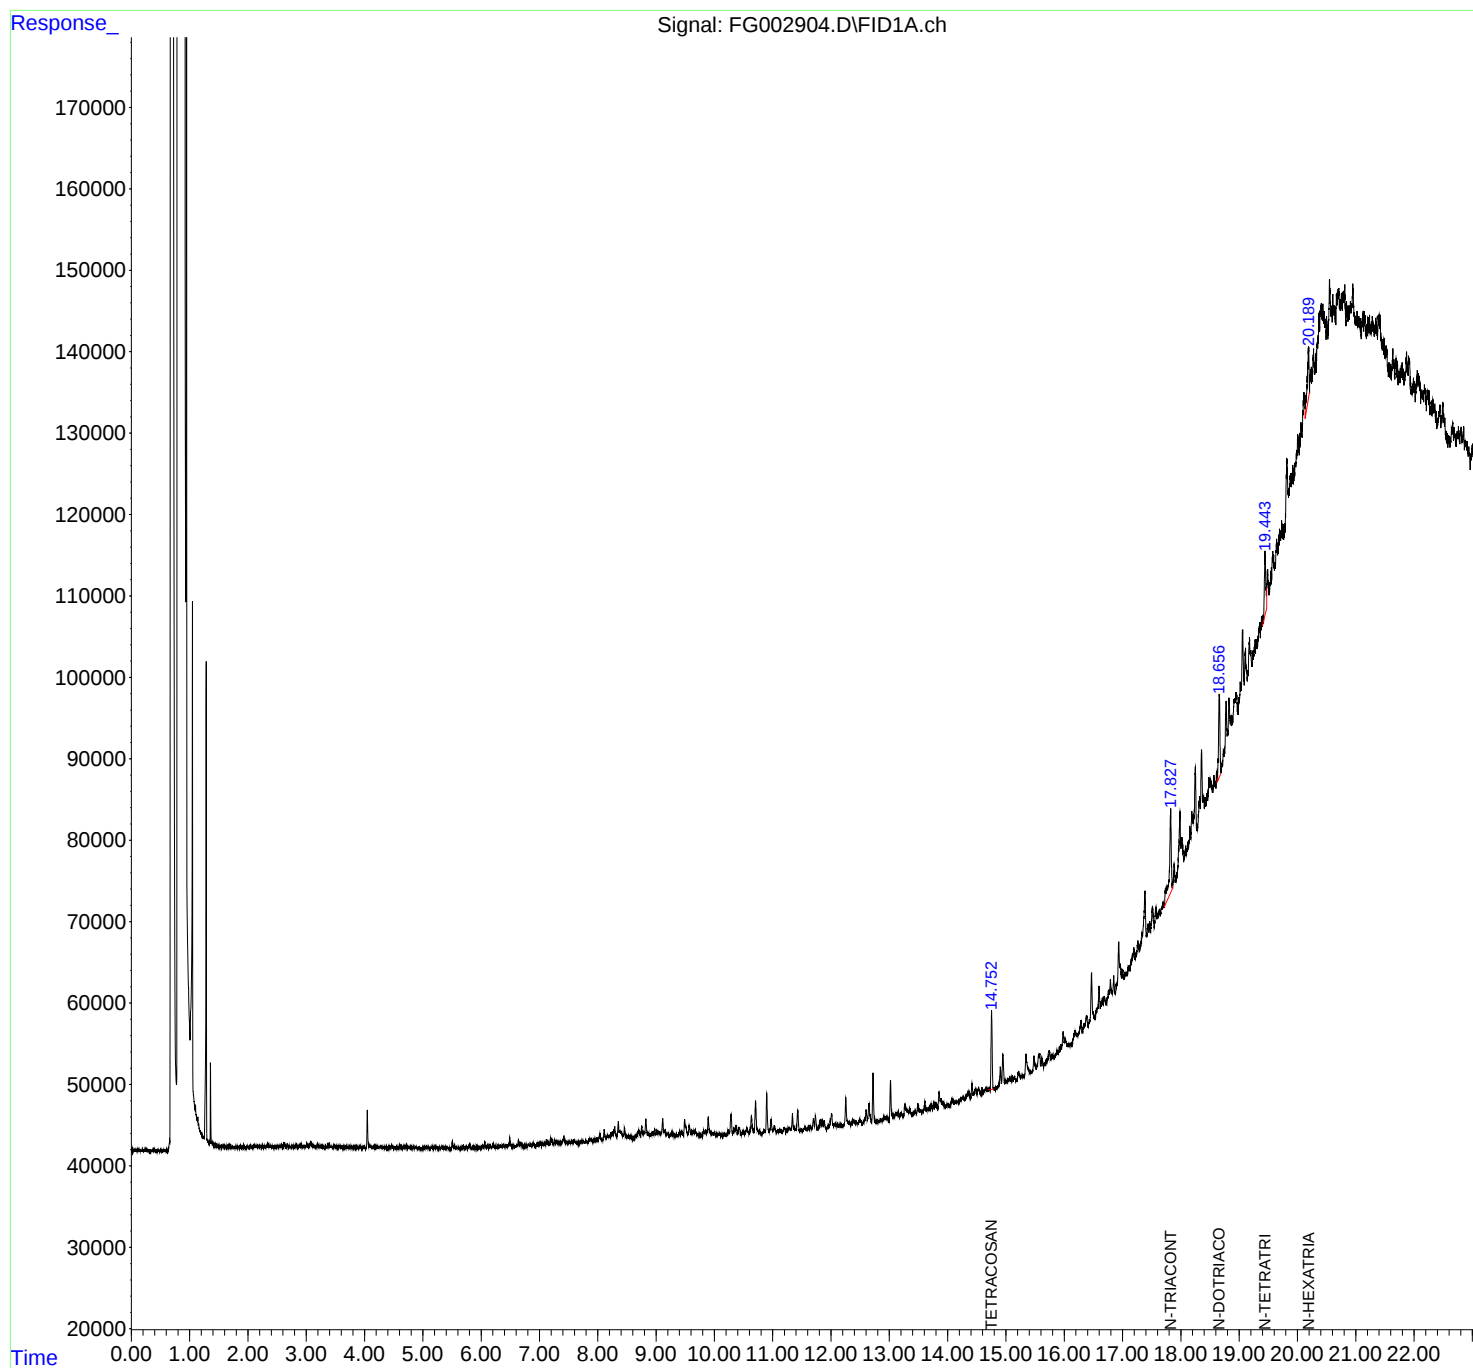

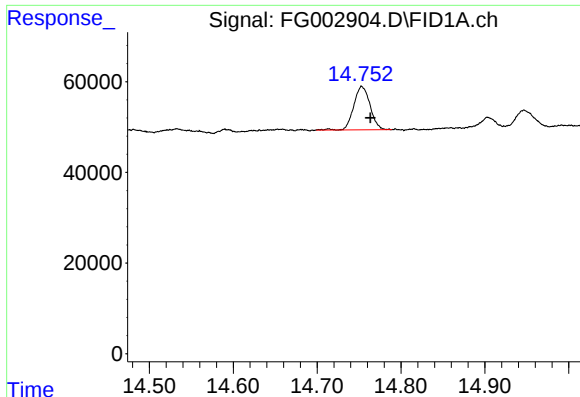


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.753 min
Delta R.T.: -0.010 min
Response: 128567
Conc: 1.17 ug/ml

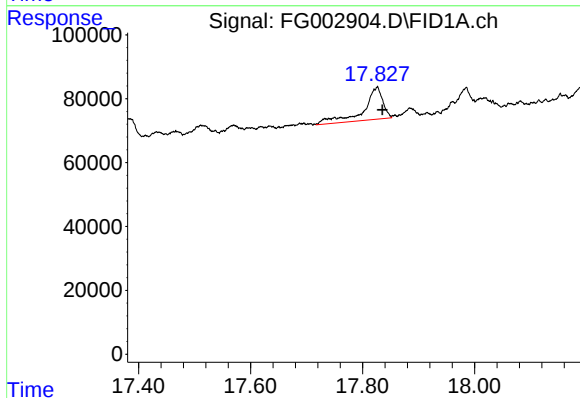


#13 N-TRIACONTANE

R.T.: 17.826 min
Delta R.T.: -0.009 min
Response: 241306
Conc: 2.01 ug/ml

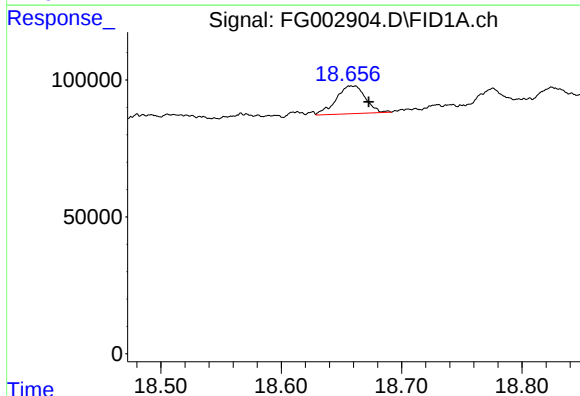


#14 N-DOTRIACONTANE

R.T.: 18.659 min
Delta R.T.: -0.014 min
Response: 170811
Conc: 1.48 ug/ml

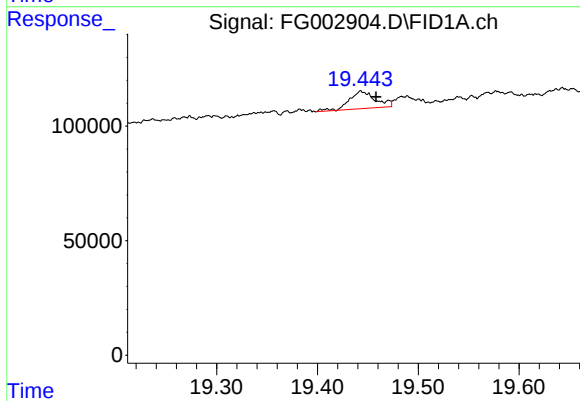

#15 N-TETRATRIACONTANE

R.T.: 19.443 min
Delta R.T.: -0.015 min
Response: 137688
Conc: 1.24 ug/ml

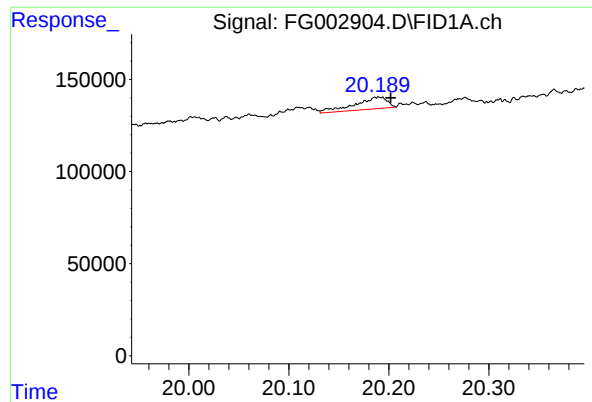

#16 N-HEXATRIACONTANE

R.T.: 20.191 min
Delta R.T.: -0.011 min
Response: 142056
Conc: 1.35 ug/ml